

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006965.D\VWD1A.CH Vial: 4
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006965.D\VWD1A.CH
 Acq On : 02-Nov-2014, 04:41 Operator: TP
 Sample : PB79747BS Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Nov 2 6:16 2014 Quant Results File: HN1029NG.RES

Instrument :
 HPLC_N
 ClientSampleId :
 PB79747BS

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1029NG.M
 Title :
 Last Update : Fri Oct 31 04:41:35 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	1447713	0.393 ng/ul
Target Compounds			
2) T Nitroglycerin	6.04	2413184	0.313 ng/ul

 Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____ Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006965.D HN1029NG.M Sat Nov 08 04:55:41 2014



Quantitation Report


Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006965.D\VWD1A.CH Vial: 4
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006965.D\VWD1A.CH
 Acq On : 02-Nov-2014, 04:41 Operator: TP
 Sample : PB79747BS Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Nov 2 6:16 2014 Quant Results File: HN1029NG.RES

Instrument :
 HPLC_N
 ClientSampleId :
 PB79747BS

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1029NG.M
 Title :
 Last Update : Fri Oct 31 04:41:35 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

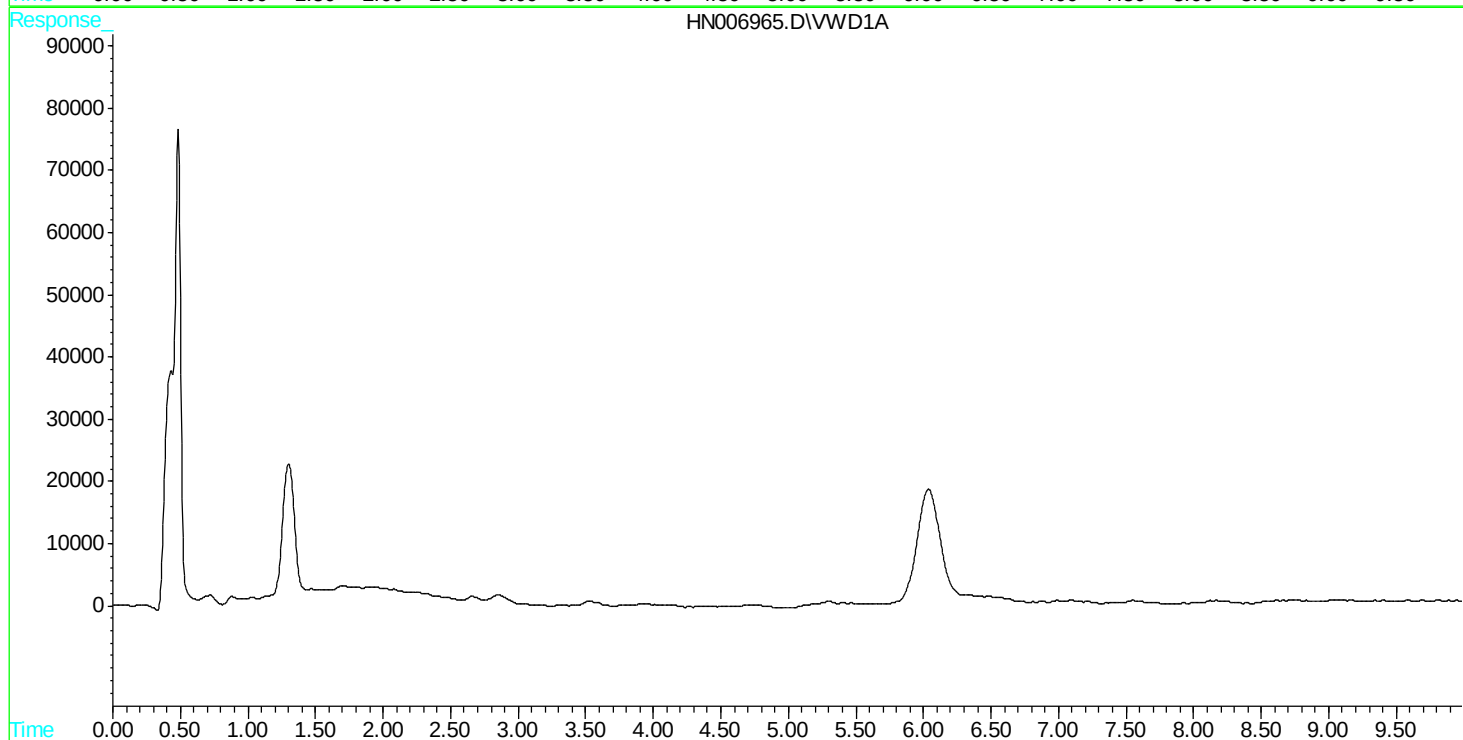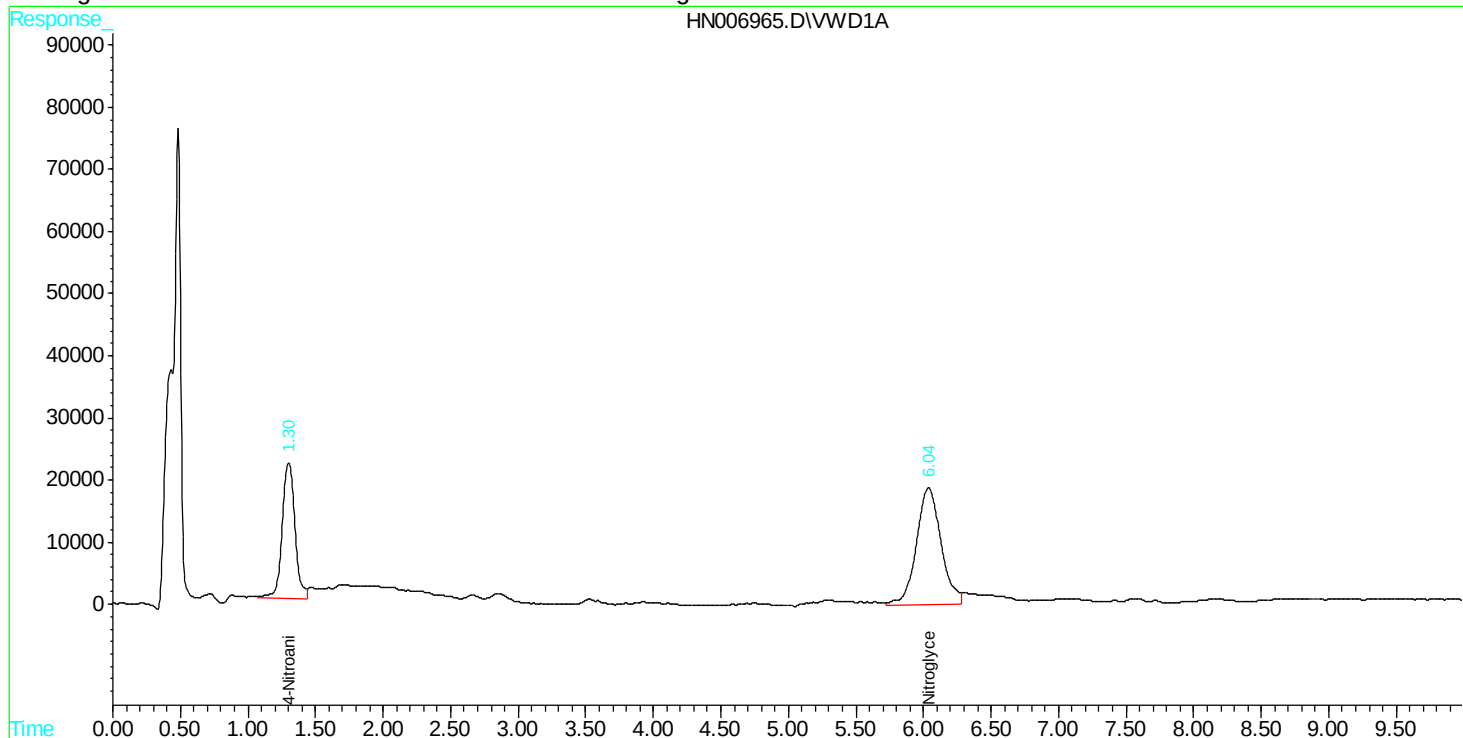


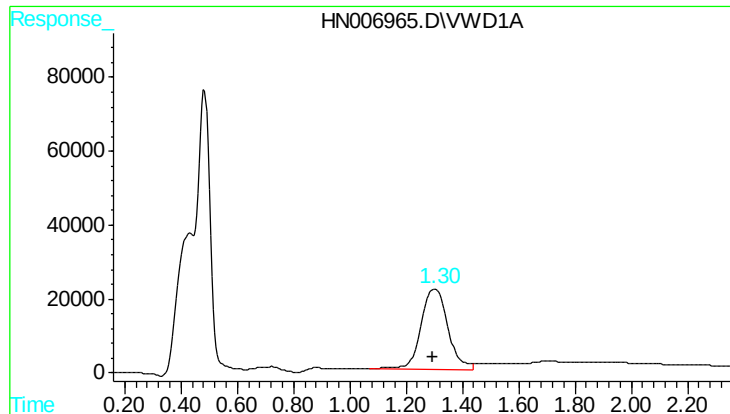

#1 4-Nitroaniline

R.T.: 1.302 min
Delta R.T.: 0.006 min
Response: 1447713
Conc: 0.39 ng/ul

Instrument :
HPLC_N
ClientSampleId :
PB79747BS

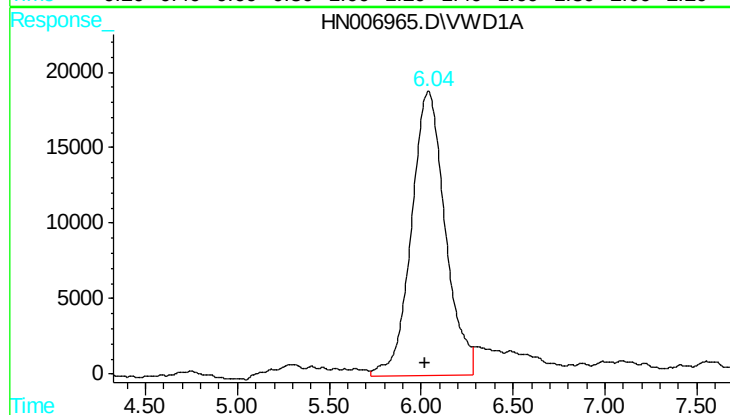

#2 Nitroglycerin

R.T.: 6.039 min
Delta R.T.: 0.018 min
Response: 2413184
Conc: 0.31 ng/ul