

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN110614\
 Data File : HN007065.D
 Signal(s) : VWD1A.CH
 Acq On : 06-Nov-2014, 21:17
 Operator : TP
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDCCC0500

Integration File: autoint1.e
 Quant Time: Mar 11 04:28:14 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Quant Title :
 QLast Update : Sat Mar 07 03:03:02 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.299	1509451	432.471 ug/L
Target Compounds			
2) T HMX	0.871	1900915	451.254 ug/L
3) T RDX	1.685	2623183	518.702 ug/L
4) T 1,3,5-Trinitrobenzene	2.655	5239095	514.255 ug/L
5) T 1,3-Dinitrobenzene	3.519f	8147562	510.722 ng/ml
6) T 3,5-Dinitroaniline	3.899f	5812563	517.564 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN110614\
Data File : HN007065.D
Signal(s) : VWD1A.CH
Acq On : 06-Nov-2014, 21:17
Operator : TP
Sample : HSTDCCC0500
Misc :
ALS Vial : 81 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

Integration File: autoint1.e
Quant Time: Mar 11 04:28:14 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

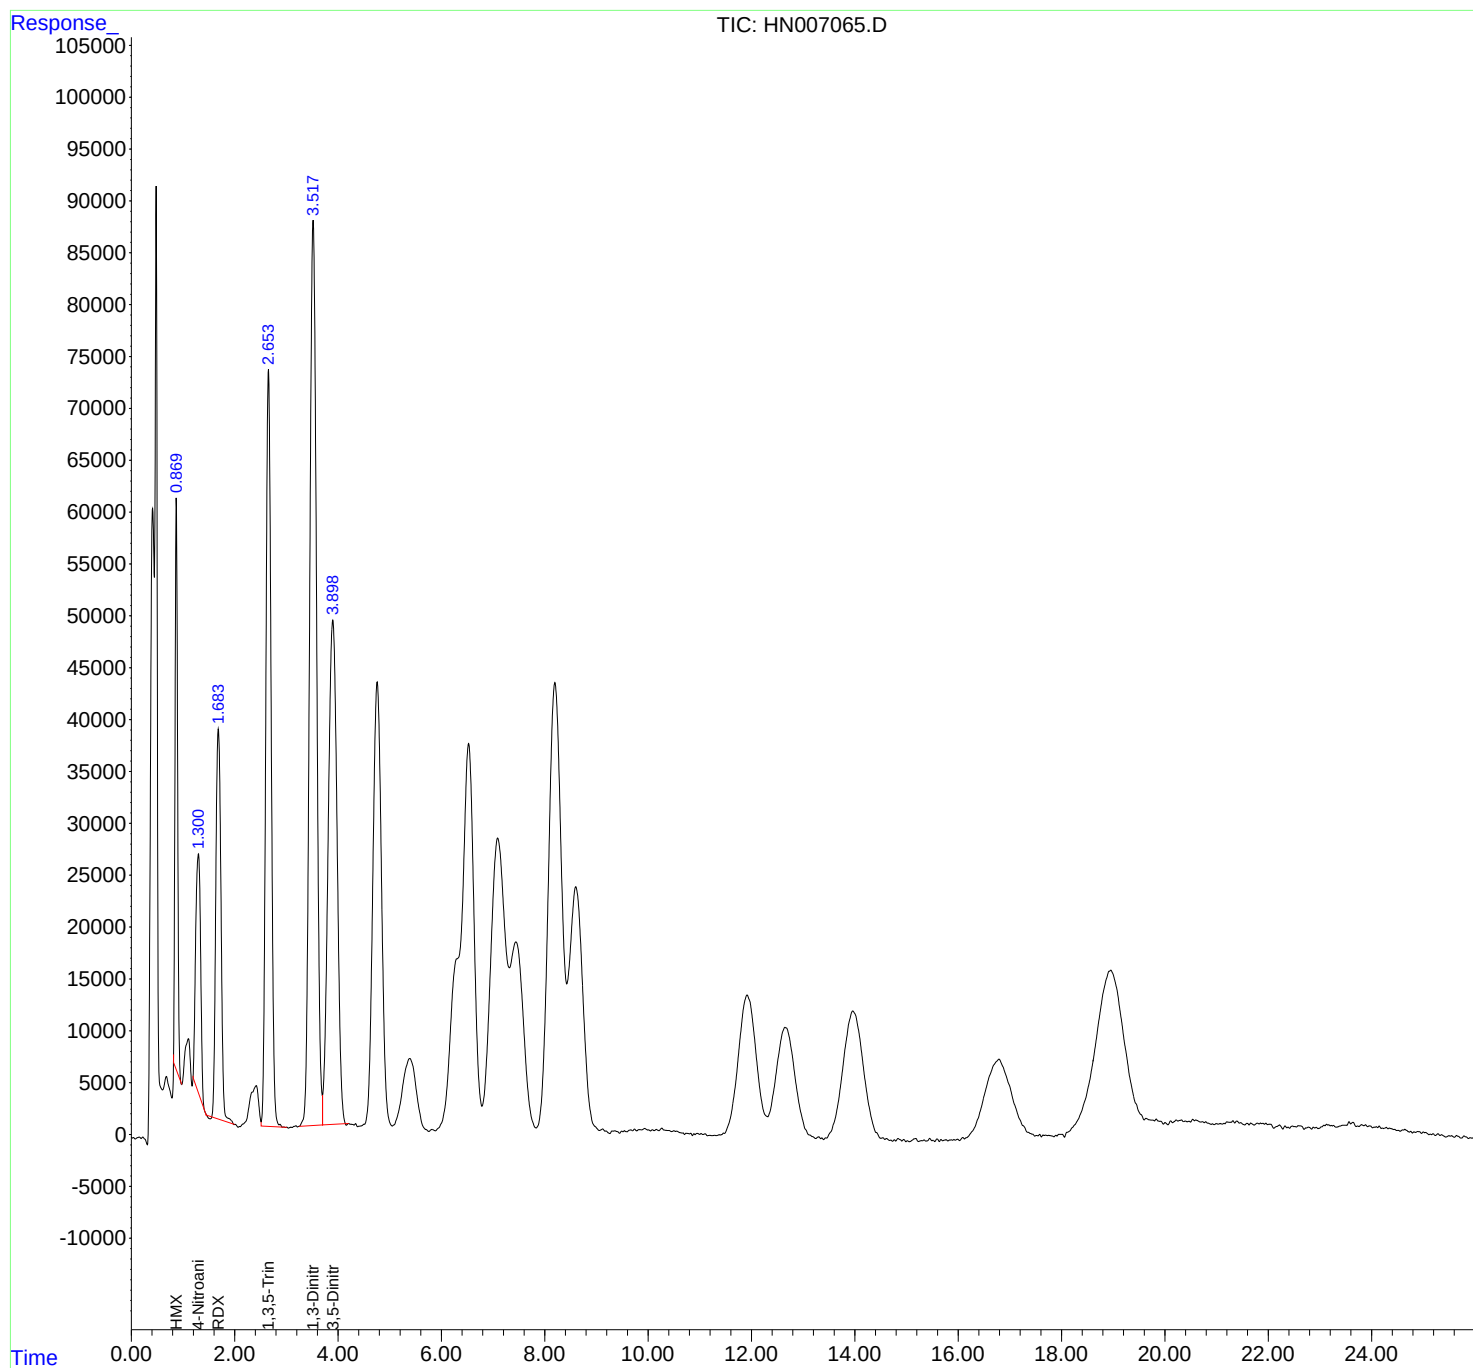


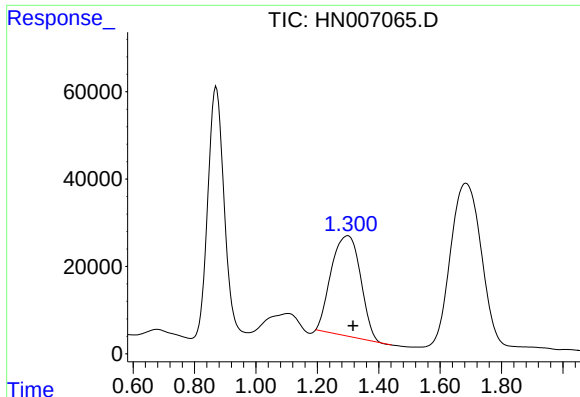

#1 4-Nitroaniline


R.T.: 1.299 min
Delta R.T.: -0.018 min
Response: 1509451
Conc: 432.47 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

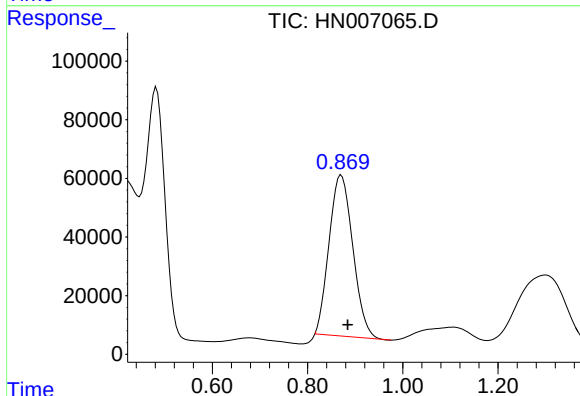


#2 HMX

R.T.: 0.871 min
Delta R.T.: -0.014 min
Response: 1900915
Conc: 451.25 ug/L

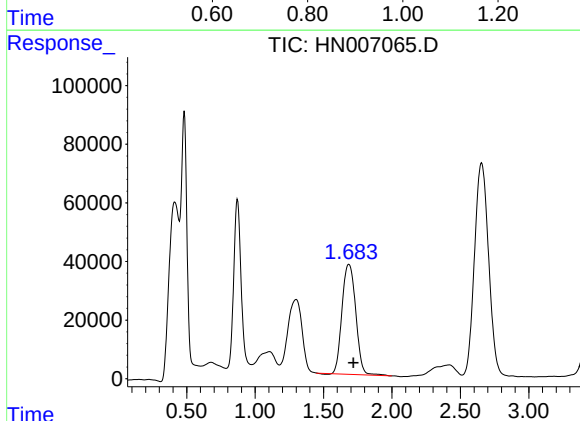


#3 RDX

R.T.: 1.685 min
Delta R.T.: -0.033 min
Response: 2623183
Conc: 518.70 ug/L

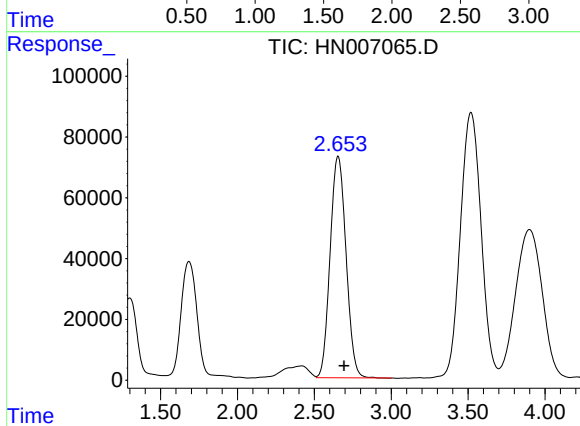

#4 1,3,5-Trinitrobenzene


R.T.: 2.655 min
Delta R.T.: -0.038 min
Response: 5239095
Conc: 514.26 ug/L

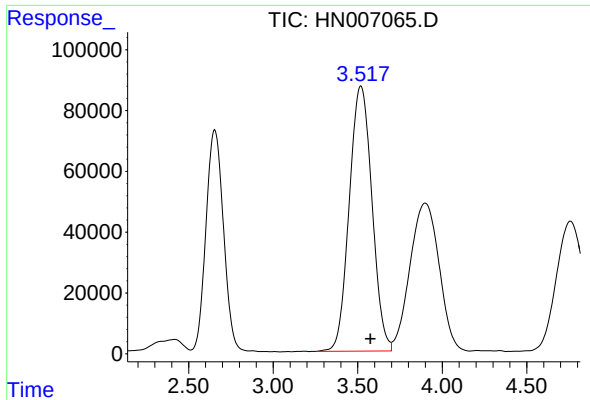

#5 1,3-Dinitrobenzene

R.T.: 3.519 min
Delta R.T.: -0.056 min
Response: 8147562
Conc: 510.72 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

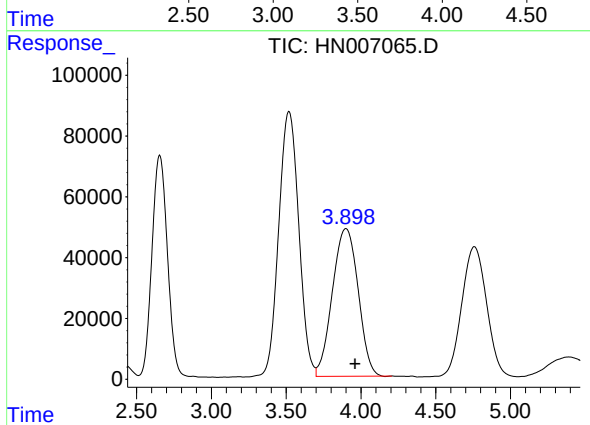

#6 3,5-Dinitroaniline

R.T.: 3.899 min
Delta R.T.: -0.062 min
Response: 5812563
Conc: 517.56 ug/L