

Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN110614\  
 Data File : HN007057.D  
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
 Acq On : 06-Nov-2014, 17:58  
 Operator : TP  
 Sample : F4372-03MS  
 Misc :  
 ALS Vial : 71 Sample Multiplier: 1

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 YS19-SD01-1014MS

Integration File signal 1: AUTOINT1.E  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 07 04:37:19 2015  
 Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1029NG.M  
 Quant Title :  
 QLast Update : Sat Mar 07 04:29:22 2015  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 50 ul  
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T.  | Response | Conc Units  |
|-----------------------------|-------|----------|-------------|
| -----                       |       |          |             |
| System Monitoring Compounds |       |          |             |
| 1) S 4-Nitroaniline         | 1.307 | 1163901  | 0.318 ng/ul |
|                             |       |          |             |
| Target Compounds            |       |          |             |
| 2) T Nitroglycerin          | 6.060 | 2440921  | 0.323 ng/ul |
| -----                       |       |          |             |

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN110614\  
Data File : HN007057.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 06-Nov-2014, 17:58  
Operator : TP  
Sample : F4372-03MS  
Misc :  
ALS Vial : 71 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SD01-1014MS

Integration File signal 1: AUTOINT1.E  
Integration File signal 2: autoint2.e  
Quant Time: Mar 07 04:37:19 2015  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1029NG.M  
Quant Title :  
QLast Update : Sat Mar 07 04:29:22 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

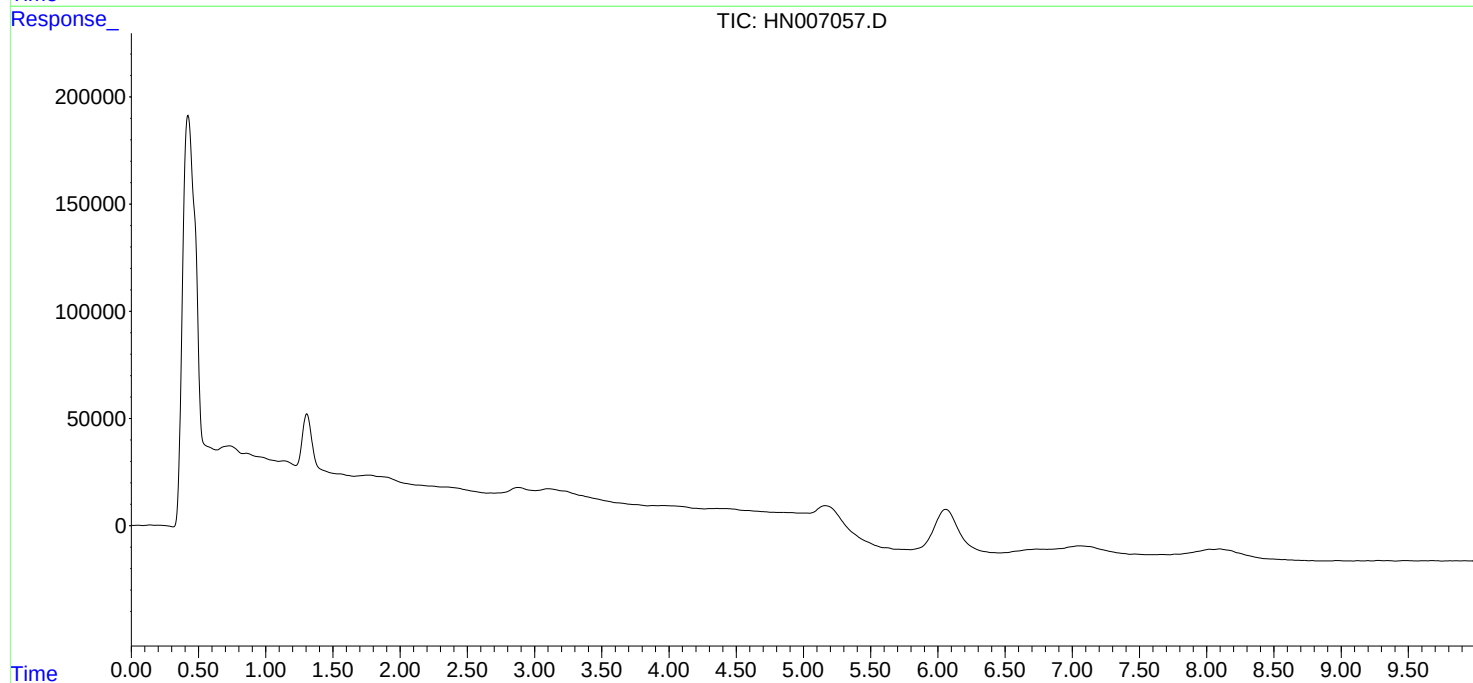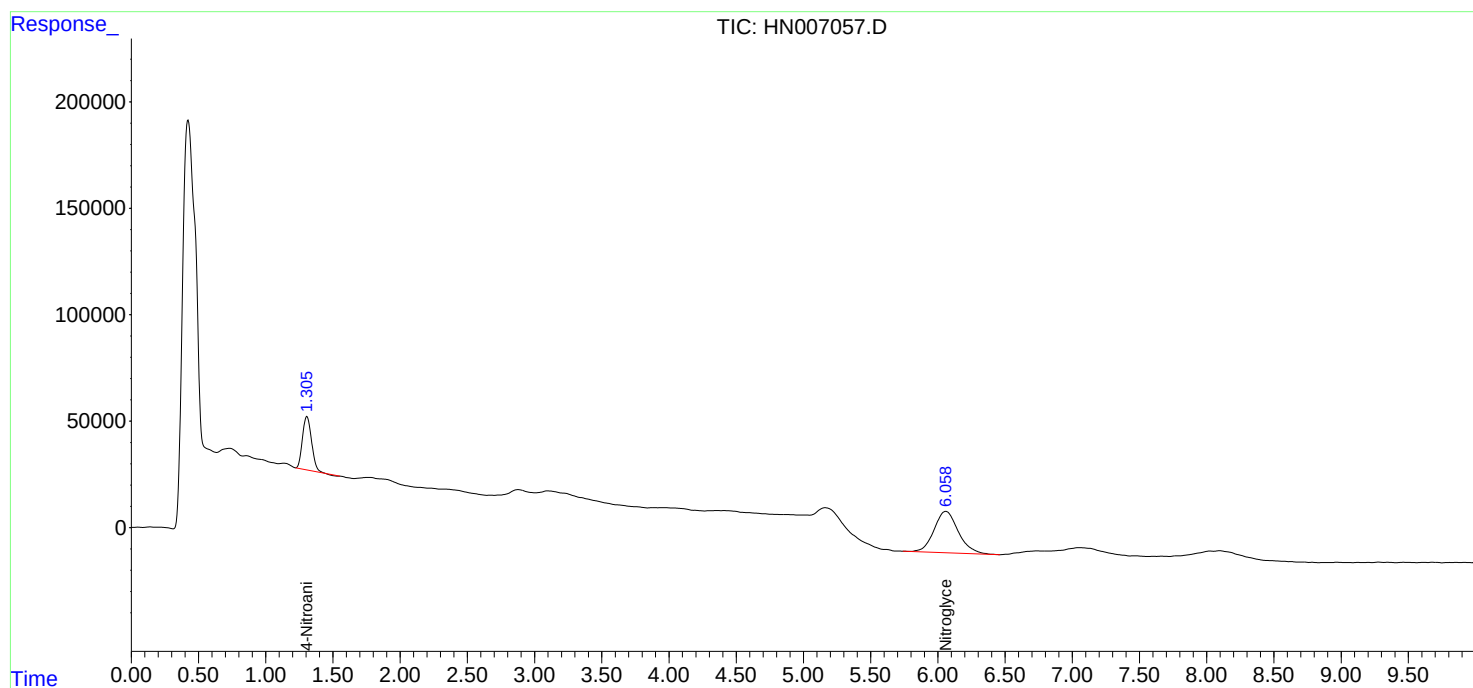


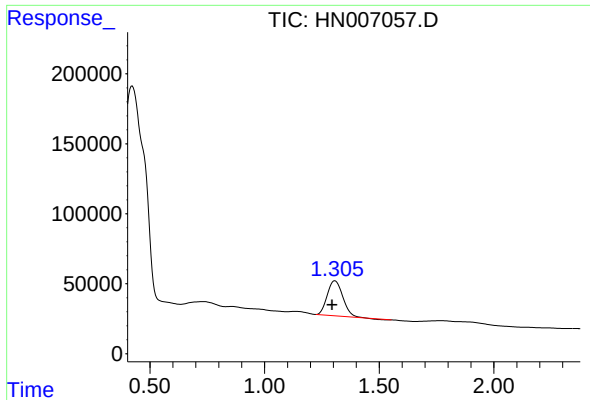

#1 4-Nitroaniline

R.T.: 1.307 min  
Delta R.T.: 0.013 min  
Response: 1163901  
Conc: 0.32 ng/ul

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SD01-1014MS

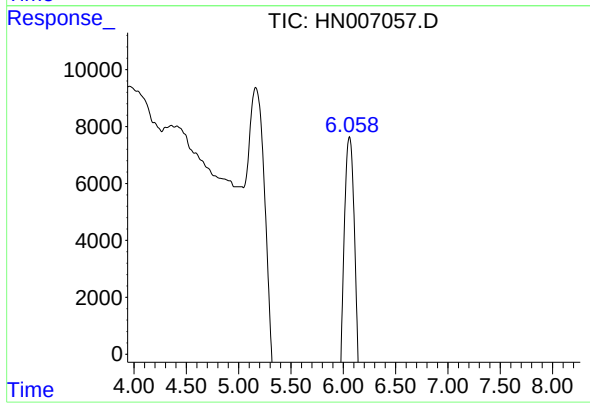

#2 Nitroglycerin

R.T.: 6.060 min  
Delta R.T.: 0.020 min  
Response: 2440921  
Conc: 0.32 ng/ul