

Data File : S:\HPCHEM1\HPLC_N\DATA\HN110813\HN005668.D Vial: 3
Acq On : 08-Nov-2013, 16:45 Operator: QM
Sample : HSTDICC010 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 9 2:15 2013 Quant Results File: HN1108NG.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC010

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN1108NG.M
Title :
Last Update : Sat Nov 09 01:52:27 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.29	38848853	9.343 ng/ul
Target Compounds			
2) T Nitroglycerin	5.86	85126431	10.253 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005668.D HN1108NG.M

Sat Nov 09 02:15:57 2013

RPT1


Quantitation Report


Data File : S:\HPCHEM1\HPLC_N\DATA\HN110813\HN005668.D Vial: 3
Acq On : 08-Nov-2013, 16:45 Operator: QM
Sample : HSTDICC010 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 9 2:15 2013 Quant Results File: HN1108NG.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC010

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN1108NG.M
Title :
Last Update : Sat Nov 09 01:52:27 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

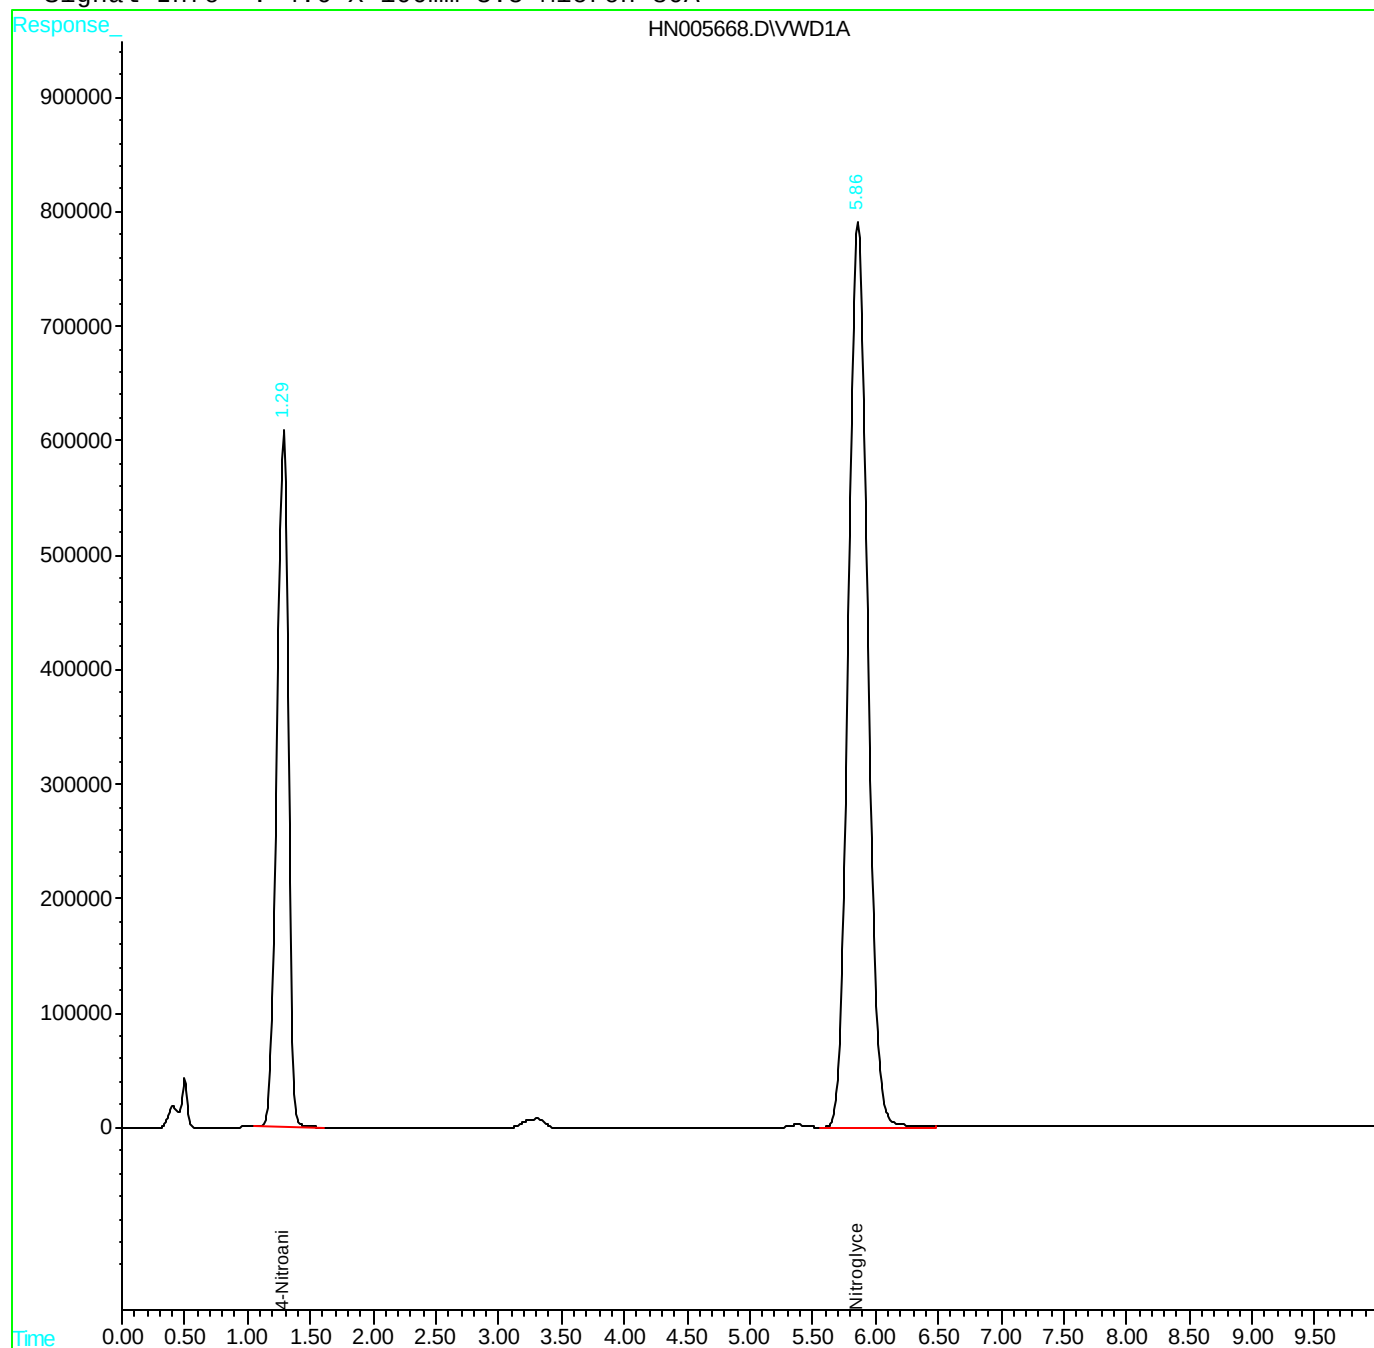


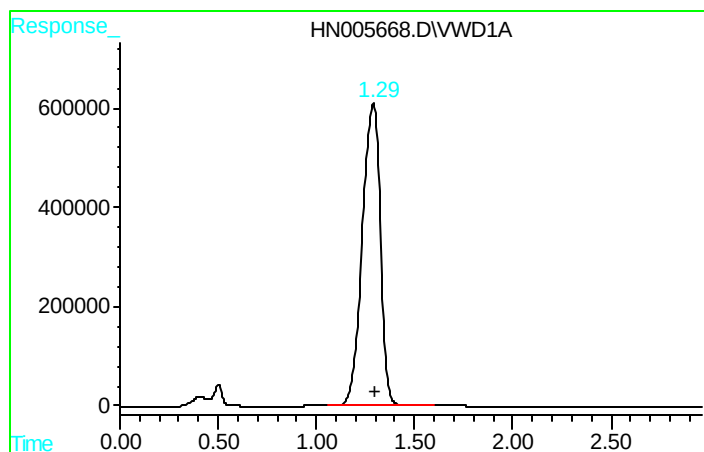

#1 4-Nitroaniline

R.T.: 1.291 min
Delta R.T.: -0.003 min
Response: 38848853
Conc: 9.34 ng/ul

Instrument :
HPLC_N
LabSampleId :
HSTDIC010

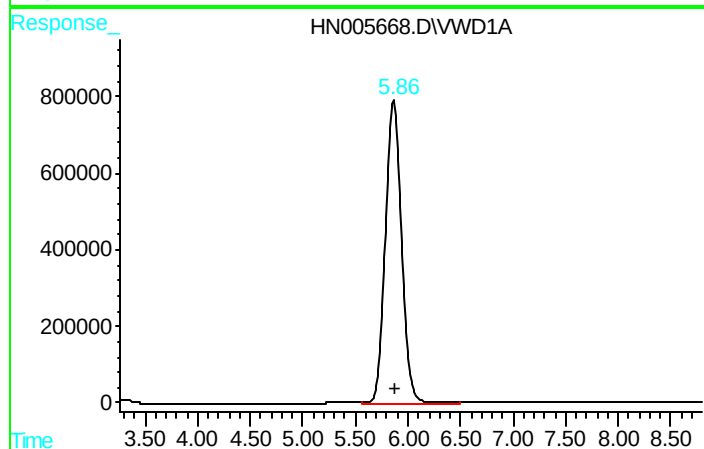

#2 Nitroglycerin

R.T.: 5.862 min
Delta R.T.: -0.007 min
Response: 85126431
Conc: 10.25 ng/ul