

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN110813\HN005671.D Vial: 6
Acq On : 08-Nov-2013, 17:21 Operator: QM
Sample : HSTDICC0.5 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 11 15:19 2013 Quant Results File: HN1108NG.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC0.5

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN1108NG.M
Title :
Last Update : Sat Nov 09 01:52:27 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.29	1958713	0.507 ng/ul
Target Compounds			
2) T Nitroglycerin	5.87	4774949	0.561 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005671.D HN1108NG.M

Mon Nov 11 15:19:16 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN110813\HN005671.D Vial: 6
Acq On : 08-Nov-2013, 17:21 Operator: QM
Sample : HSTDICC0.5 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 11 15:19 2013 Quant Results File: HN1108NG.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC0.5

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN1108NG.M
Title :
Last Update : Sat Nov 09 01:52:27 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

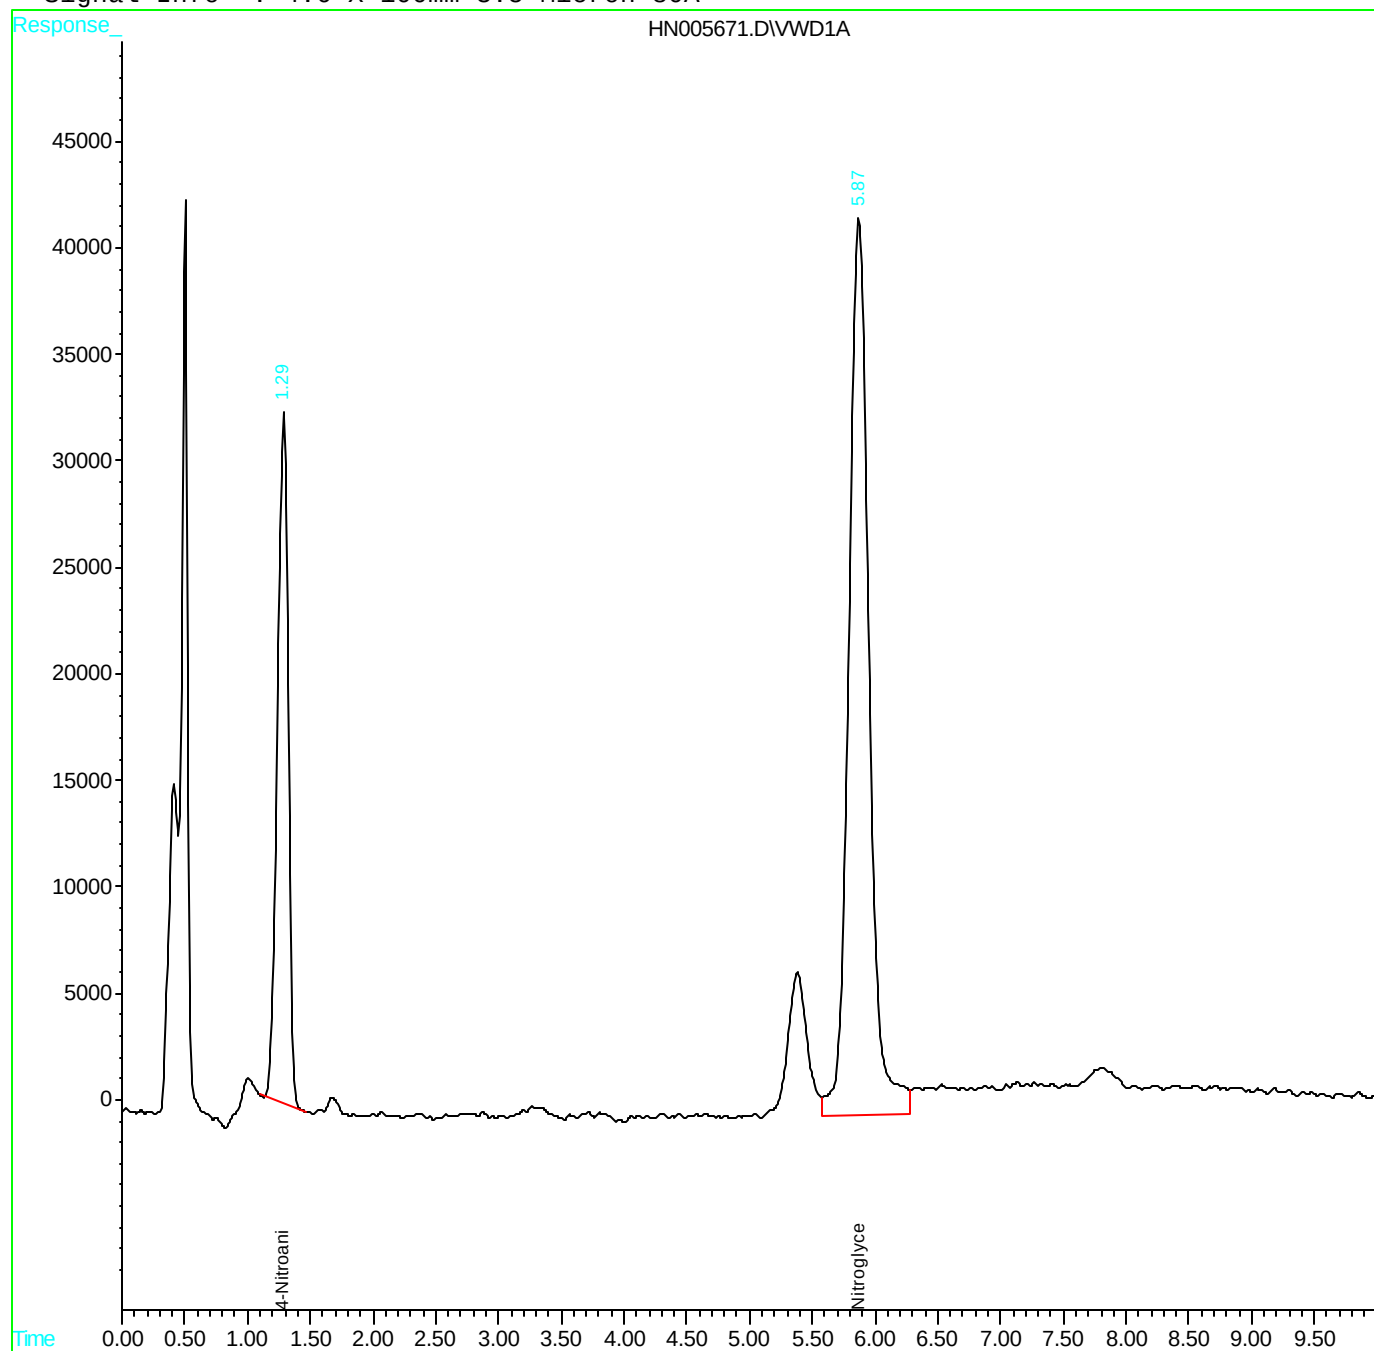


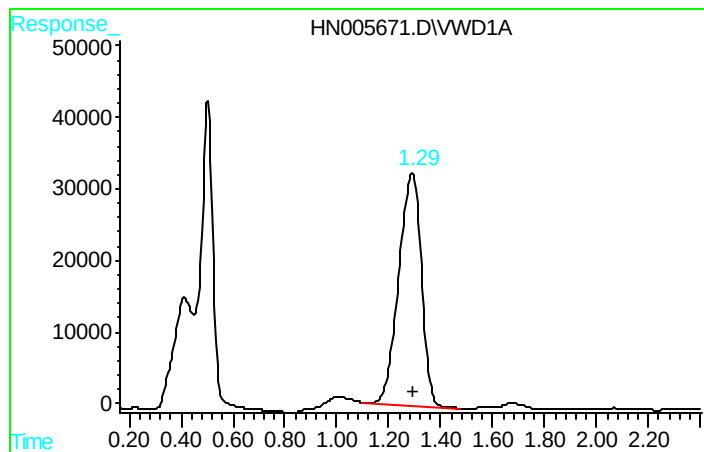

#1 4-Nitroaniline

R.T.: 1.292 min
Delta R.T.: -0.002 min
Response: 1958713
Conc: 0.51 ng/ul

Instrument :
HPLC_N
LabSampleId :
HSTDICC0.5

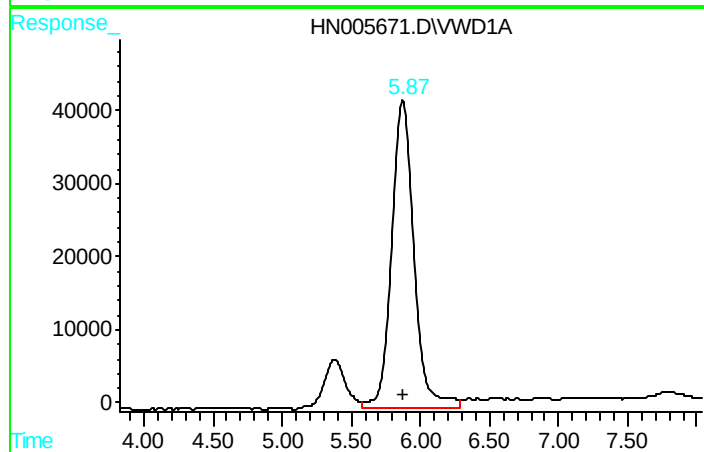

#2 Nitroglycerin

R.T.: 5.871 min
Delta R.T.: 0.003 min
Response: 4774949
Conc: 0.56 ng/ul