

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN110813\HN005666.D Vial: 1
Acq On : 08-Nov-2013, 16:08 Operator: QM
Sample : HSTDICC050 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 9 2:14 2013 Quant Results File: HN1108NG.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC050

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN1108NG.M
Title :
Last Update : Sat Nov 09 01:52:27 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.29	190899825	45.912 ng/ul
Target Compounds			
2) T Nitroglycerin	5.83	413616880	49.816 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005666.D HN1108NG.M

Tue Nov 12 02:51:43 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN110813\HN005666.D Vial: 1
Acq On : 08-Nov-2013, 16:08 Operator: QM
Sample : HSTDICC050 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 9 2:14 2013 Quant Results File: HN1108NG.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC050

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN1108NG.M
Title :
Last Update : Sat Nov 09 01:52:27 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

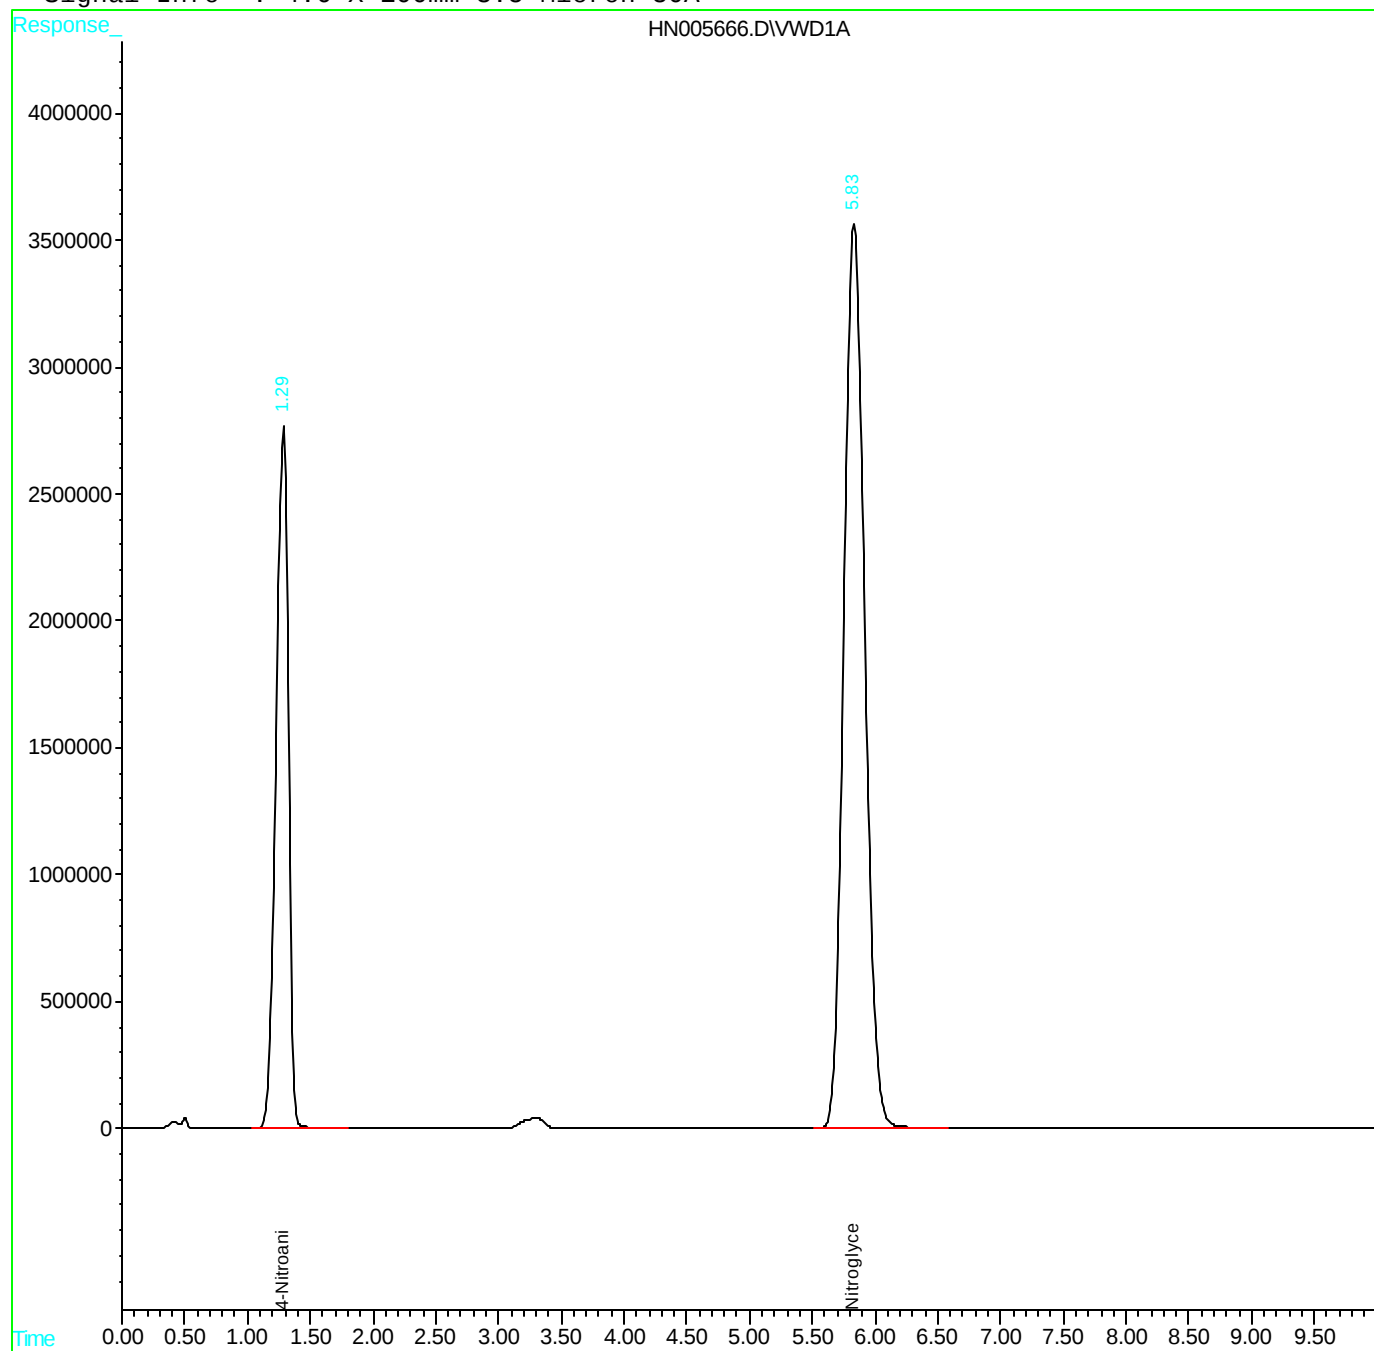


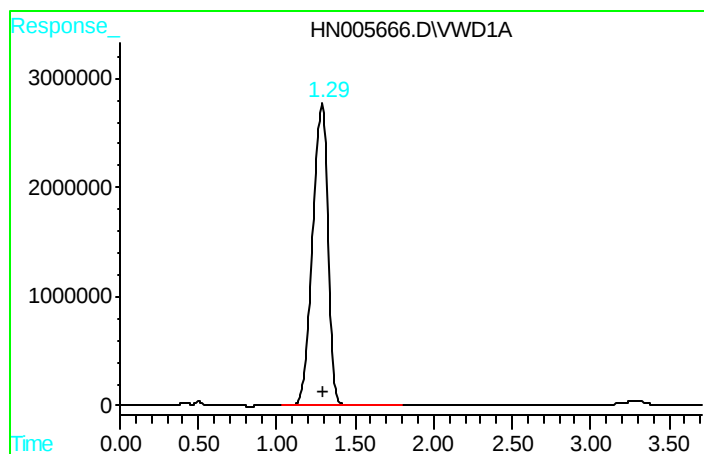

#1 4-Nitroaniline

R.T.: 1.290 min
 Delta R.T.: -0.004 min
 Response: 190899825
 Conc: 45.91 ng/ul

Instrument :
 HPLC_N
 LabSampleId :
 HSTDIC050

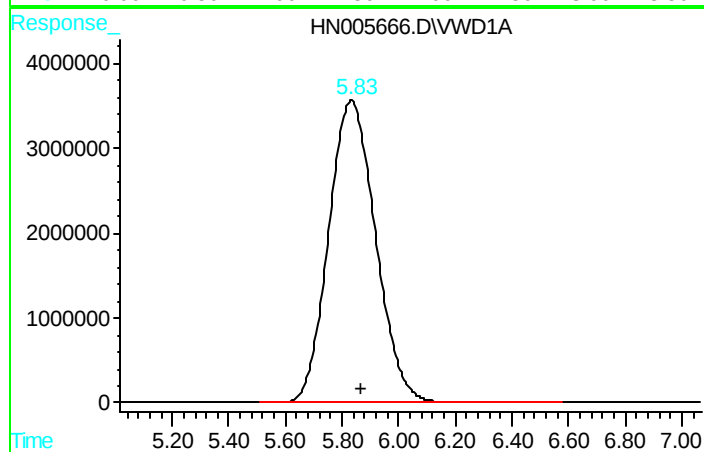

#2 Nitroglycerin

R.T.: 5.833 min
 Delta R.T.: -0.036 min
 Response: 413616880
 Conc: 49.82 ng/ul