

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN110813\HN005670.D Vial: 5
Acq On : 08-Nov-2013, 17:09 Operator: QM
Sample : HSTDICC001 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 9 2:16 2013 Quant Results File: HN1108NG.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC001

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN1108NG.M
Title :
Last Update : Sat Nov 09 01:52:27 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.29	3849009	0.926 ng/ul
Target Compounds			
2) T Nitroglycerin	5.87	8738260	1.052 ng/ul

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005670.D HN1108NG.M

Tue Nov 12 02:50:31 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN110813\HN005670.D Vial: 5
Acq On : 08-Nov-2013, 17:09 Operator: QM
Sample : HSTDICC001 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 9 2:16 2013 Quant Results File: HN1108NG.RES

Instrument :
HPLC_N
LabSampleId :
HSTDICC001

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN1108NG.M
Title :
Last Update : Sat Nov 09 01:52:27 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

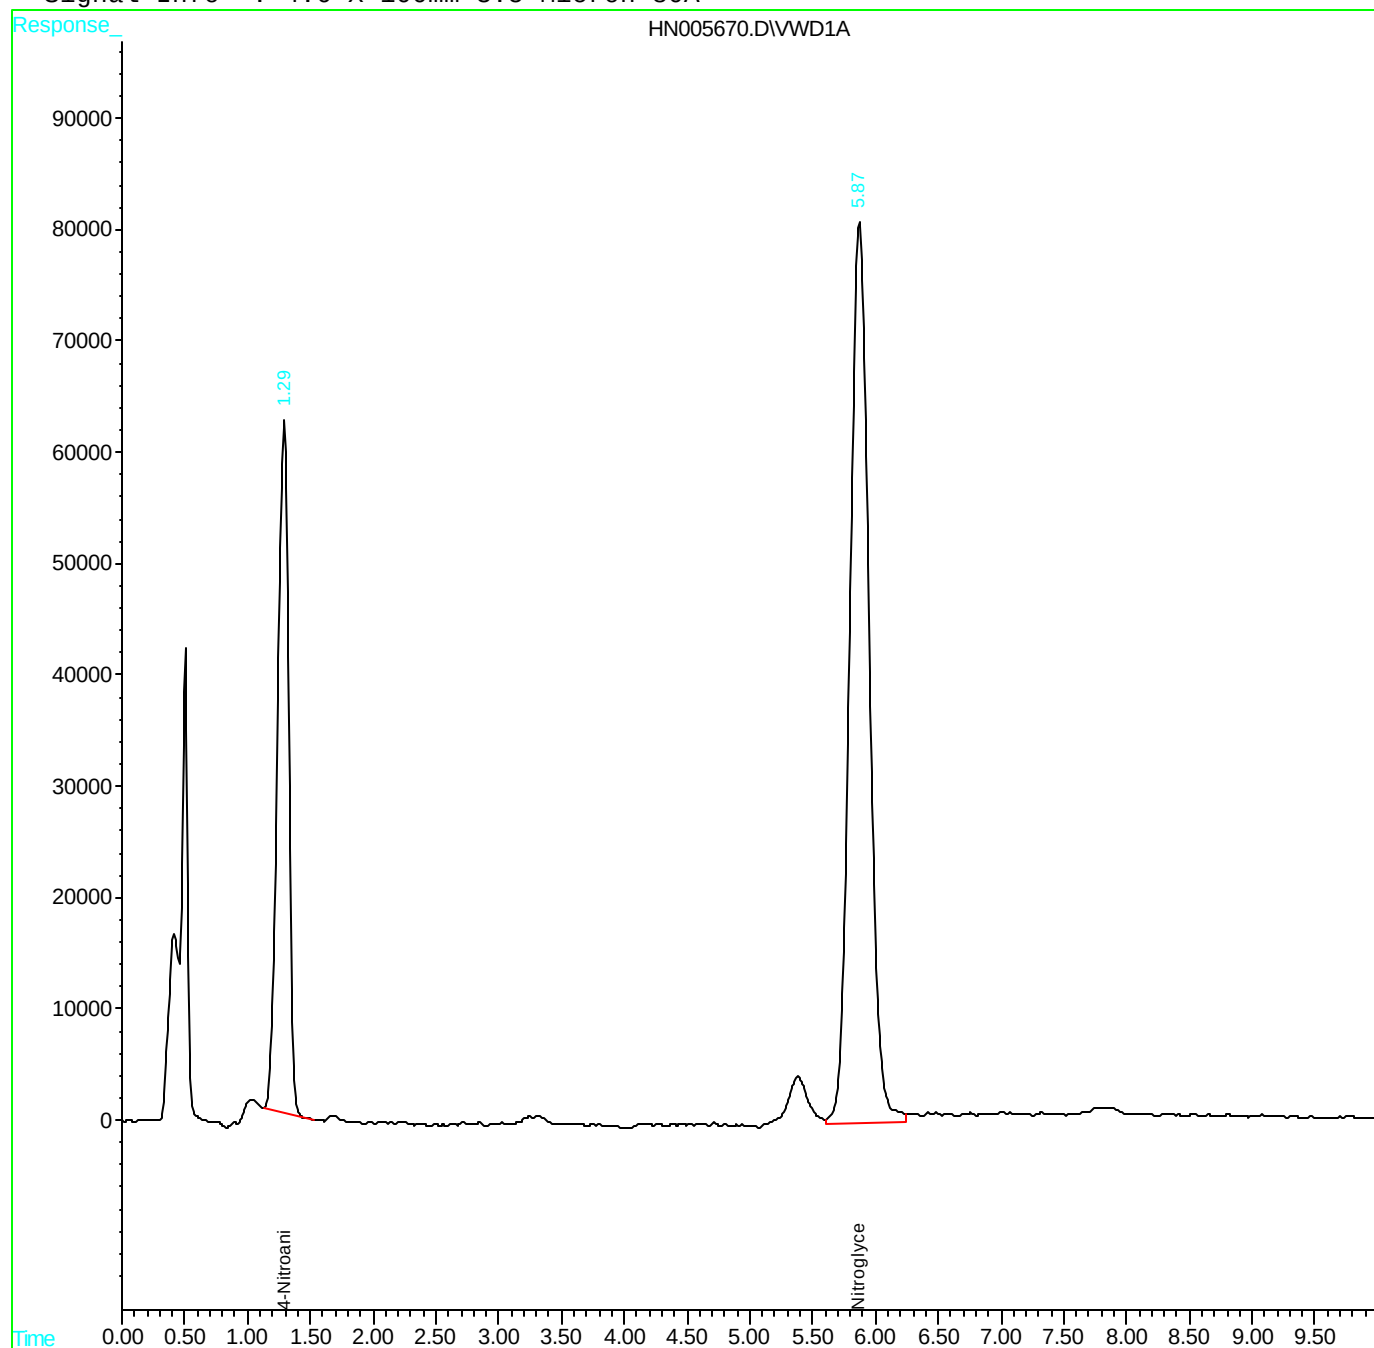


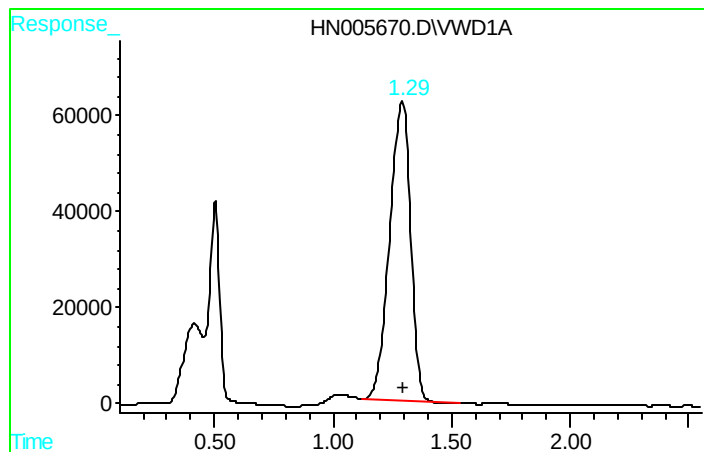

#1 4-Nitroaniline

R.T.: 1.294 min
 Delta R.T.: 0.000 min
 Response: 3849009
 Conc: 0.93 ng/ul

Instrument :
 HPLC_N
 LabSampleId :
 HSTDIC001

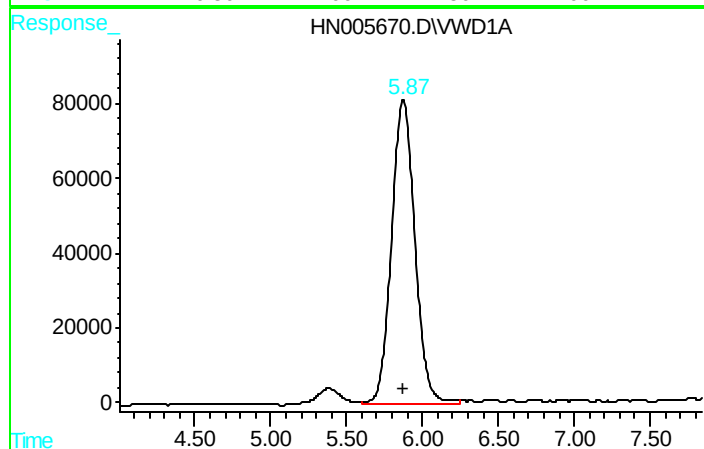

#2 Nitroglycerin

R.T.: 5.874 min
 Delta R.T.: 0.005 min
 Response: 8738260
 Conc: 1.05 ng/ul