

Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN110813\HN005671.D Vial: 6  
 Acq On : 08-Nov-2013, 17:21 Operator: QM  
 Sample : HSTDIC0.5 Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile : AUTOINT1.E  
 Quant Time: Nov 11 15:19 2013 Quant Results File: HN1108NG.RES

Instrument :  
 HPLC\_N  
 LabSampleId :  
 HSTDIC0.5

Manual Integrations  
 APPROVED  
 QI  
 11/11/2013 6:42:05 PM

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN1108NG.M  
 Title :  
 Last Update : Sat Nov 09 01:52:27 2013  
 Response via : Initial Calibration  
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
 Signal Phase : ZORBAX Extend-C18  
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
1) S 4-Nitroaniline	1.29	1958713	0.507 ng/ul
Target Compounds			
2) T Nitroglycerin	5.87	4287767	0.504 ng/ulm

-----  
 Analyst Signature: \_\_\_\_\_ Analyst Name: \_\_\_\_\_ Date: \_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #: \_\_\_\_\_

\_\_\_Peak integrated by software incorrectly.Compound #: \_\_\_\_\_

\_\_\_OTHER: \_\_\_\_\_ Compound #: \_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN110813\HN005671.D Vial: 6  
Acq On : 08-Nov-2013, 17:21 Operator: QM  
Sample : HSTDICC0.5 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : AUTOINT1.E  
Quant Time: Nov 11 15:19 2013 Quant Results File: HN1108NG.RES


Instrument :  
HPLC\_N  
LabSampleId :  
HSTDICC0.5

Manual Integrations  
APPROVED  
QI  
11/11/2013 6:42:05 PM

Quant Method : Z:\HPCHEM1\HPLC\_N\METHOD\HN1108NG.M  
Title :  
Last Update : Sat Nov 09 01:52:27 2013  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

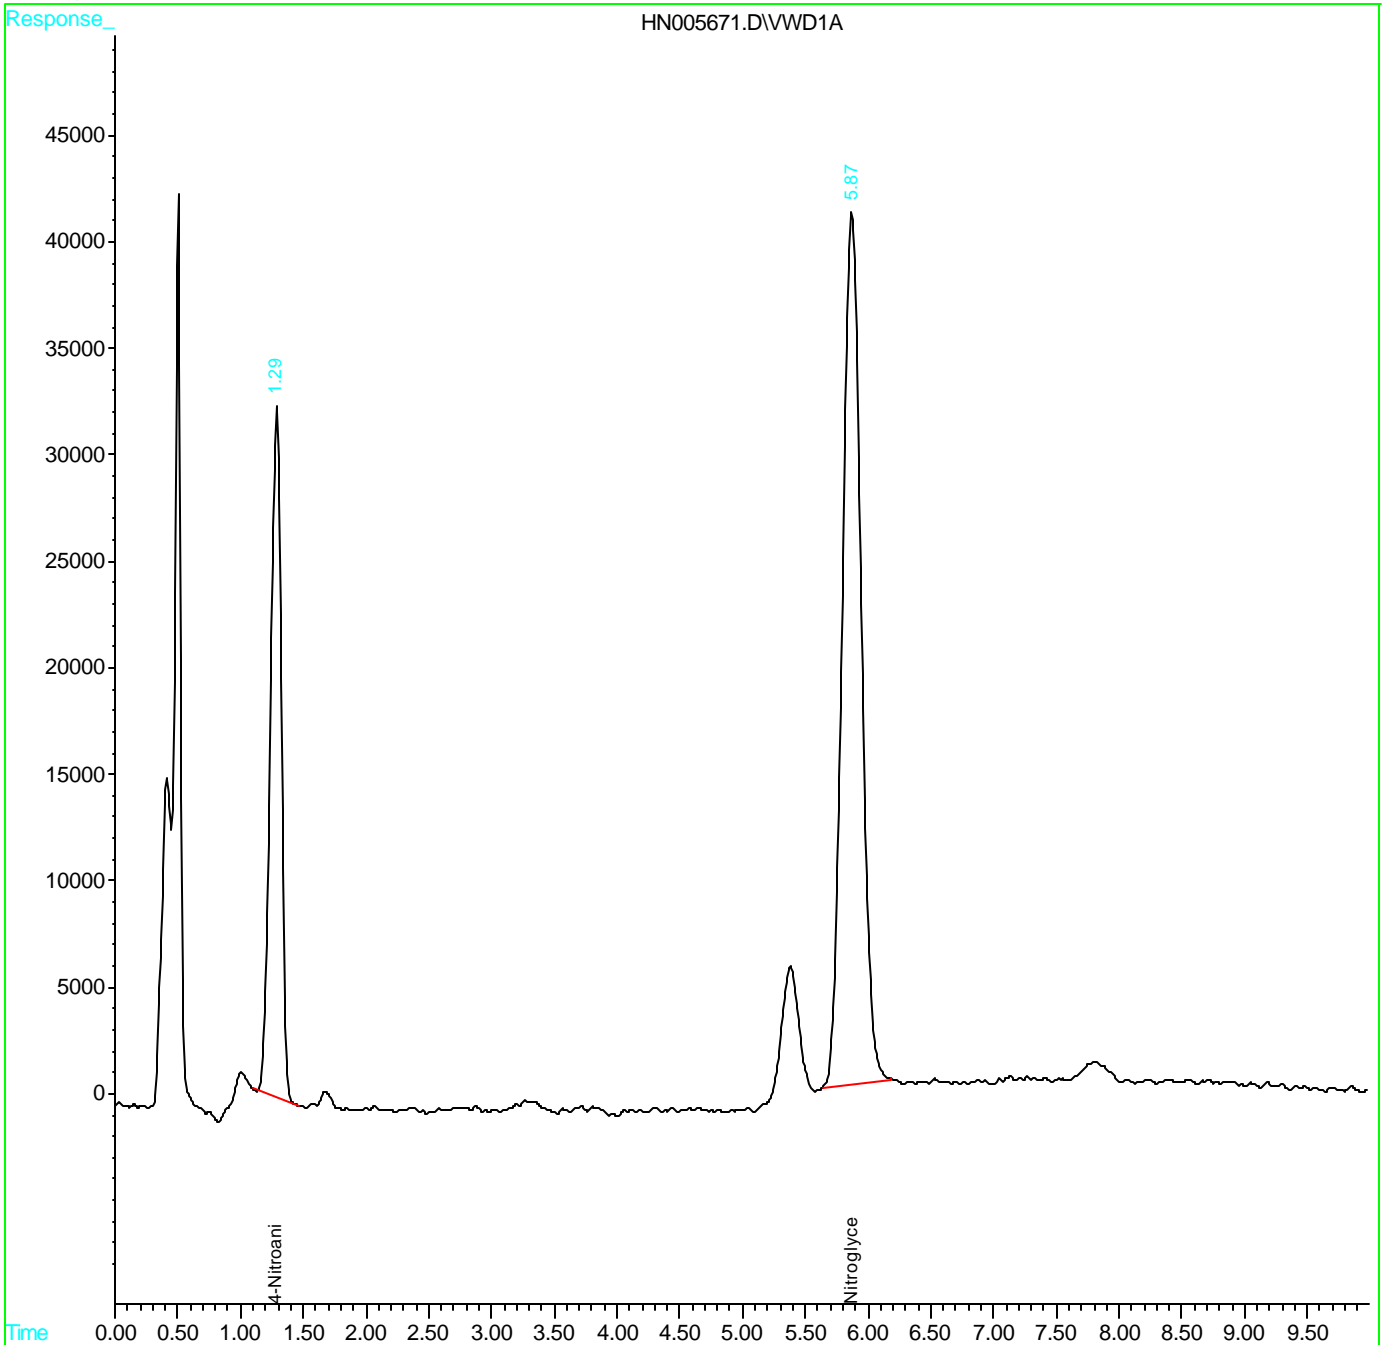

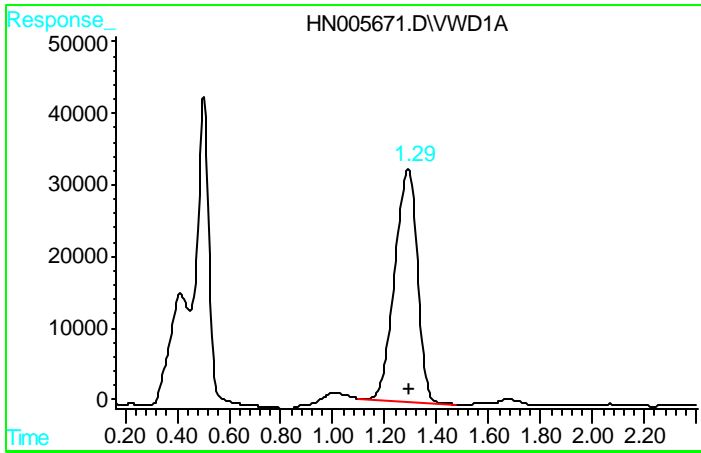


#1 4-Nitroaniline

R.T.: 1.292 min  
 Delta R.T.: -0.002 min  
 Response: 1958713  
 Conc: 0.51 ng/ul

Instrument :  
 HPLC\_N  
 LabSampleId :  
 HSTDIC0.5

Manual Integrations  
 APPROVED  
 QI  
 11/11/2013 6:42:05 PM

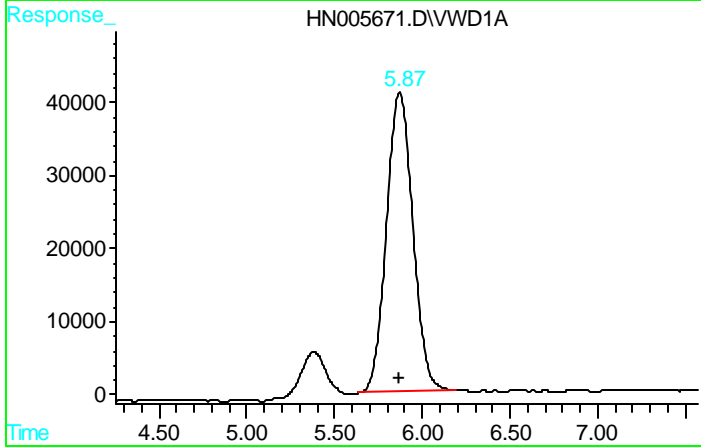

#2 Nitroglycerin

R.T.: 5.869 min  
 Delta R.T.: 0.000 min  
 Response: 4287767  
 Conc: 0.50 ng/ul m