

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN110813\HN005684.D Vial: 14
Acq On : 08-Nov-2013, 23:01 Operator: QM
Sample : PB72976BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Nov 11 12:13 2013 Quant Results File: HN110813.RES

Instrument :
HPLC_N
ClientSampleId :
PB72976BL

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN110813.M
Title :
Last Update : Mon Jul 22 14:51:19 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.29	1182593	320.371 ug/L

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005684.D HN110813.M

Tue Nov 12 02:41:29 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN110813\HN005684.D Vial: 14
Acq On : 08-Nov-2013, 23:01 Operator: QM
Sample : PB72976BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Nov 11 12:13 2013 Quant Results File: HN110813.RES

Instrument :
HPLC_N
ClientSampleId :
PB72976BL

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN110813.M
Title :
Last Update : Mon Jul 22 14:51:19 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

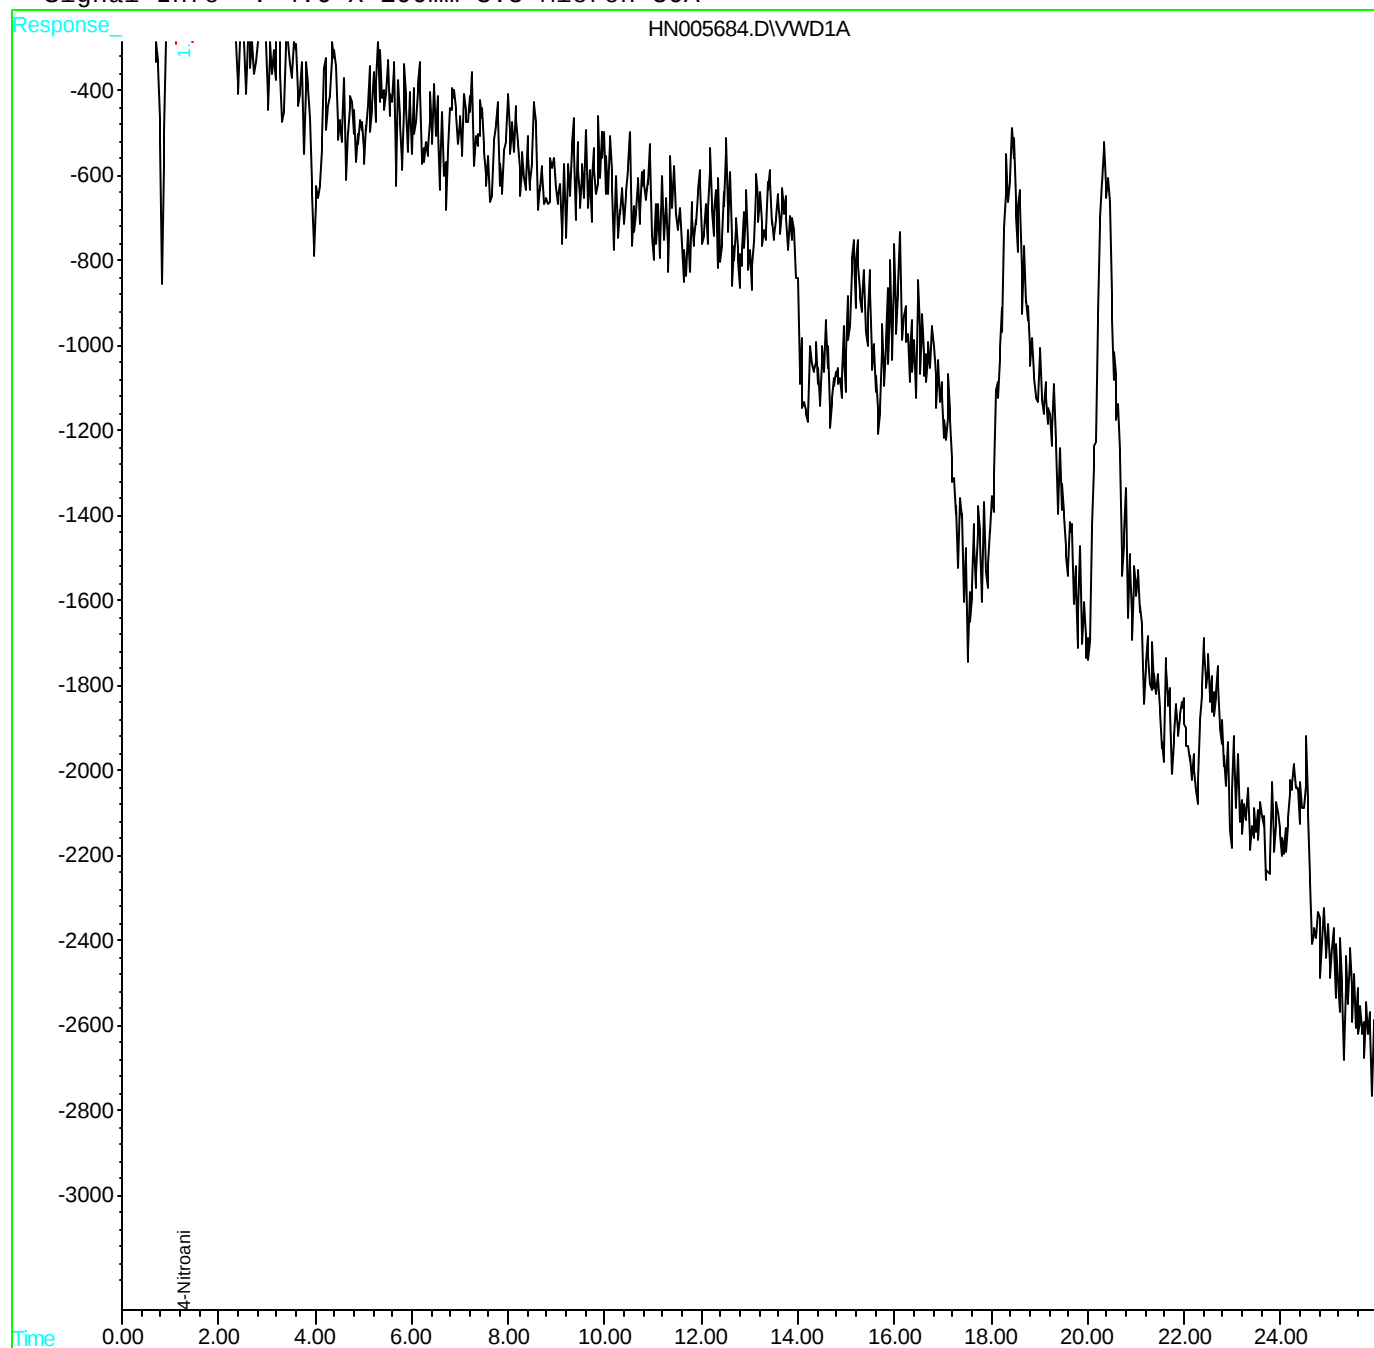

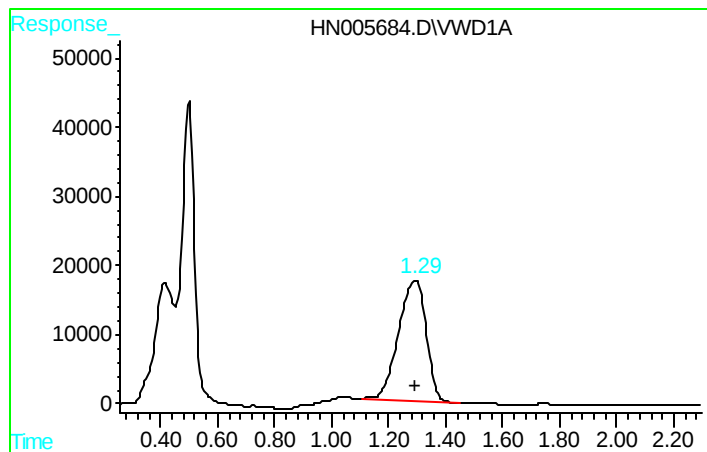

#1 4-Nitroaniline

R.T.: 1.294 min
Delta R.T.: 0.002 min
Response: 1182593
Conc: 320.37 ug/L

Instrument :
HPLC_N
ClientSampleId :
PB72976BL