

Data File : H:\VOL1\HPLC\HPLC N\121109\HN000573.D Vial: 2
 Acq On : 09-Nov-2012, 18:51 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Nov 16 15:37 2012 Quant Results File: HN101012.RES

Instrument :
 HPLC_N
 LabSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)
 Title : SW8330 / 8330A confirmation
 Last Update : Fri Nov 16 15:37:27 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330VWDC.M

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.83	9862361	953.239 ug/L
Target Compounds				
2) T	HMX	13.50	10094133	977.462 ug/L
3) T	RDX	11.11	13640341	978.960 ug/L
4) T	1,3,5-Trinitrobenzene	25.89	13871446	497.765 ug/L
5) T	Tetryl	37.40	21158067	978.992 ug/L
6) T	2,4,6-Trinitrotoluene	35.20	12985589	483.593 ug/L
7) T	2-Amino-4,6-dinitrotoluene	16.98	23110132	495.013 ug/L
8) T	4-Amino-2,6-dinitrotoluene	16.98	23110132	495.013 ug/L
9) T	2,4-Dinitrotoluene	22.82	18881388	498.476 ug/L
10) T	2,6-Dinitrotoluene	21.32	9647805	491.896 ug/L
11) T	1,3-Dinitrobenzene	16.35	20018218	494.789 ug/L
12) T	Nitrobenzene	12.64	13110266	501.911 ug/L
13) T	2-Nitrotoluene	17.46	16723810	1046.341 ug/L
14) T	3-Nitrotoluene	18.77	17963620	975.815 ug/L
15) T	4-Nitrotoluene	18.02	14010560	1026.612 ug/L
16) T	3,5-Dinitroaniline	14.21	32500494	971.906 ug/L

Quantitation Report

Data File : H:\VOL1\HPLC\HPLC N\121109\HN000573.D

Vial: 2

Acq On : 09-Nov-2012, 18:51

Operator: HLM

Sample : 8330-CCV

Inst : G1314A

Misc :

Multiplr: 1.00

IntFile : events.e

Quant Time: Nov 16 15:37 2012 Quant Results File: HN101012.RES

Instrument :

HPLC_N

LabSampleId :

8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)

Title : SW8330 / 8330A confirmation

Last Update : Fri Nov 16 15:37:27 2012


Response via : Multiple Level Calibration


DataAcq Meth : 8330VWDC.M

Volume Inj. :

Signal Phase :

Signal Info :

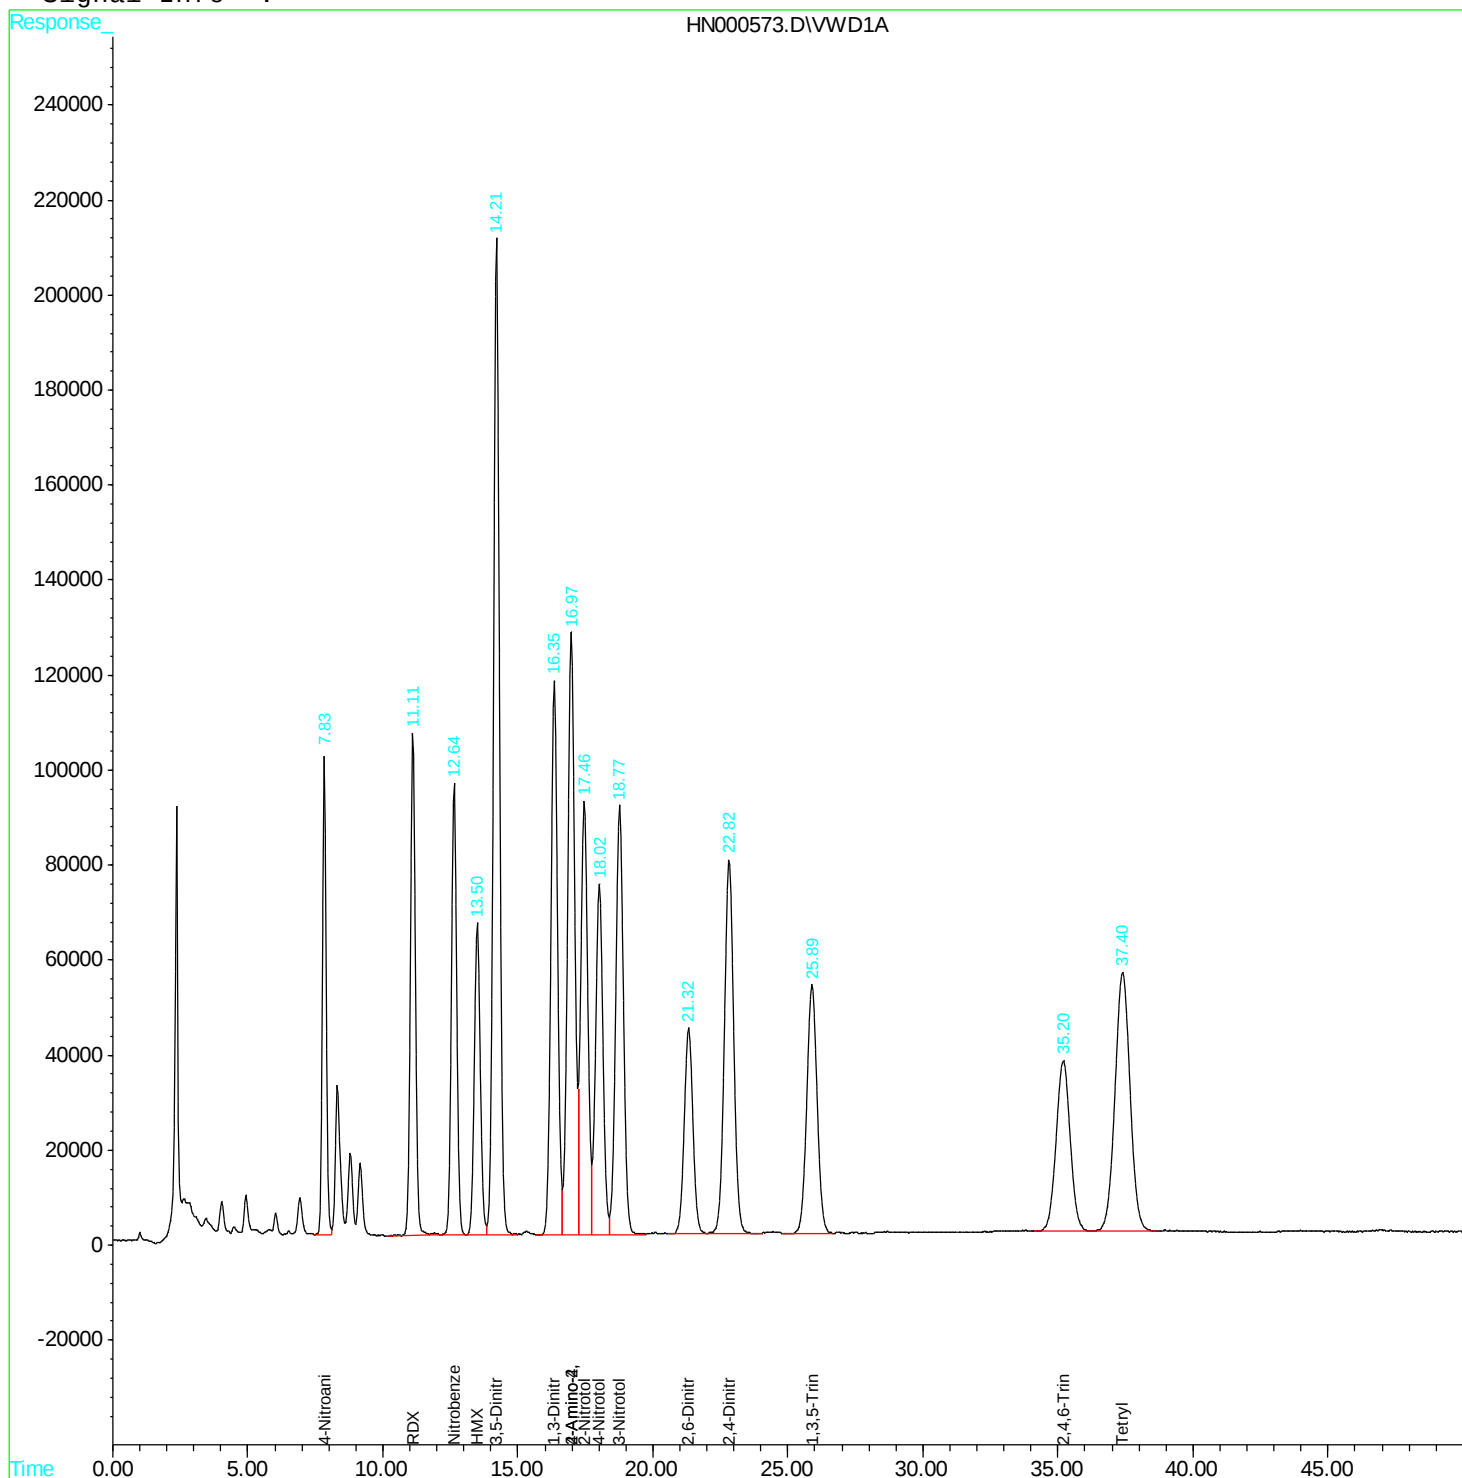


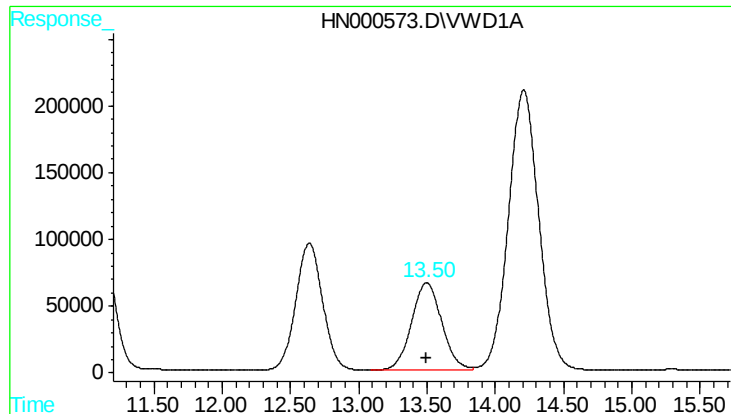

#2 HMX


R.T.: 13.498 min
Delta R.T.: 0.002 min
Response: 10094133
Conc: 977.46 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-CCV

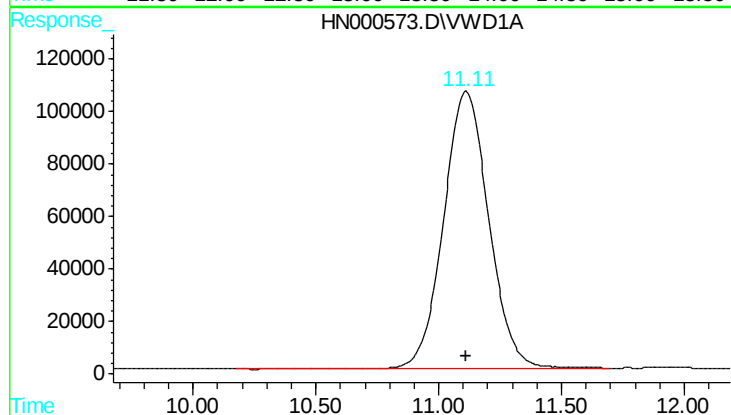


#3 RDX

R.T.: 11.112 min
Delta R.T.: 0.002 min
Response: 13640341
Conc: 978.96 ug/L

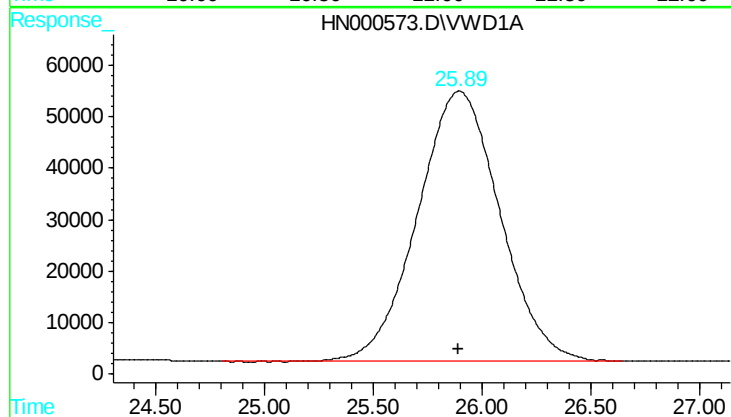


#4 1,3,5-Trinitrobenzene

R.T.: 25.894 min
Delta R.T.: 0.002 min
Response: 13871446
Conc: 497.76 ug/L

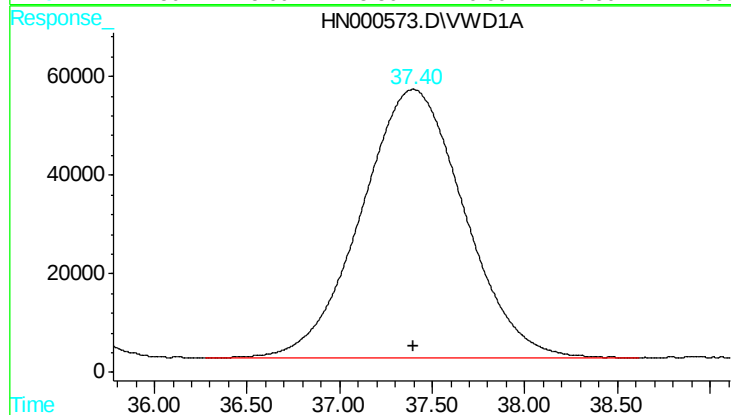

#5 Tetryl


R.T.: 37.397 min
Delta R.T.: 0.000 min
Response: 21158067
Conc: 978.99 ug/L

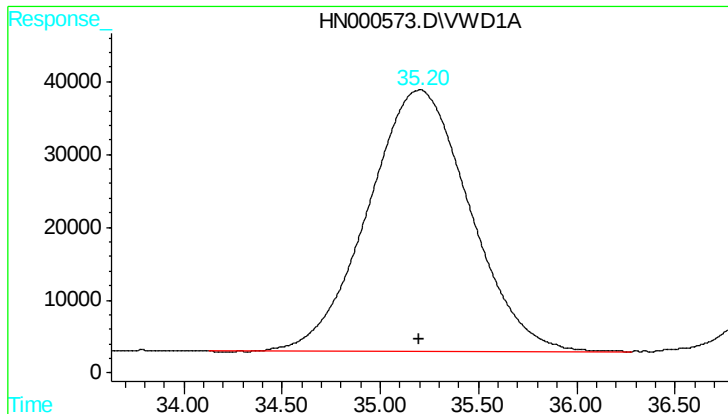

#6 2,4,6-Trinitrotoluene


R.T.: 35.197 min
Delta R.T.: -0.004 min
Response: 12985589
Conc: 483.59 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-CCV

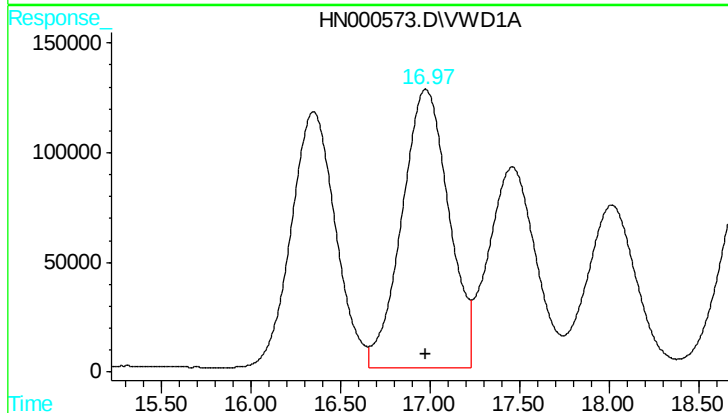


#7 2-Amino-4,6-dinitrotoluene

R.T.: 16.975 min
Delta R.T.: 0.002 min
Response: 23110132
Conc: 495.01 ug/L

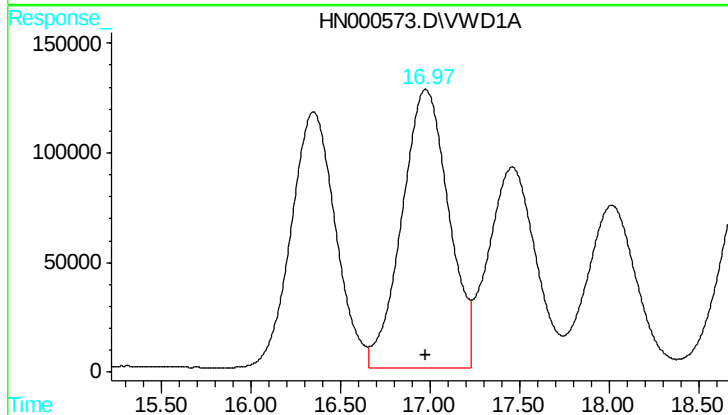


#8 4-Amino-2,6-dinitrotoluene

R.T.: 16.975 min
Delta R.T.: 0.002 min
Response: 23110132
Conc: 495.01 ug/L

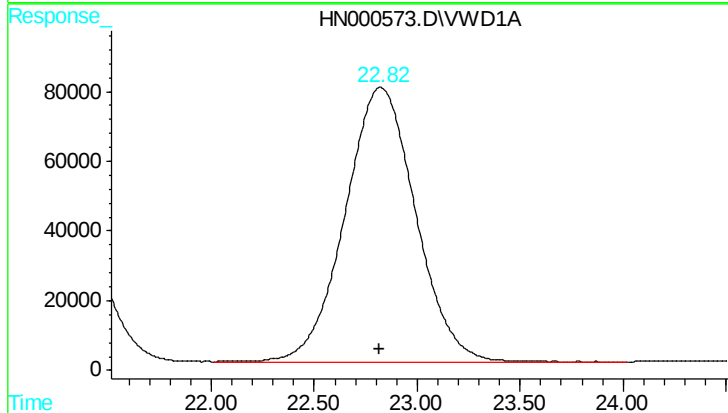

#9 2,4-Dinitrotoluene


R.T.: 22.822 min
Delta R.T.: 0.003 min
Response: 18881388
Conc: 498.48 ug/L

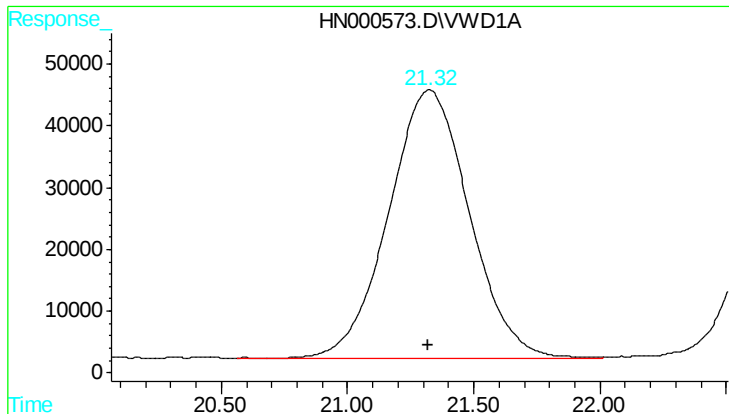

#10 2,6-Dinitrotoluene


R.T.: 21.323 min
Delta R.T.: 0.002 min
Response: 9647805
Conc: 491.90 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-CCV

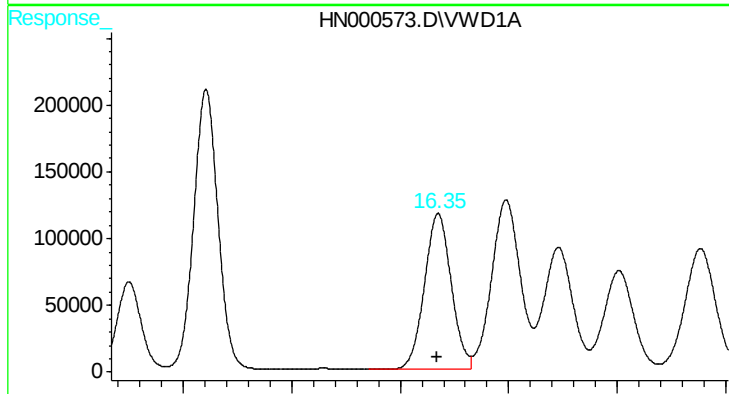


#11 1,3-Dinitrobenzene

R.T.: 16.348 min
Delta R.T.: 0.002 min
Response: 20018218
Conc: 494.79 ug/L

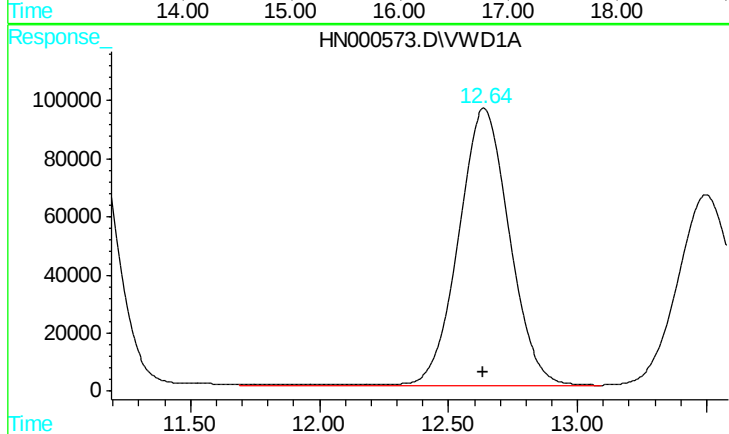


#12 Nitrobenzene

R.T.: 12.638 min
Delta R.T.: 0.002 min
Response: 13110266
Conc: 501.91 ug/L

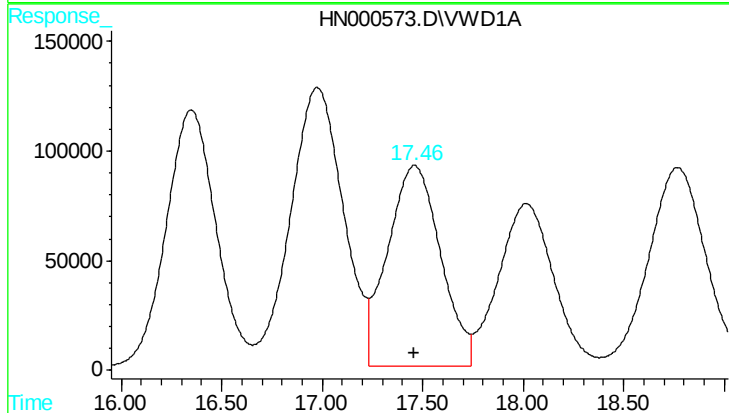

#13 2-Nitrotoluene


R.T.: 17.459 min
Delta R.T.: 0.002 min
Response: 16723810
Conc: 1046.34 ug/L

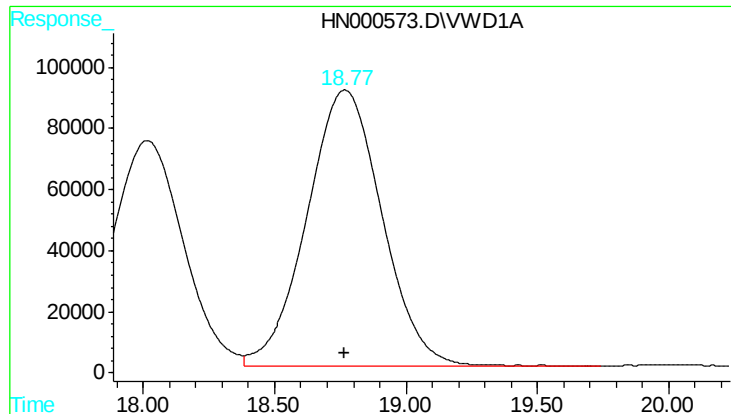

#14 3-Nitrotoluene


R.T.: 18.769 min
Delta R.T.: 0.002 min
Response: 17963620
Conc: 975.82 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-CCV

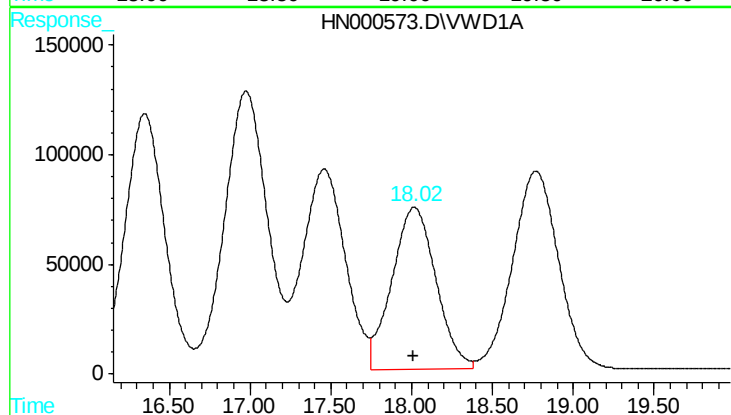

#15 4-Nitrotoluene

R.T.: 18.017 min
Delta R.T.: 0.001 min
Response: 14010560
Conc: 1026.61 ug/L

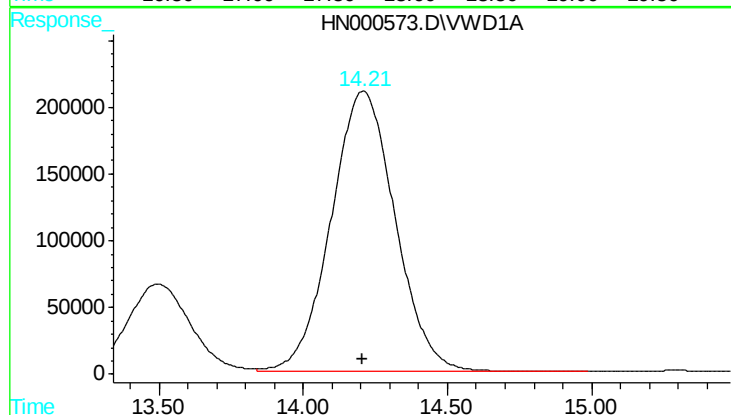

#16 3,5-Dinitroaniline

R.T.: 14.208 min
Delta R.T.: 0.002 min
Response: 32500494
Conc: 971.91 ug/L