

Data File : H:\VOL1\HPLC\HPLC N\121109\HN000578.D Vial: 2
 Acq On : 09-Nov-2012, 23:14 Operator: HLM
 Sample : 8330-CCV Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile : events.e
 Quant Time: Nov 16 15:38 2012 Quant Results File: HN101012.RES

Instrument :
 HPLC_N
 LabSampleId :
 8330-CCV

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)
 Title : SW8330 / 8330A confirmation
 Last Update : Fri Nov 16 15:37:27 2012
 Response via : Initial Calibration
 DataAcq Meth : 8330VWDC.M

Volume Inj. :
 Signal Phase :
 Signal Info :

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
1) S	4-Nitroaniline	7.86f	9994688	966.029 ug/L
Target Compounds				
2) T	HMX	13.56	10297098	997.116 ug/L
3) T	RDX	11.15f	13807539	990.959 ug/L
4) T	1,3,5-Trinitrobenzene	26.00	14108480	506.271 ug/L
5) T	Tetryl	37.58	21435327	991.821 ug/L
6) T	2,4,6-Trinitrotoluene	35.36	13215076	492.139 ug/L
7) T	2-Amino-4,6-dinitrotoluene	17.04	23448225	502.254 ug/L
8) T	4-Amino-2,6-dinitrotoluene	17.04	23448225	502.254 ug/L
9) T	2,4-Dinitrotoluene	22.91	19252922	508.284 ug/L
10) T	2,6-Dinitrotoluene	21.41	9922644	505.908 ug/L
11) T	1,3-Dinitrobenzene	16.41	20313138	502.079 ug/L
12) T	Nitrobenzene	12.68f	13287132	508.682 ug/L
13) T	2-Nitrotoluene	17.52	16922789	1058.790 ug/L
14) T	3-Nitrotoluene	18.83	18126717	984.770 ug/L
15) T	4-Nitrotoluene	18.08	14198384	1040.374 ug/L
16) T	3,5-Dinitroaniline	14.26	33036950	987.948 ug/L

Quantitation Report

Data File : H:\VOL1\HPLC\HPLC N\121109\HN000578.D
 Acq On : 09-Nov-2012, 23:14
 Sample : 8330-CCV
 Misc :
 IntFile : events.e
 Quant Time: Nov 16 15:38 2012


Vial: 2
 Operator: HLM
 Inst : G1314A
 Multiplr: 1.00


Instrument :
 HPLC_N
 LabSampleId :
 8330-CCV

Quant Results File: HN101012.RES

Quant Method : H:\VOL1\HPLC\HPLC N\METHODS\HN101012.M (Chemstation Integrator)
 Title : SW8330 / 8330A confirmation
 Last Update : Fri Nov 16 15:37:27 2012
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330VWDC.M

Volume Inj. :
 Signal Phase :
 Signal Info :

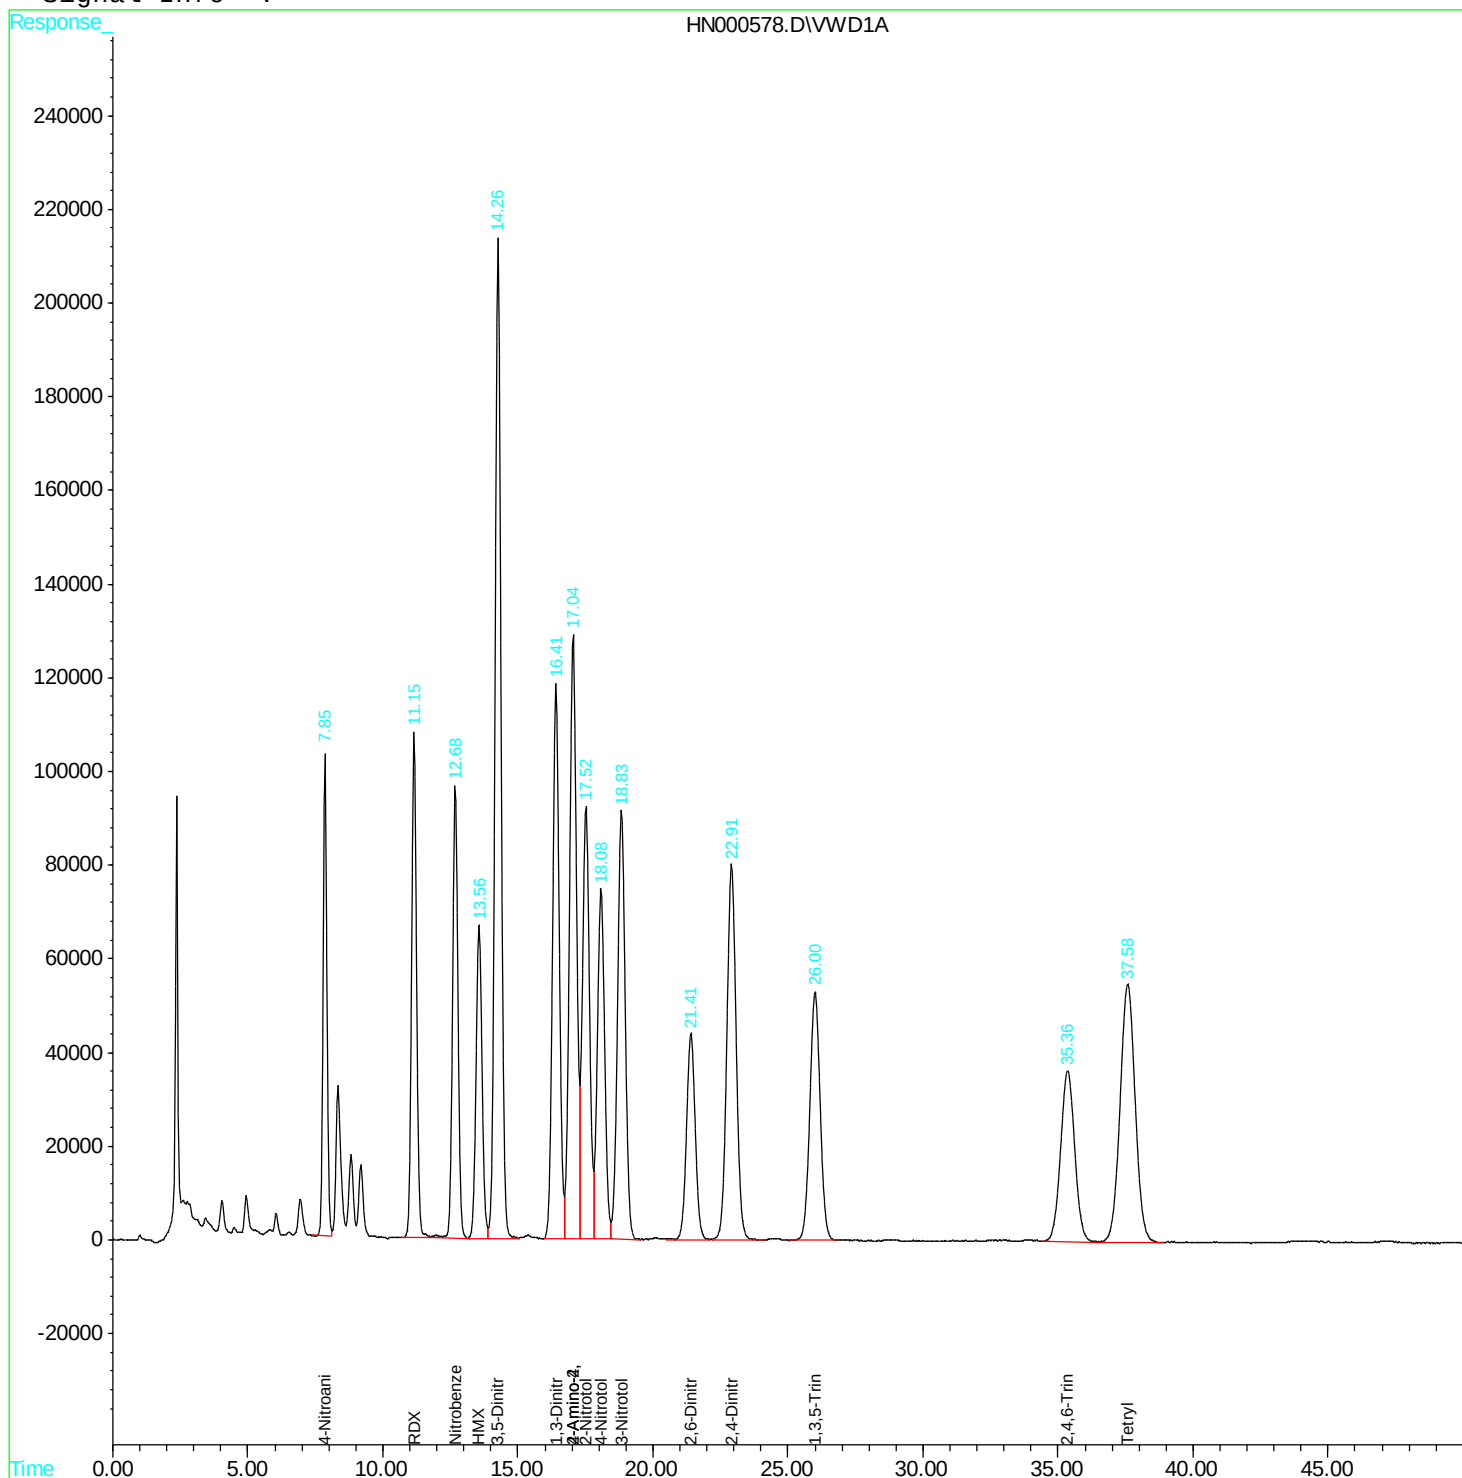


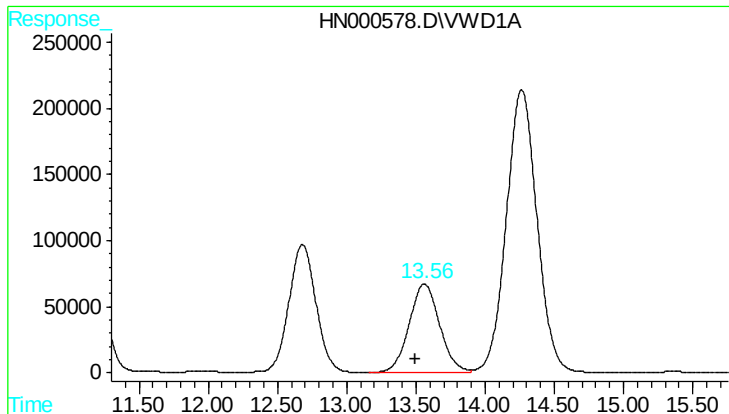

#2 HMX


R.T.: 13.560 min
Delta R.T.: 0.064 min
Response: 10297098
Conc: 997.12 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-CCV

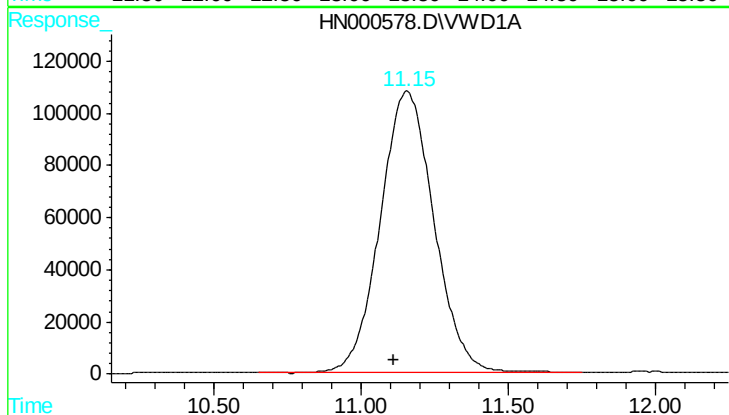


#3 RDX

R.T.: 11.155 min
Delta R.T.: 0.045 min
Response: 13807539
Conc: 990.96 ug/L

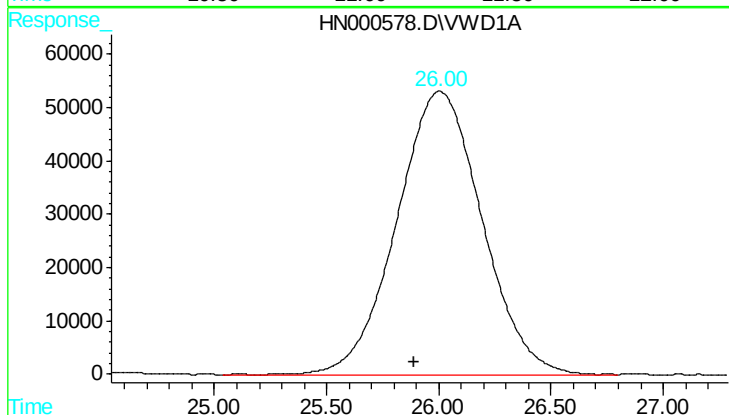


#4 1,3,5-Trinitrobenzene

R.T.: 26.003 min
Delta R.T.: 0.112 min
Response: 14108480
Conc: 506.27 ug/L

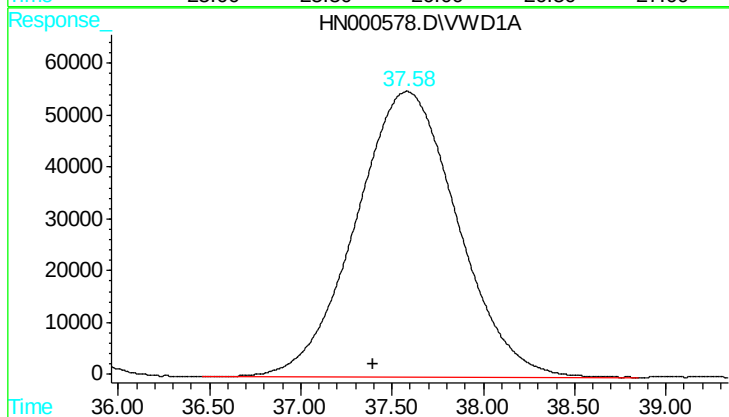

#5 Tetryl


R.T.: 37.581 min
Delta R.T.: 0.185 min
Response: 21435327
Conc: 991.82 ug/L

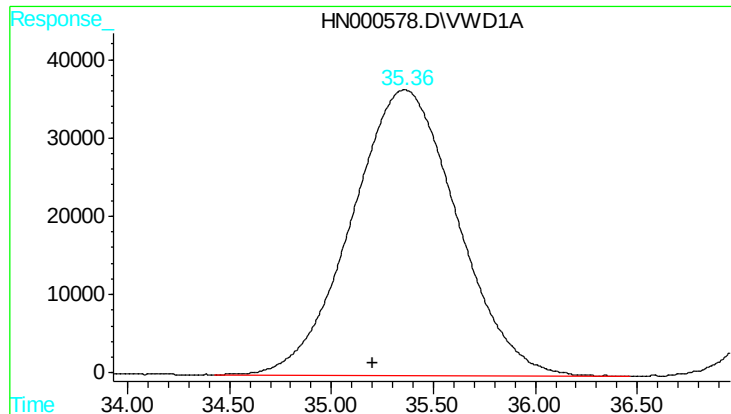

#6 2,4,6-Trinitrotoluene


R.T.: 35.358 min
Delta R.T.: 0.157 min
Response: 13215076
Conc: 492.14 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-CCV

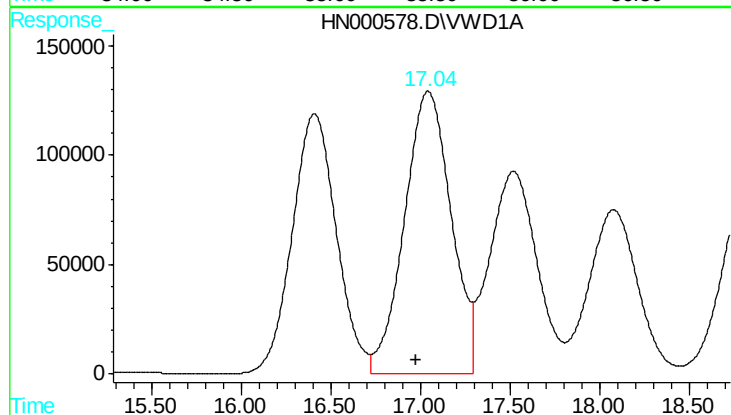


#7 2-Amino-4,6-dinitrotoluene

R.T.: 17.043 min
Delta R.T.: 0.070 min
Response: 23448225
Conc: 502.25 ug/L

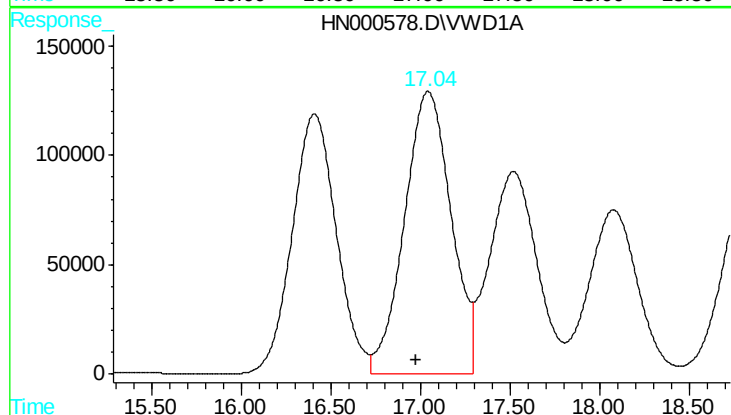


#8 4-Amino-2,6-dinitrotoluene

R.T.: 17.043 min
Delta R.T.: 0.070 min
Response: 23448225
Conc: 502.25 ug/L

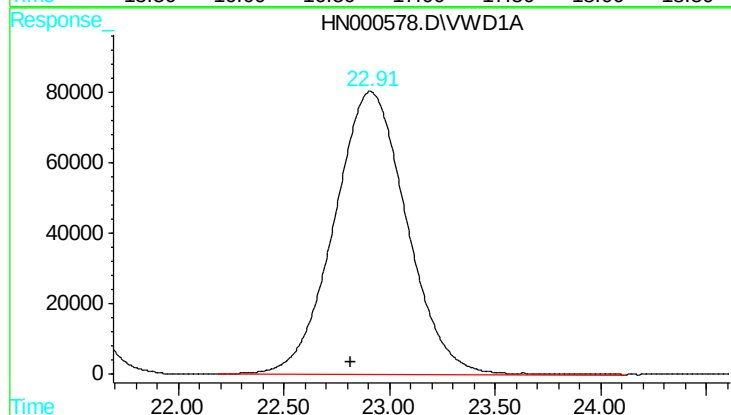

#9 2,4-Dinitrotoluene


R.T.: 22.910 min
Delta R.T.: 0.091 min
Response: 19252922
Conc: 508.28 ug/L

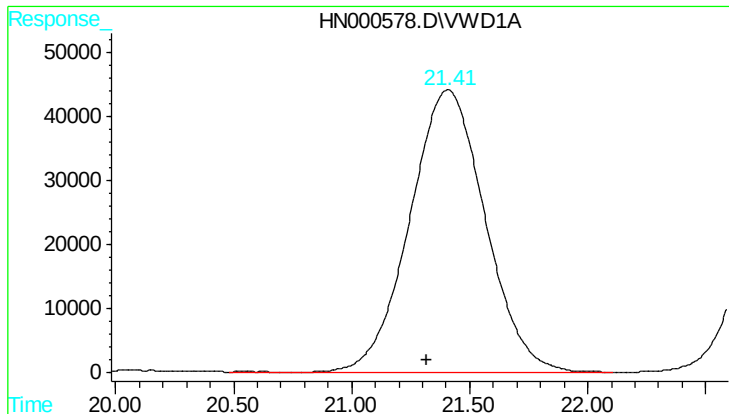

#10 2,6-Dinitrotoluene


R.T.: 21.408 min
Delta R.T.: 0.086 min
Response: 9922644
Conc: 505.91 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-CCV

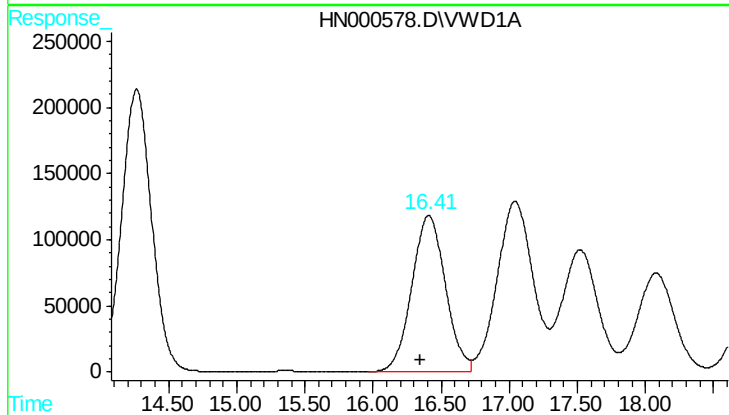


#11 1,3-Dinitrobenzene

R.T.: 16.409 min
Delta R.T.: 0.062 min
Response: 20313138
Conc: 502.08 ug/L

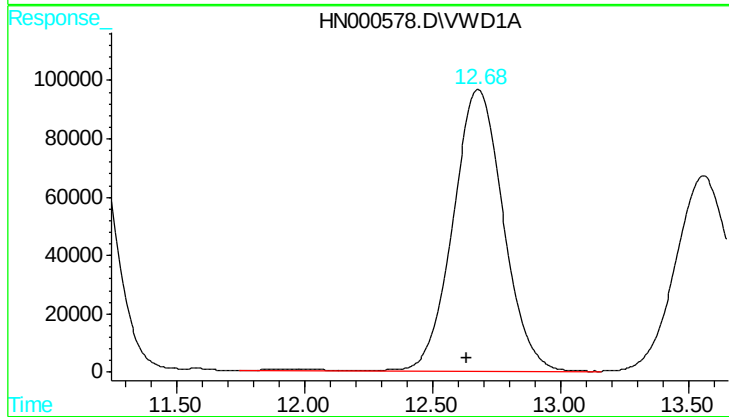


#12 Nitrobenzene

R.T.: 12.680 min
Delta R.T.: 0.044 min
Response: 13287132
Conc: 508.68 ug/L

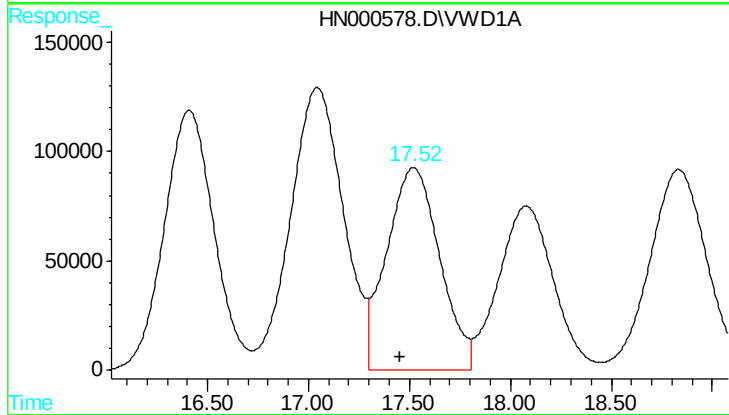

#13 2-Nitrotoluene


R.T.: 17.520 min
Delta R.T.: 0.063 min
Response: 16922789
Conc: 1058.79 ug/L

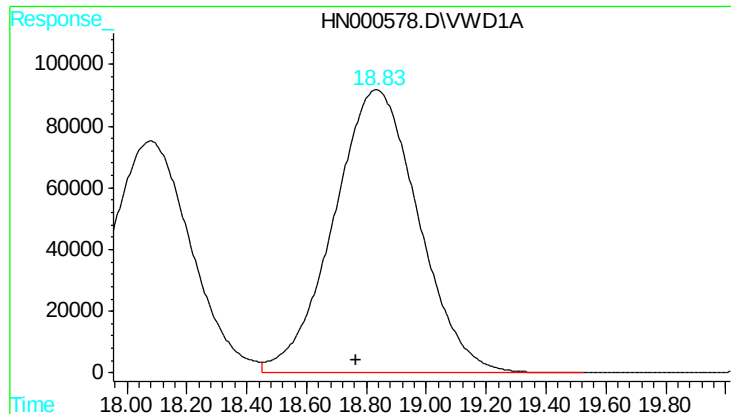

#14 3-Nitrotoluene


R.T.: 18.834 min
Delta R.T.: 0.067 min
Response: 18126717
Conc: 984.77 ug/L

Instrument :
HPLC_N
LabSampleId :
8330-CCV

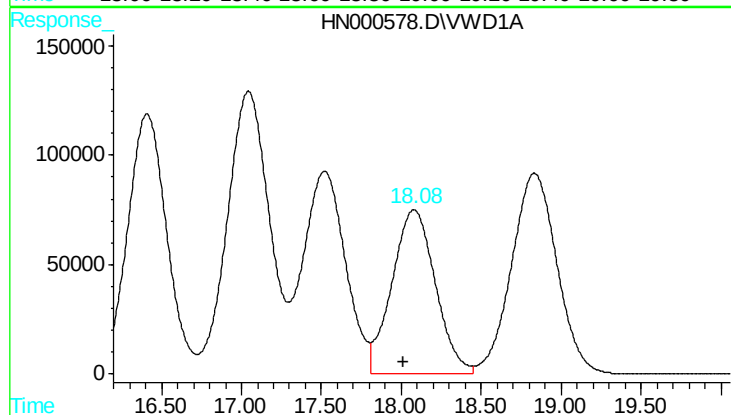

#15 4-Nitrotoluene

R.T.: 18.079 min
Delta R.T.: 0.063 min
Response: 14198384
Conc: 1040.37 ug/L

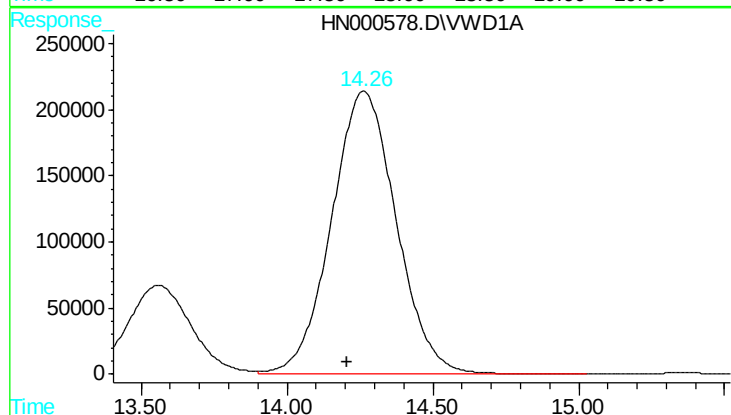

#16 3,5-Dinitroaniline

R.T.: 14.264 min
Delta R.T.: 0.058 min
Response: 33036950
Conc: 987.95 ug/L