

Data Path : S:\HPCHEM1\HPLC_N\Data\HN110912\
 Data File : HN000575.D
 Signal(s) : VWD1A.CH
 Acq On : 09-Nov-2012, 20:37
 Operator : HLM
 Sample : D4671-01RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 871RE

Integration File: events.e
 Quant Time: Nov 17 04:43:53 2012
 Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Fri Nov 16 15:37:27 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	7.851f	1585841	153.278 ug/L
Target Compounds			
3) T RDX	11.141	4670814	335.222 ug/L
4) T 1,3,5-Trinitrobenzene	25.965	16421080	589.256 ug/L
6) T 2,4,6-Trinitrotoluene	35.299	14152114	527.035 ug/L
7) T 2-Amino-4,6-dinitroto...	17.021	54001991	1156.708 ug/L
8) T 4-Amino-2,6-dinitroto...	17.021	54001991	1156.708 ug/L
9) T 2,4-Dinitrotoluene	22.885	102019621	2693.357 ug/L
10) T 2,6-Dinitrotoluene	21.382	27988386	1426.995 ug/L
11) T 1,3-Dinitrobenzene	16.370	206800	5.111 ug/L m
12) T Nitrobenzene	12.670	13510491	517.233 ug/L
13) T 2-Nitrotoluene	17.505	34799712	2177.276 ug/L
14) T 3-Nitrotoluene	18.818	39209389	2142.348 ug/L
15) T 4-Nitrotoluene	18.063	32142933	2355.246 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN110912\
Data File : HN000575.D
Signal(s) : VWD1A.CH
Acq On : 09-Nov-2012, 20:37
Operator : HLM
Sample : D4671-01RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
871RE

Integration File: events.e
Quant Time: Nov 17 04:43:53 2012
Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Fri Nov 16 15:37:27 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

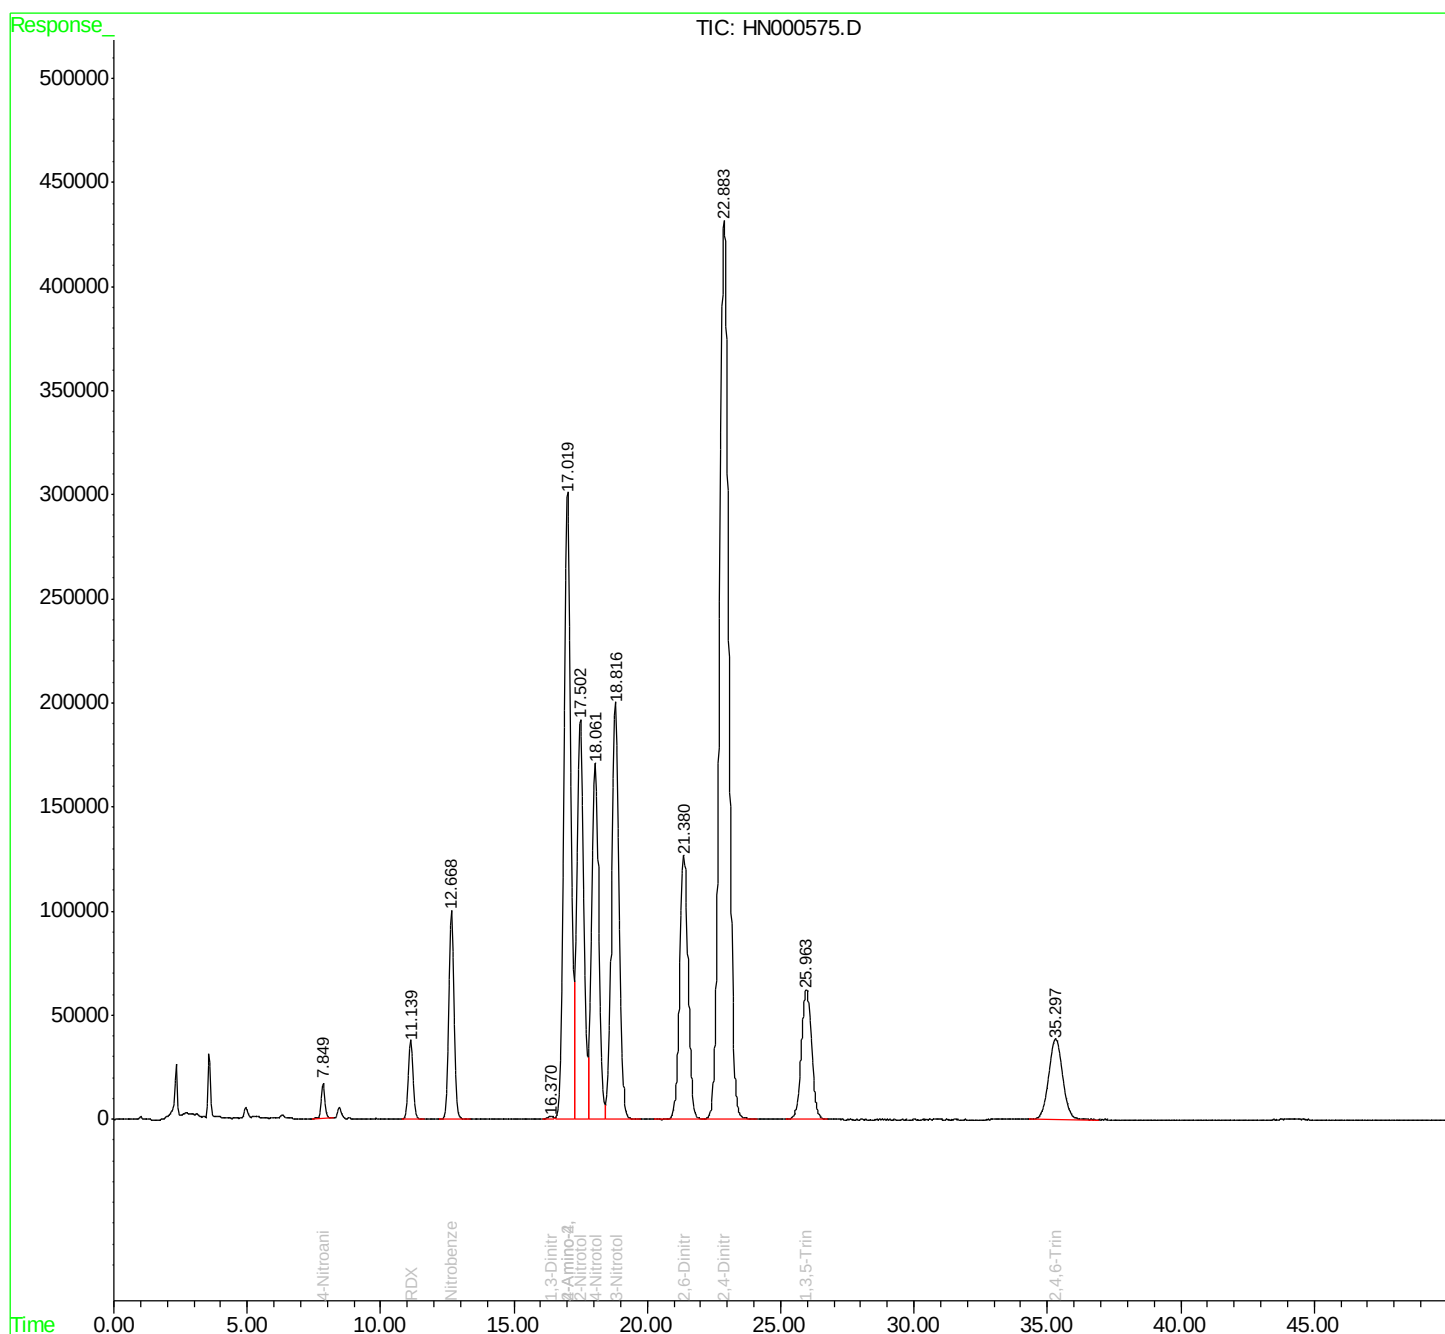


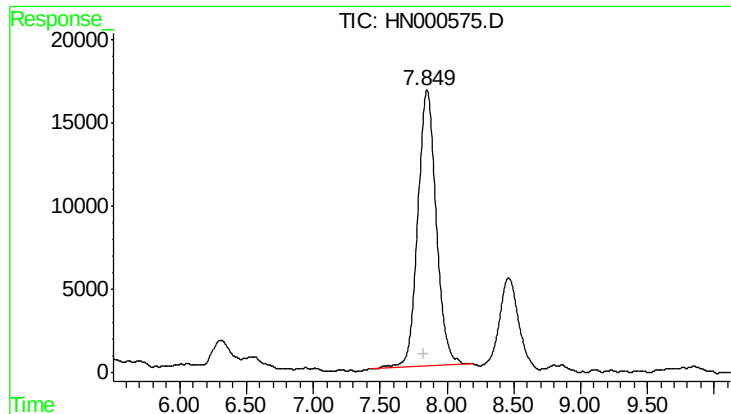

#1 4-Nitroaniline


R.T.: 7.851 min
Delta R.T.: 0.023 min
Response: 1585841
Conc: 153.28 ug/L

Instrument :
HPLC_N
ClientSampleId :
871RE

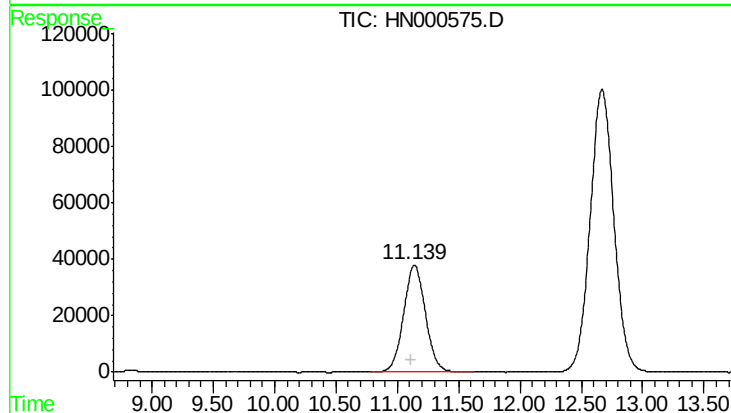


#3 RDX

R.T.: 11.141 min
Delta R.T.: 0.031 min
Response: 4670814
Conc: 335.22 ug/L

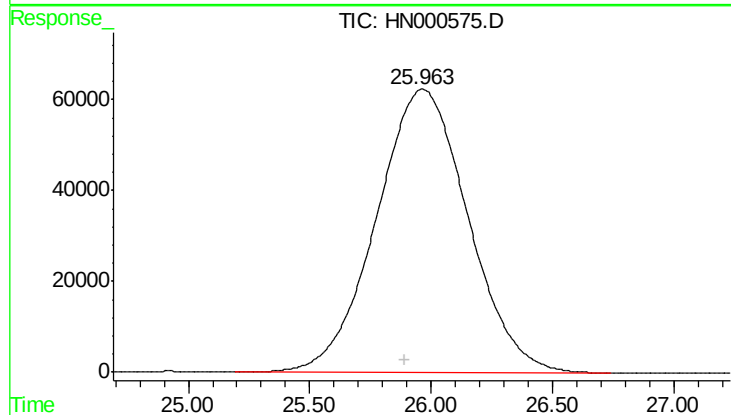


#4 1,3,5-Trinitrobenzene

R.T.: 25.965 min
Delta R.T.: 0.073 min
Response: 16421080
Conc: 589.26 ug/L

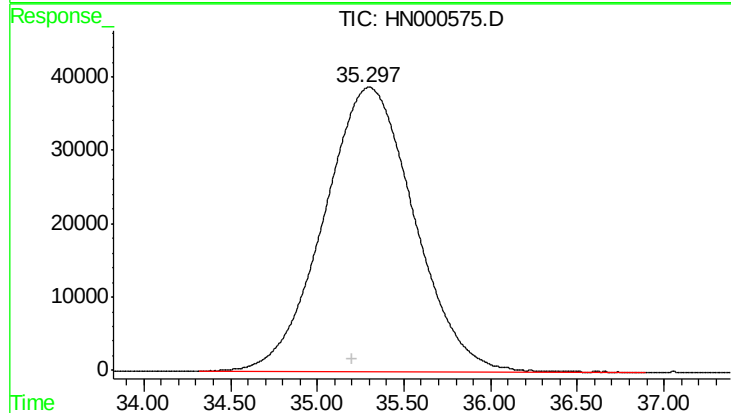

#6 2,4,6-Trinitrotoluene


R.T.: 35.299 min
Delta R.T.: 0.098 min
Response: 14152114
Conc: 527.04 ug/L

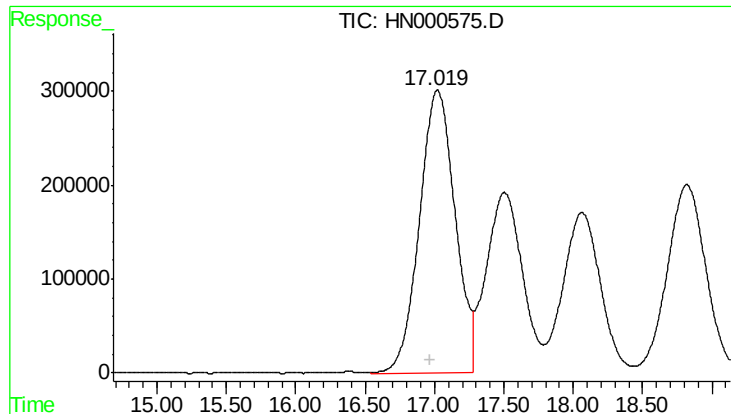

#7 2-Amino-4,6-dinitrotoluene


R.T.: 17.021 min
Delta R.T.: 0.048 min
Response: 54001991
Conc: 1156.71 ug/L

Instrument :
HPLC_N
ClientSampleId :
871RE

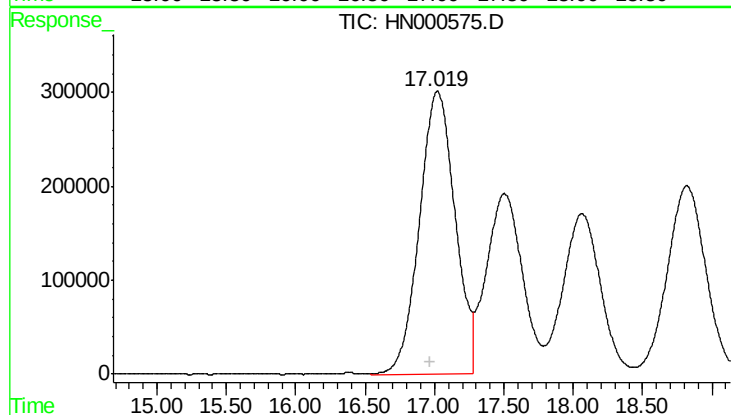


#8 4-Amino-2,6-dinitrotoluene

R.T.: 17.021 min
Delta R.T.: 0.048 min
Response: 54001991
Conc: 1156.71 ug/L

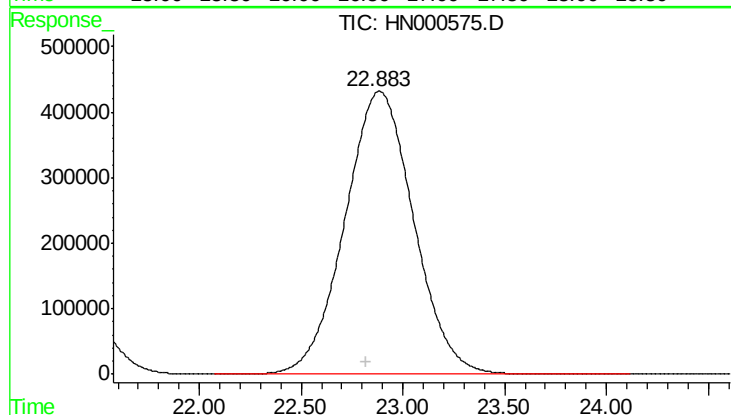


#9 2,4-Dinitrotoluene

R.T.: 22.885 min
Delta R.T.: 0.066 min
Response: 102019621
Conc: 2693.36 ug/L

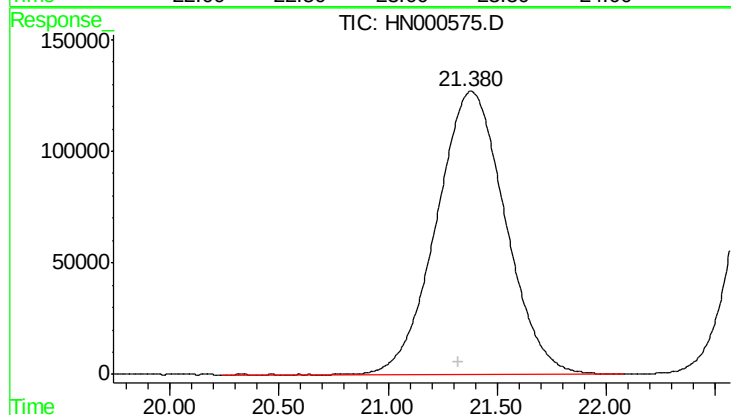

#10 2,6-Dinitrotoluene


R.T.: 21.382 min
Delta R.T.: 0.061 min
Response: 27988386
Conc: 1426.99 ug/L

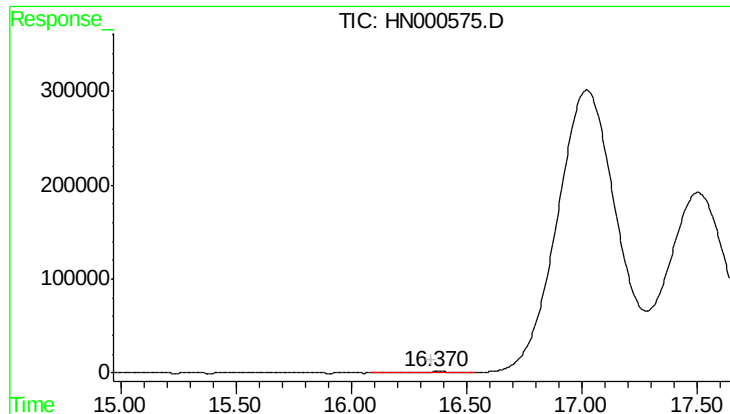

#11 1,3-Dinitrobenzene


R.T.: 16.370 min
Delta R.T.: 0.023 min
Response: 206800
Conc: 5.11 ug/L m

Instrument :
HPLC_N
ClientSampleId :
871RE

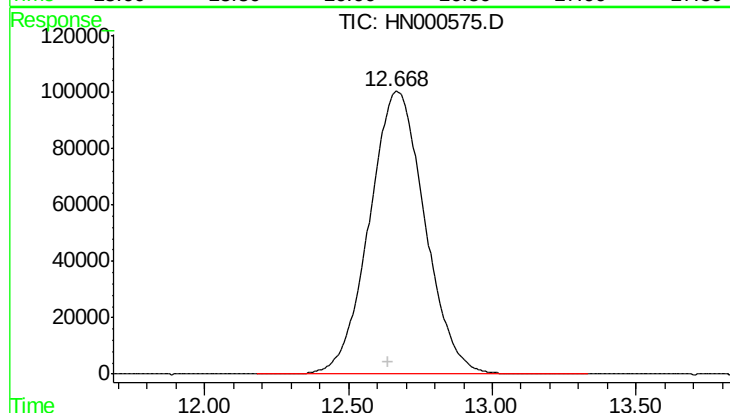


#12 Nitrobenzene

R.T.: 12.670 min
Delta R.T.: 0.034 min
Response: 13510491
Conc: 517.23 ug/L

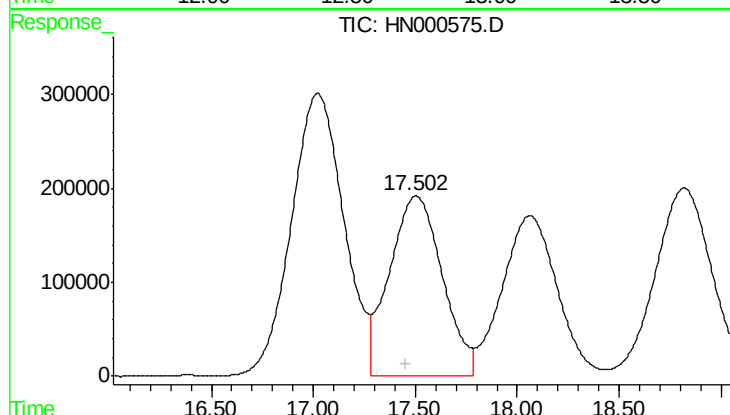


#13 2-Nitrotoluene

R.T.: 17.505 min
Delta R.T.: 0.048 min
Response: 34799712
Conc: 2177.28 ug/L

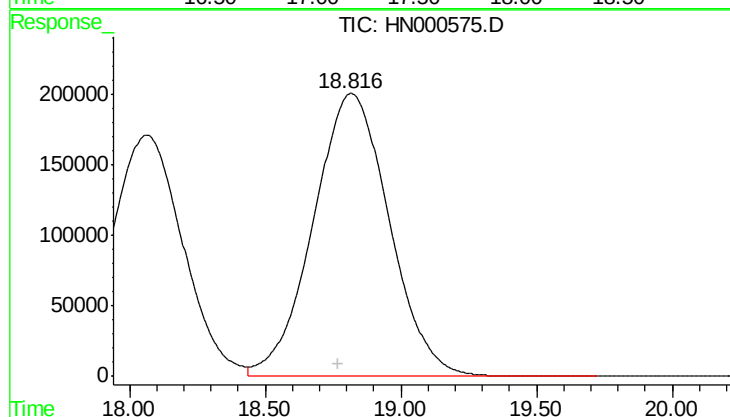

#14 3-Nitrotoluene

R.T.: 18.818 min
Delta R.T.: 0.051 min
Response: 39209389
Conc: 2142.35 ug/L

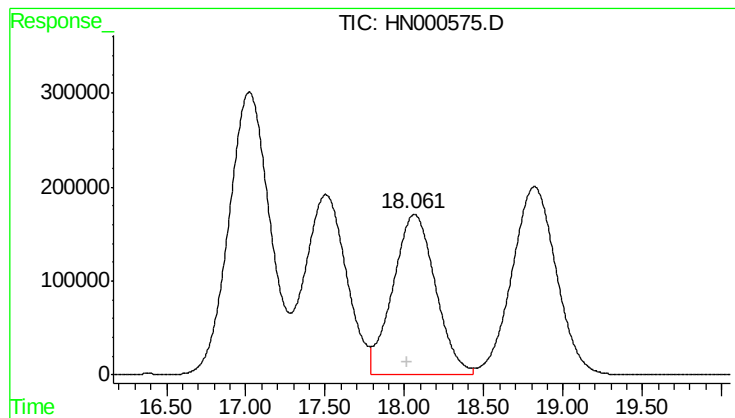

#15 4-Nitrotoluene

R.T.: 18.063 min
Delta R.T.: 0.048 min
Response: 32142933
Conc: 2355.25 ug/L

Instrument :
HPLC_N
ClientSampleId :
871RE