

Data Path : S:\HPCHEM1\HPLC_N\Data\HN110912\
 Data File : HN000576.D
 Signal(s) : VWD1A.CH
 Acq On : 09-Nov-2012, 21:29
 Operator : HLM
 Sample : D4671-03RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 871RE

Integration File: events.e
 Quant Time: Nov 17 04:43:59 2012
 Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
 Quant Title : SW8330 / 8330A confirmation
 QLast Update : Fri Nov 16 15:37:27 2012
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. :
 Signal Phase :
 Signal Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	7.857f	1477464	142.803 ug/L
Target Compounds			
3) T RDX	11.153f	4488265	322.120 ug/L
4) T 1,3,5-Trinitrobenzene	25.989	15543652	557.771 ug/L
6) T 2,4,6-Trinitrotoluene	35.330	13143614	489.478 ug/L
7) T 2-Amino-4,6-dinitroto...	17.039	51083675	1094.198 ug/L
8) T 4-Amino-2,6-dinitroto...	17.039	51083675	1094.198 ug/L
9) T 2,4-Dinitrotoluene	22.906	96171855	2538.974 ug/L
10) T 2,6-Dinitrotoluene	21.402	26410181	1346.529 ug/L
11) T 1,3-Dinitrobenzene	16.406	178999	4.424 ug/L m
12) T Nitrobenzene	12.681f	12760197	488.509 ug/L
13) T 2-Nitrotoluene	17.519	32886090	2057.549 ug/L
14) T 3-Nitrotoluene	18.834	37008842	2021.524 ug/L
15) T 4-Nitrotoluene	18.078	30325647	2222.086 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : S:\HPCHEM1\HPLC_N\Data\HN110912\
Data File : HN000576.D
Signal(s) : VWD1A.CH
Acq On : 09-Nov-2012, 21:29
Operator : HLM
Sample : D4671-03RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
871RE

Integration File: events.e
Quant Time: Nov 17 04:43:59 2012
Quant Method : H:\VOL1\HPLC\HPLC_N\METHODS\HN101012.M
Quant Title : SW8330 / 8330A confirmation
QLast Update : Fri Nov 16 15:37:27 2012
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. :
Signal Phase :
Signal Info :

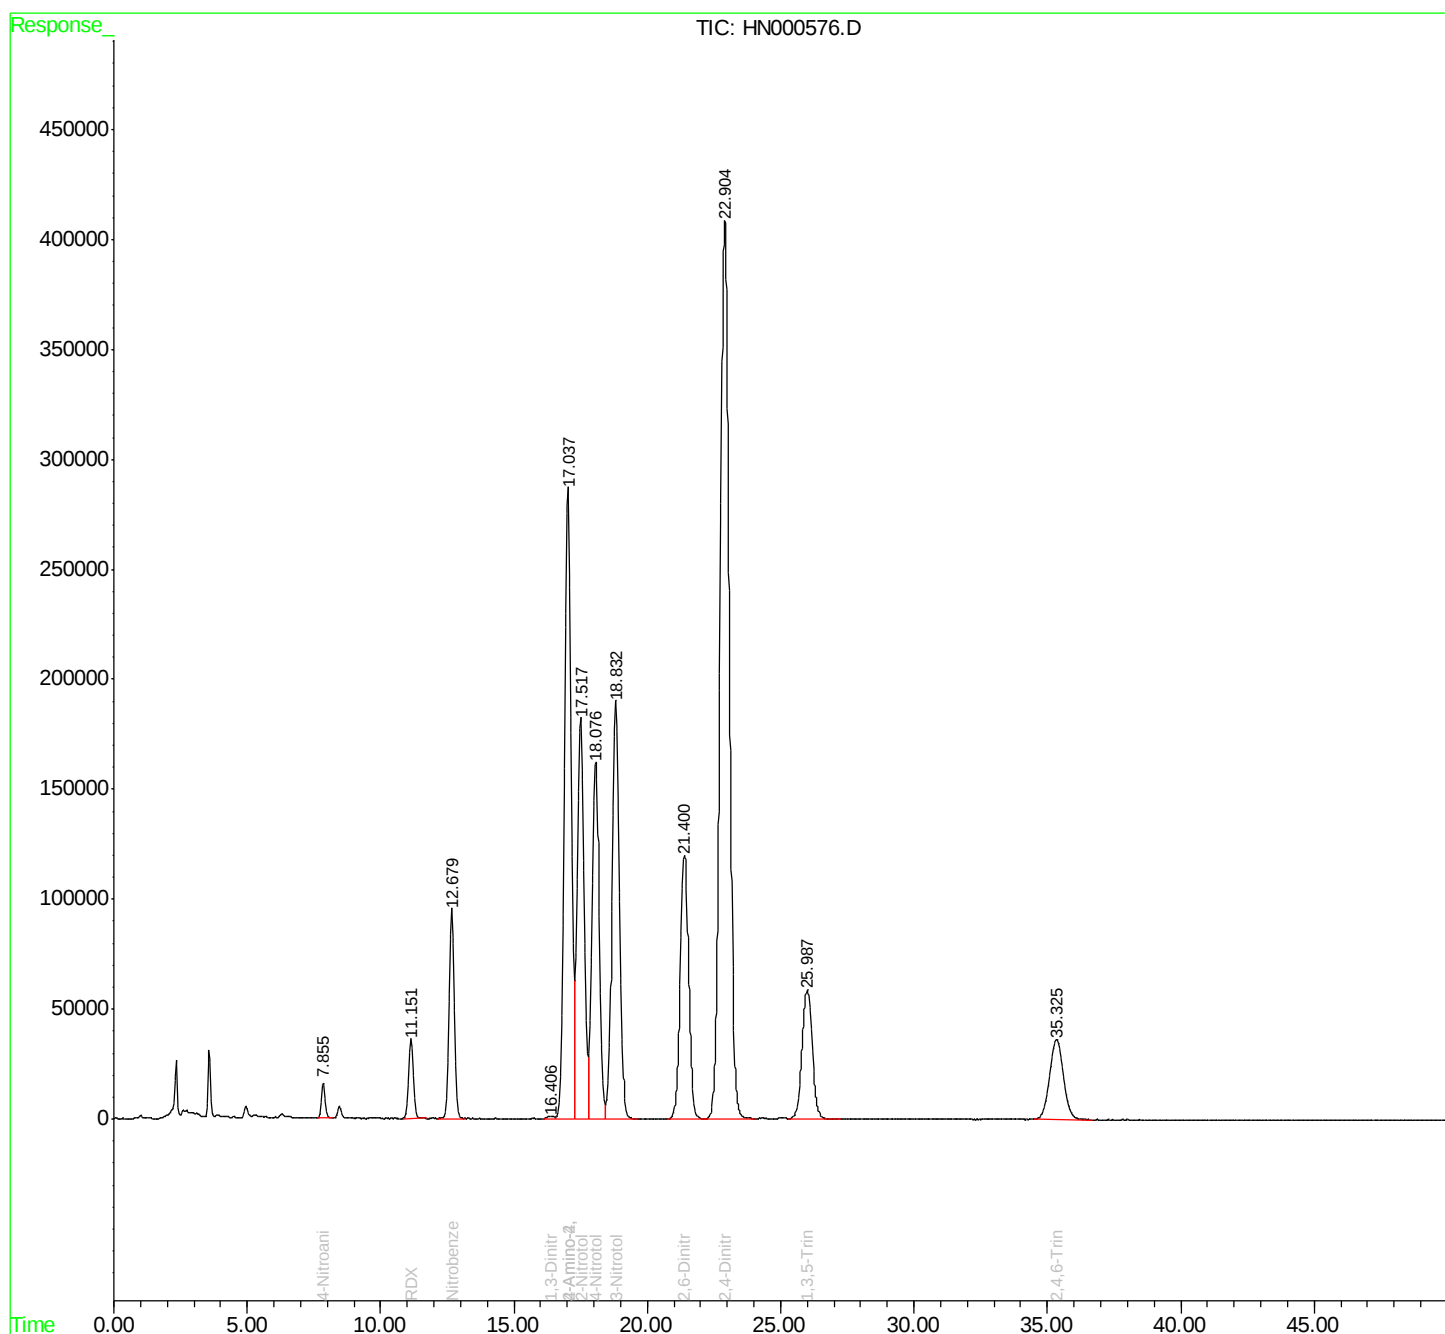


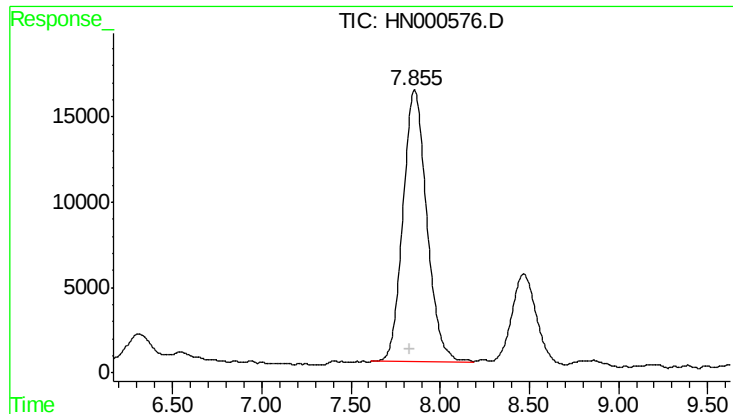

#1 4-Nitroaniline


R.T.: 7.857 min
Delta R.T.: 0.029 min
Response: 1477464
Conc: 142.80 ug/L

Instrument :
HPLC_N
ClientSampleId :
871RE

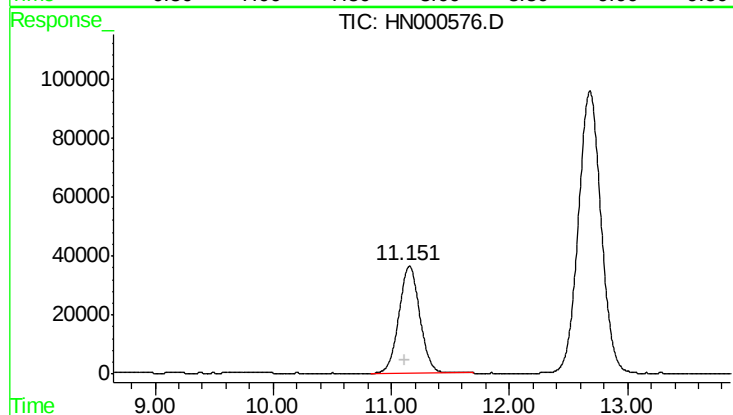


#3 RDX

R.T.: 11.153 min
Delta R.T.: 0.043 min
Response: 4488265
Conc: 322.12 ug/L

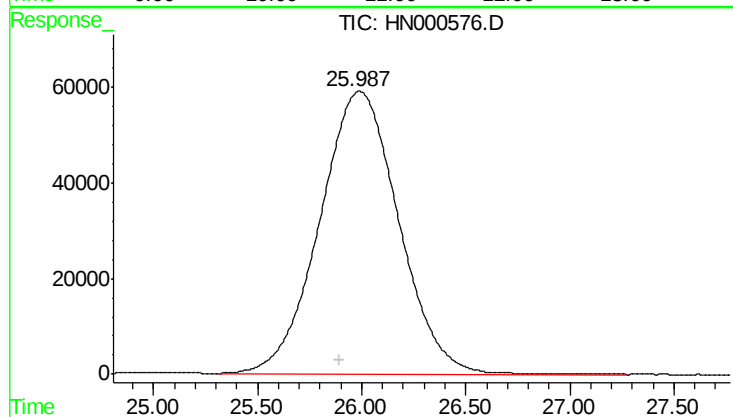


#4 1,3,5-Trinitrobenzene

R.T.: 25.989 min
Delta R.T.: 0.098 min
Response: 15543652
Conc: 557.77 ug/L

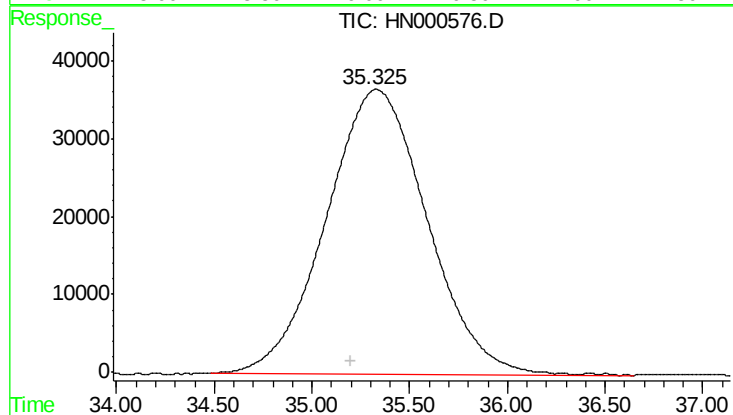

#6 2,4,6-Trinitrotoluene


R.T.: 35.330 min
Delta R.T.: 0.129 min
Response: 13143614
Conc: 489.48 ug/L

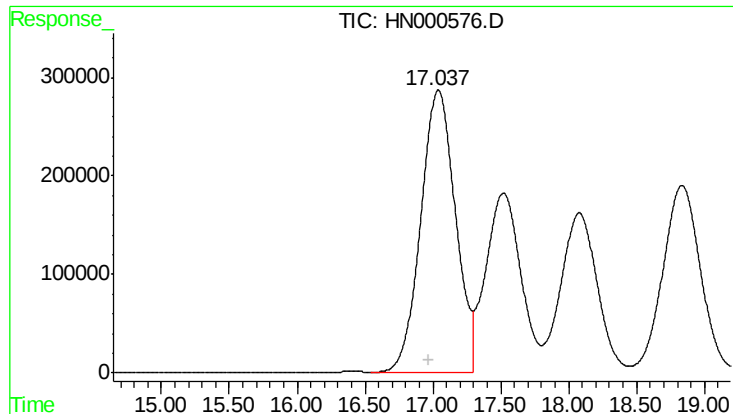

#7 2-Amino-4,6-dinitrotoluene


R.T.: 17.039 min
Delta R.T.: 0.066 min
Response: 51083675
Conc: 1094.20 ug/L

Instrument :
HPLC_N
ClientSampleId :
871RE

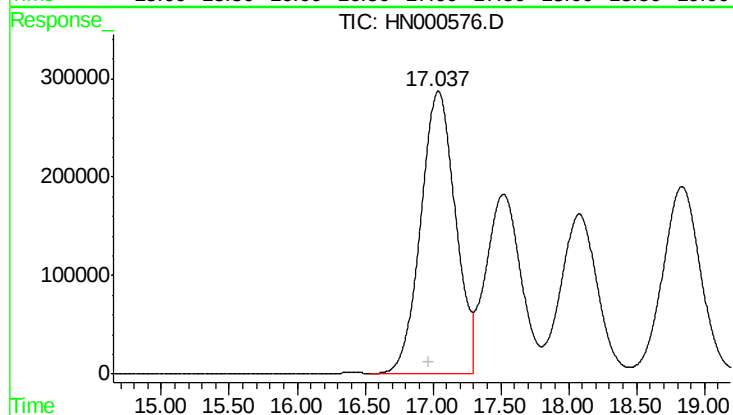


#8 4-Amino-2,6-dinitrotoluene

R.T.: 17.039 min
Delta R.T.: 0.066 min
Response: 51083675
Conc: 1094.20 ug/L

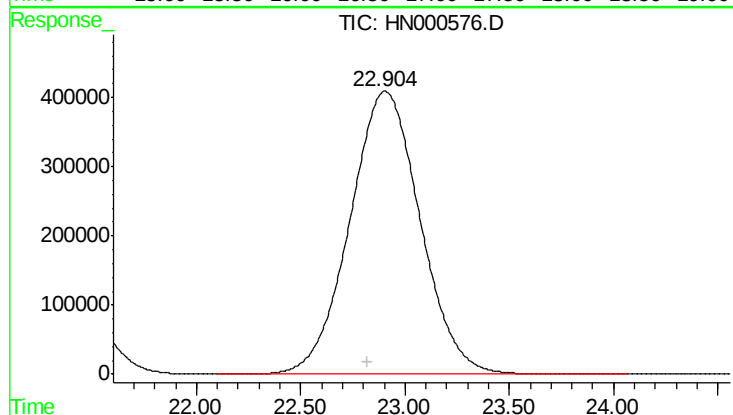


#9 2,4-Dinitrotoluene

R.T.: 22.906 min
Delta R.T.: 0.086 min
Response: 96171855
Conc: 2538.97 ug/L

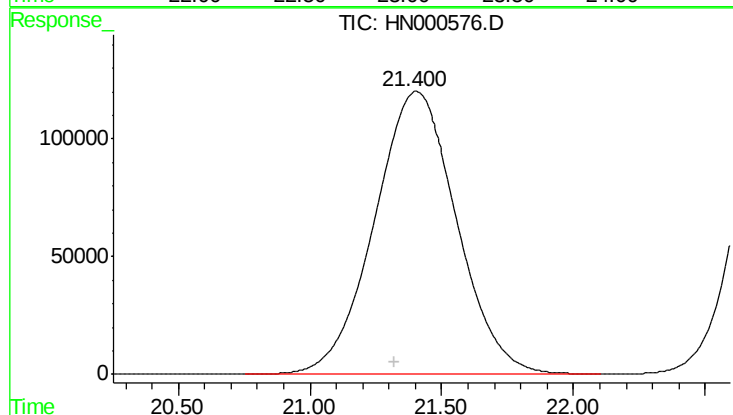

#10 2,6-Dinitrotoluene


R.T.: 21.402 min
Delta R.T.: 0.080 min
Response: 26410181
Conc: 1346.53 ug/L

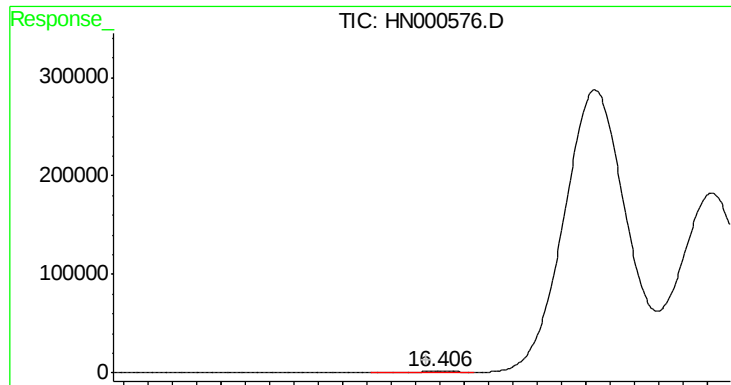

#11 1,3-Dinitrobenzene


R.T.: 16.406 min
Delta R.T.: 0.059 min
Response: 178999
Conc: 4.42 ug/L

Instrument :
HPLC_N
ClientSampleId :
871RE

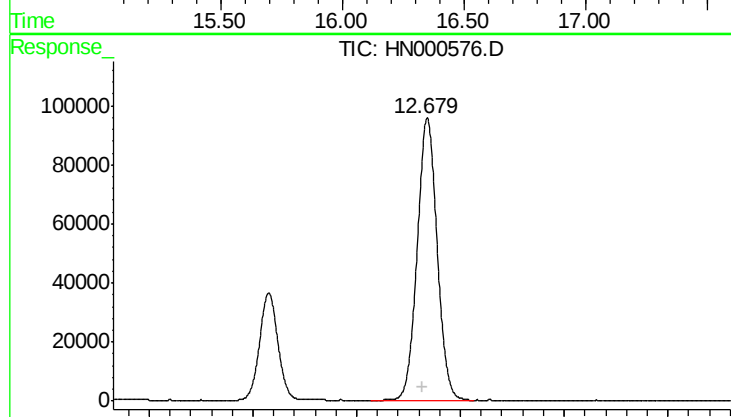


#12 Nitrobenzene

R.T.: 12.681 min
Delta R.T.: 0.045 min
Response: 12760197
Conc: 488.51 ug/L

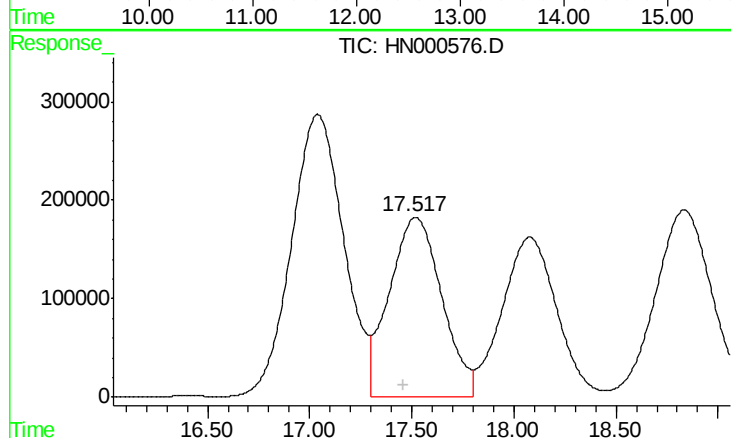


#13 2-Nitrotoluene

R.T.: 17.519 min
Delta R.T.: 0.062 min
Response: 32886090
Conc: 2057.55 ug/L

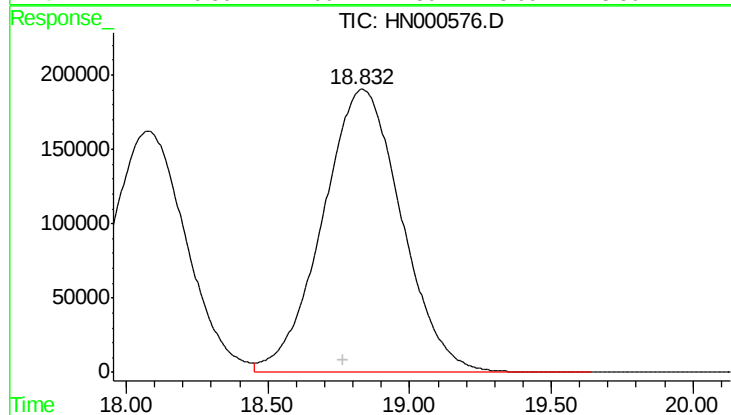

#14 3-Nitrotoluene

R.T.: 18.834 min
Delta R.T.: 0.067 min
Response: 37008842
Conc: 2021.52 ug/L

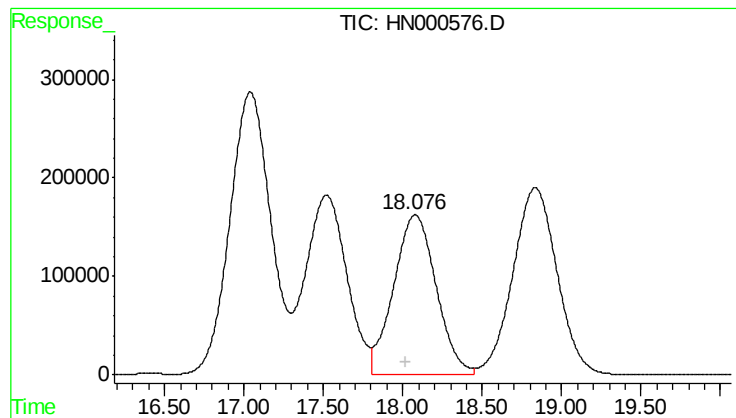

#15 4-Nitrotoluene

R.T.: 18.078 min
Delta R.T.: 0.063 min
Response: 30325647
Conc: 2222.09 ug/L

Instrument :
HPLC_N
ClientSampleId :
871RE