

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN111014\HN007069.D\VWD1A.CH Vial: 34
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN111014\HN007069.D\VWD1A.CH
 Acq On : 10-Nov-2014, 13:13 Operator: TP
 Sample : HSTDCCC005 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Nov 11 2:20 2014 Quant Results File: HN1029NG.RES

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1029NG.M
 Title :
 Last Update : Fri Oct 31 04:41:35 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	18379828	4.991 ng/ul
Target Compounds			
2) T Nitroglycerin	6.01	39171390	5.079 ng/ul

 Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN007069.D HN1029NG.M Tue Nov 11 02:17:32 2014



Quantitation Report


Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN111014\HN007069.D\VWD1A.CH Vial: 34
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN111014\HN007069.D\VWD1A.CH
 Acq On : 10-Nov-2014, 13:13 Operator: TP
 Sample : HSTDCCC005 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Nov 11 2:20 2014 Quant Results File: HN1029NG.RES

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1029NG.M
 Title :
 Last Update : Fri Oct 31 04:41:35 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

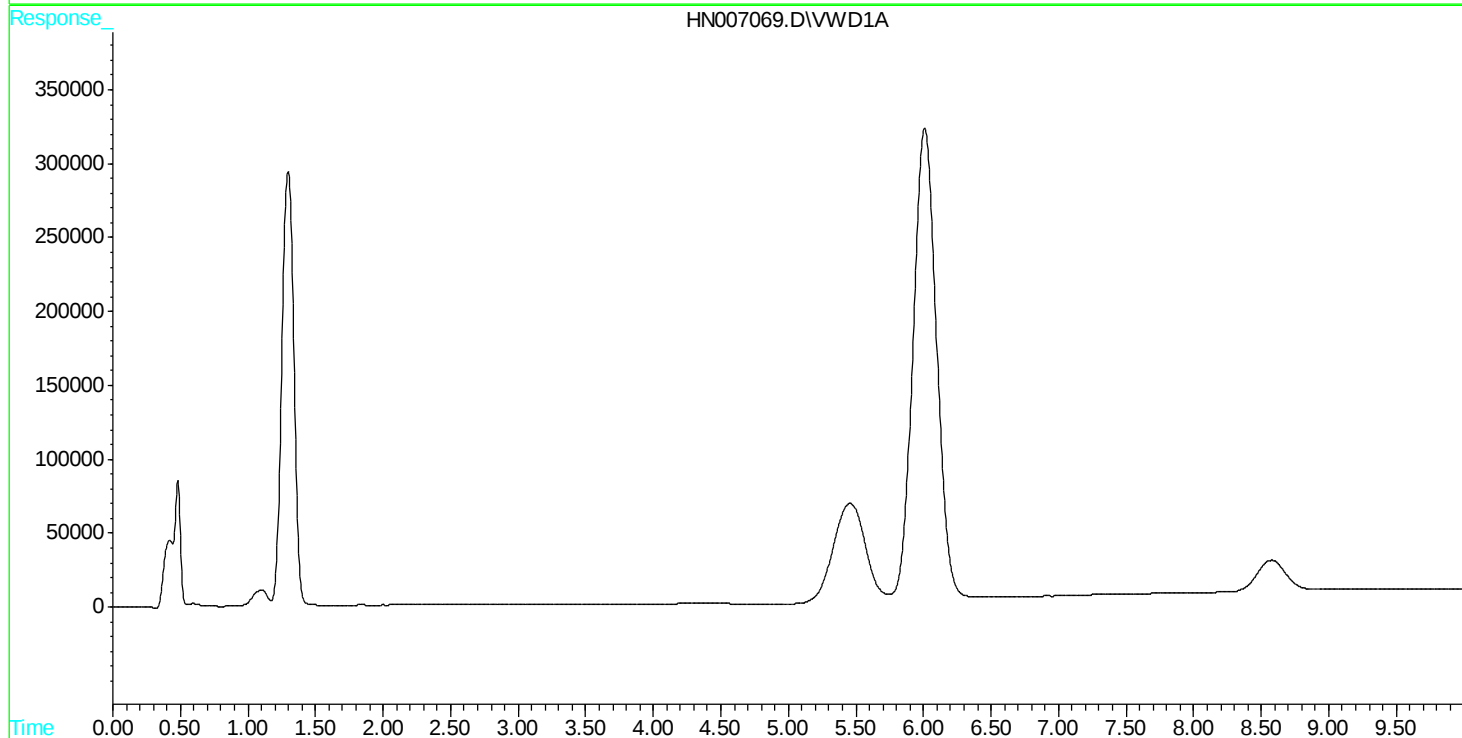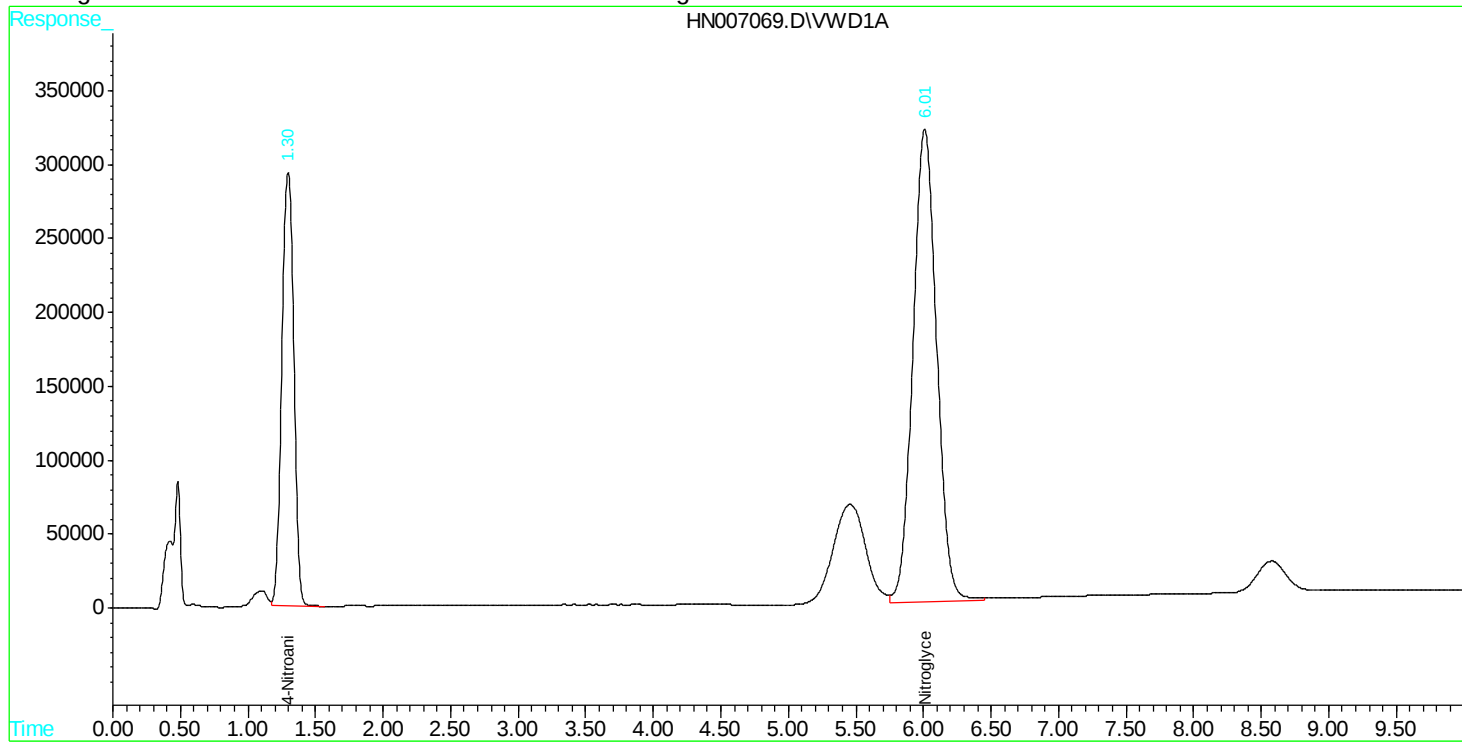


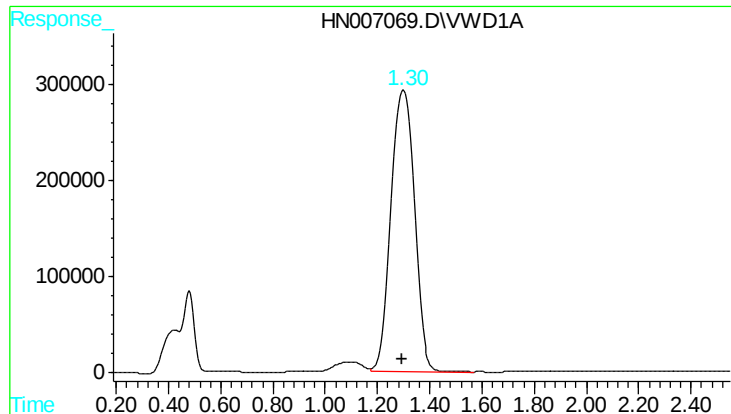

#1 4-Nitroaniline

R.T.: 1.298 min
Delta R.T.: 0.002 min
Response: 18379828
Conc: 4.99 ng/u1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC005

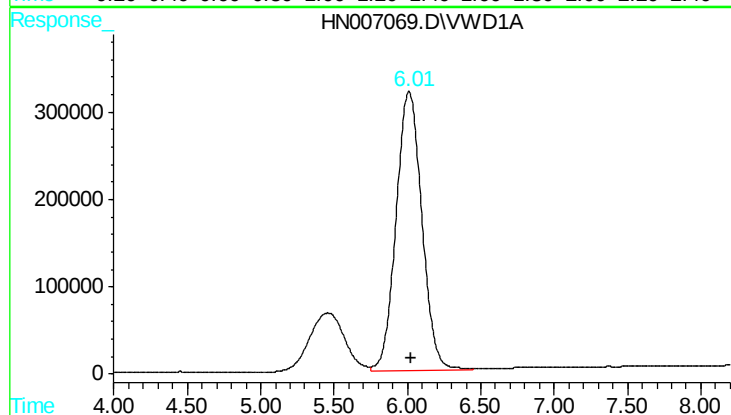

#2 Nitroglycerin

R.T.: 6.010 min
Delta R.T.: -0.011 min
Response: 39171390
Conc: 5.08 ng/u1