

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN111014\HN007090.D Vial: 34
Acq On : 10-Nov-2014, 19:19 Operator: TP
Sample : HSTDCCC005 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 11 2:21 2014 Quant Results File: HN1029NG.RES

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1029NG.M
Title :
Last Update : Fri Oct 31 04:50:16 2014
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

2) T Nitroglycerin	6.00	26423	0.003 ng/ul
--------------------	------	-------	-------------

Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.


HN007090.D HN1029NG.M Tue Nov 11 02:18:47 2014


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN111014\HN007090.D Vial: 34
Acq On : 10-Nov-2014, 19:19 Operator: TP
Sample : HSTDCCC005 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 11 2:21 2014 Quant Results File: HN1029NG.RES

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1029NG.M
Title :
Last Update : Fri Oct 31 04:50:16 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

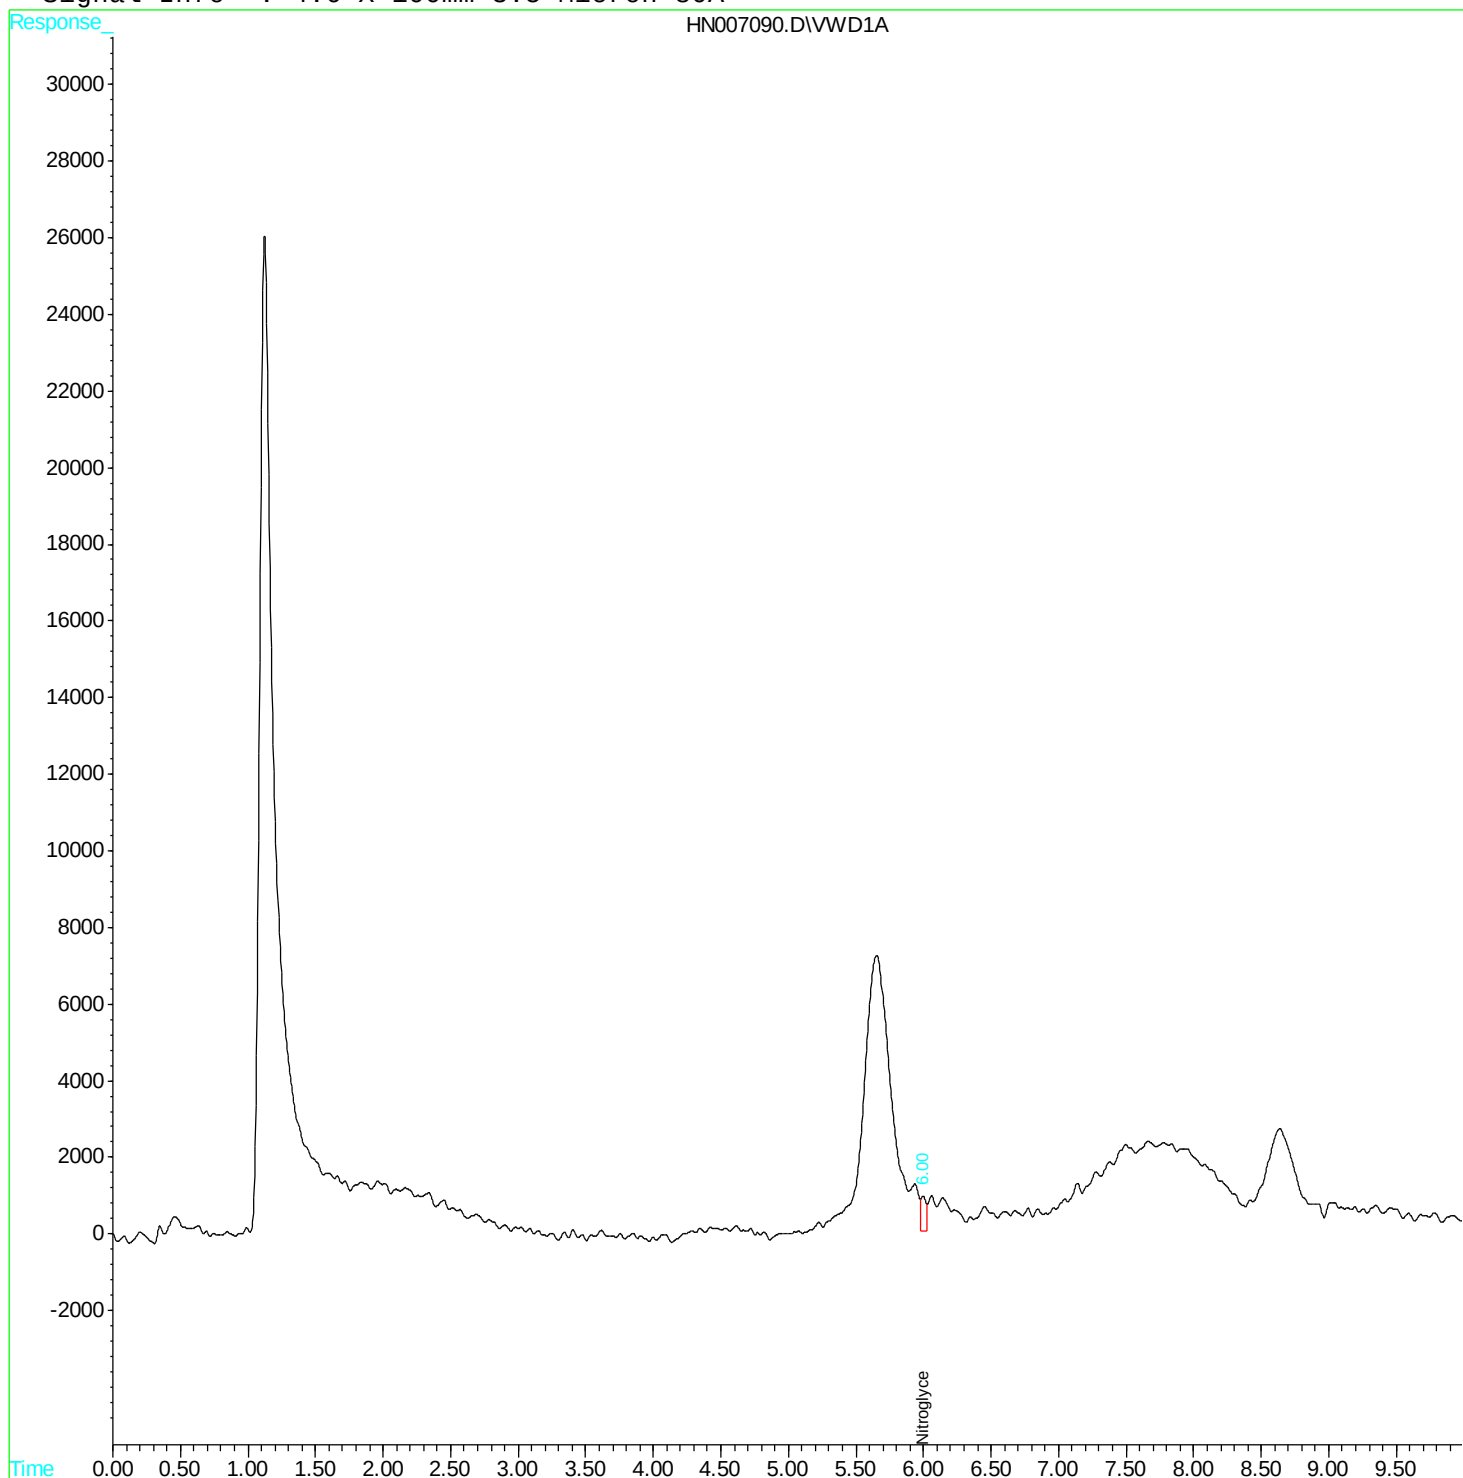


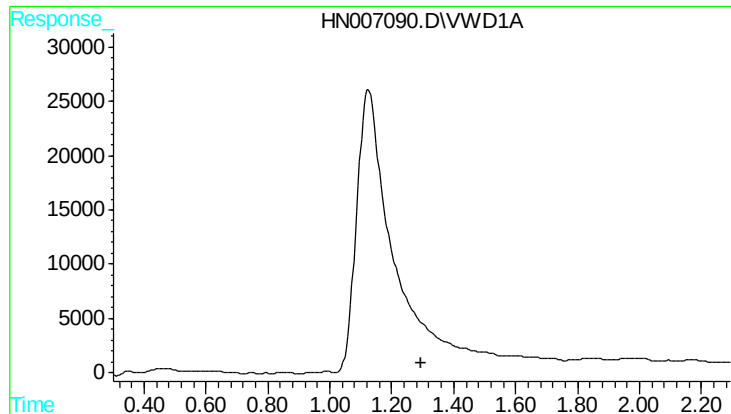

#1 4-Nitroaniline

R.T.: 0.000 min
Exp R.T.: 1.296 min
Response: 0
Conc: N.D.

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC005

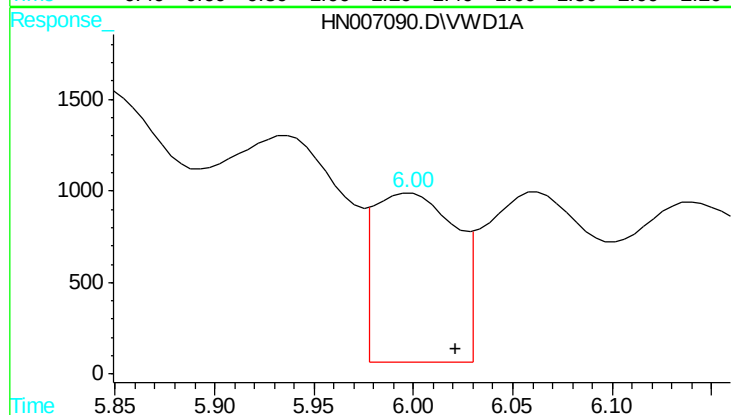

#2 Nitroglycerin

R.T.: 5.998 min
Delta R.T.: -0.023 min
Response: 26423
Conc: 0.00 ng/ul