

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN111113\HN005696.D Vial: 21
Acq On : 11-Nov-2013, 18:45 Operator: QM
Sample : PB73038BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Nov 12 10:21 2013 Quant Results File: HN111113.RES

Instrument :
HPLC_N
ClientSampleId :
PB73038BL

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN111113.M
Title :
Last Update : Mon Nov 11 16:27:41 2013
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.37	1159111	295.593 ug/L

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005696.D HN111113.M

Tue Nov 12 15:22:31 2013

RPT1


Quantitation Report


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN111113\HN005696.D Vial: 21
Acq On : 11-Nov-2013, 18:45 Operator: QM
Sample : PB73038BL Inst : G1314A
Misc : Multiplr: 1.00
IntFile : autoint1.e
Quant Time: Nov 12 10:21 2013 Quant Results File: HN111113.RES

Instrument :
HPLC_N
ClientSampleId :
PB73038BL

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN111113.M
Title :
Last Update : Mon Nov 11 16:27:41 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

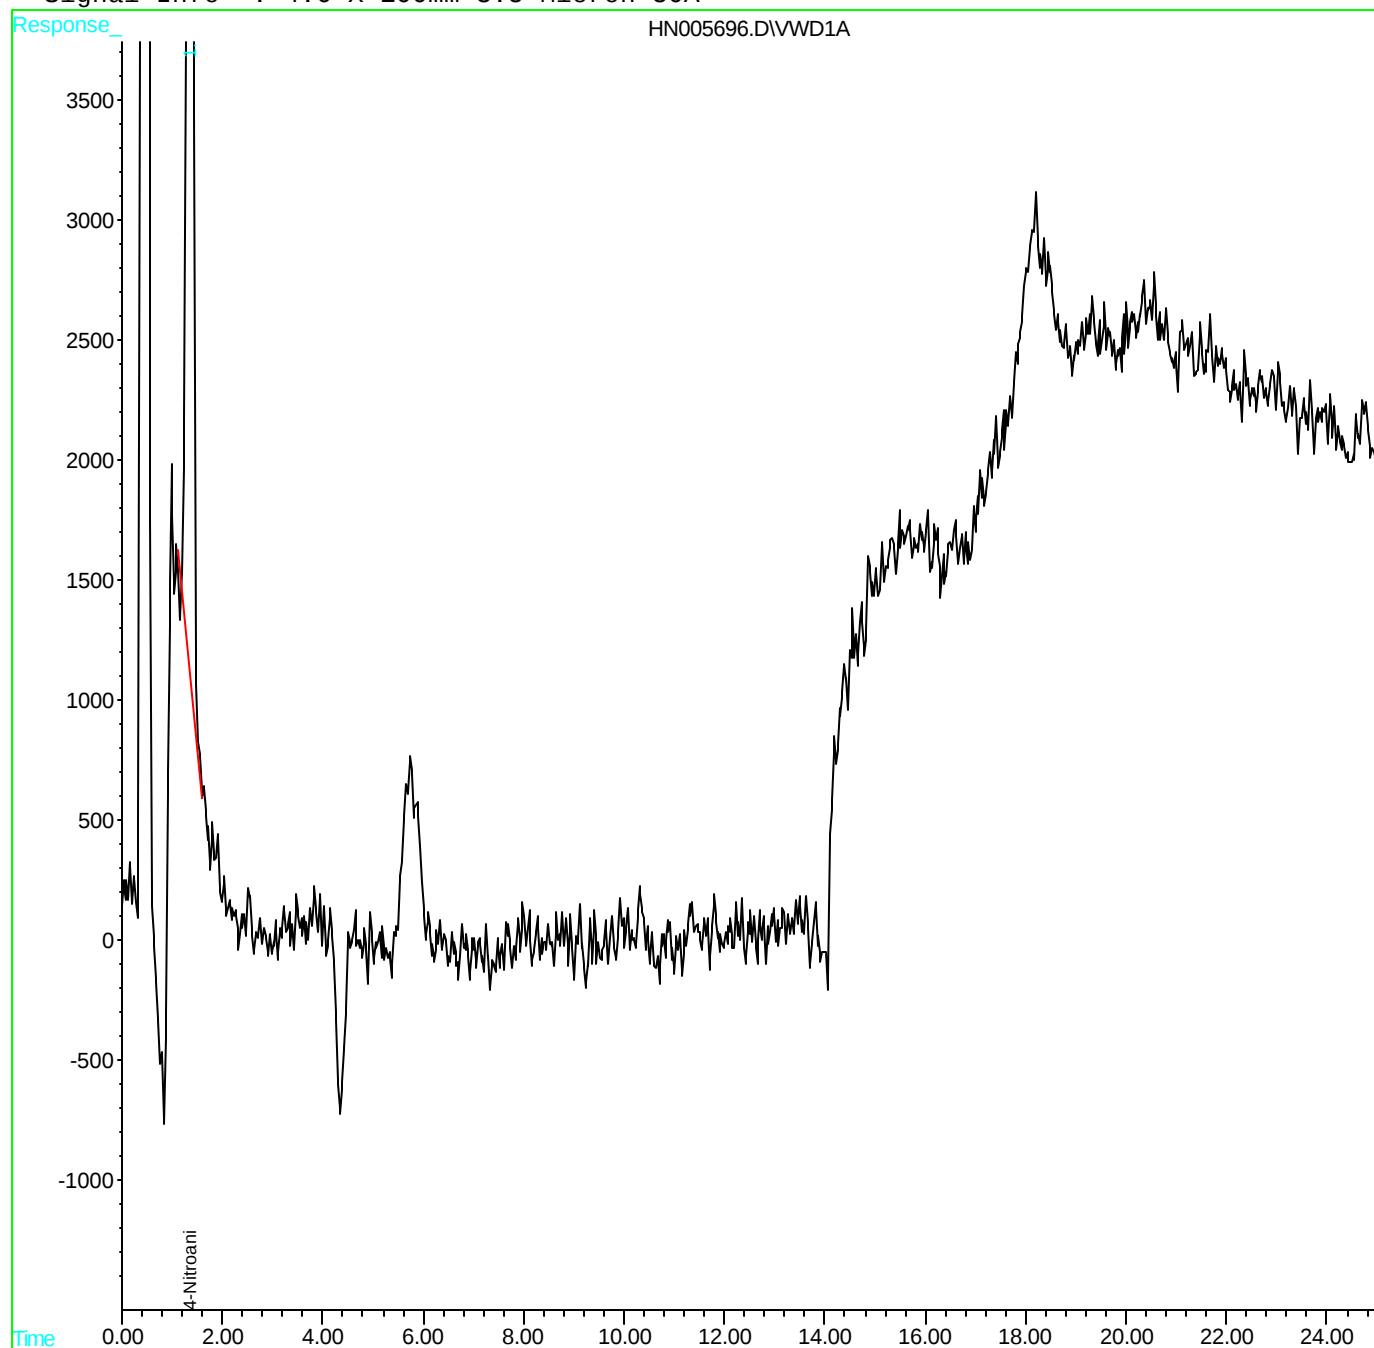

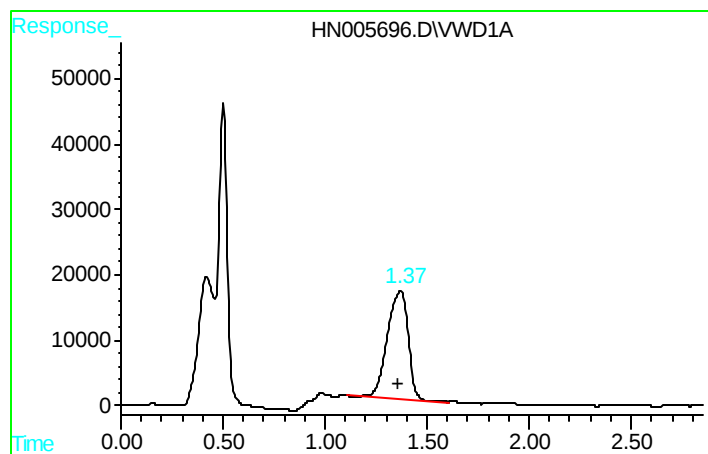

#1 4-Nitroaniline

R.T.: 1.368 min
Delta R.T.: 0.007 min
Response: 1159111
Conc: 295.59 ug/L

Instrument :
HPLC_N
ClientSampleId :
PB73038BL