

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN111113\HN005709.D Vial: 36
Acq On : 11-Nov-2013, 23:08 Operator: QM
Sample : E4140-02 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 12 11:58 2013 Quant Results File: HN1108NG.RES

Instrument :
HPLC_N
ClientSampleId :
PT-EXP-WP

Manual Integrations
APPROVED

QI
11/20/2013 6:59:51 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN1108NG.M
Title :
Last Update : Tue Nov 12 11:13:07 2013
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.38	1206848	0.313 ng/ulm

Target Compounds

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN005709.D HN1108NG.M

Tue Nov 12 15:32:59 2013

RPT1

Quantitation Report

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN111113\HN005709.D Vial: 36
Acq On : 11-Nov-2013, 23:08 Operator: QM
Sample : E4140-02 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Nov 12 11:58 2013 Quant Results File: HN1108NG.RES


Instrument :
HPLC_N
ClientSampleId :
PT-EXP-WP


Manual Integrations
APPROVED

QI
11/20/2013 6:59:51 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHOD\HN1108NG.M
Title :
Last Update : Tue Nov 12 11:13:07 2013
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

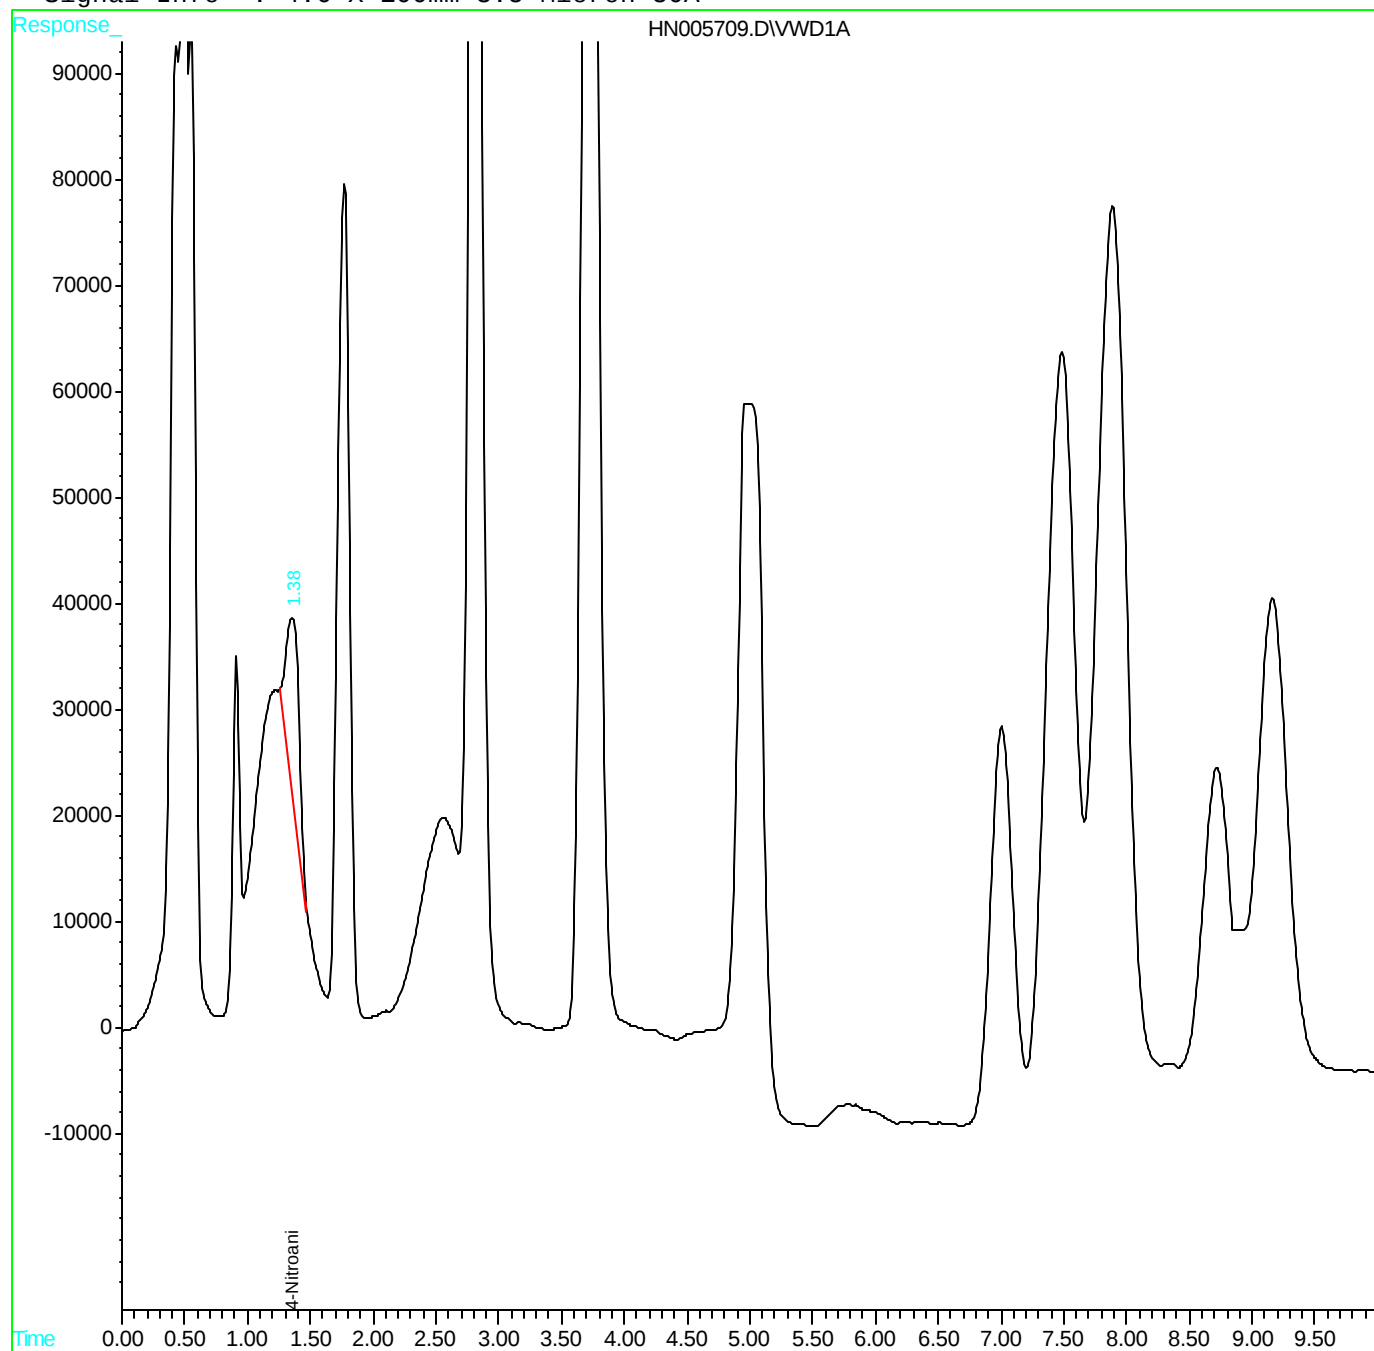

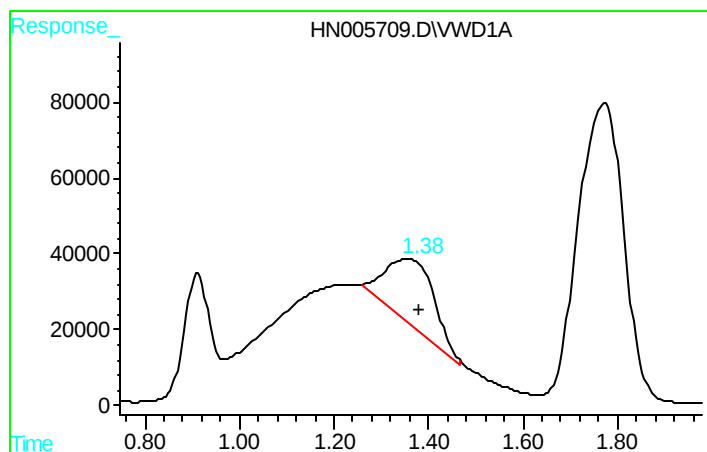

#1 4-Nitroaniline

R.T.: 1.377 min
Delta R.T.: -0.003 min
Response: 1206848
Conc: 0.31 ng/ul

Instrument :
HPLC_N
ClientSampleId :
PT-EXP-WP

Manual Integrations
APPROVED

QI
11/20/2013 6:59:51 PM