

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN111416\
 Data File : HN007783.D
 Signal(s) : vwd1A.ch
 Acq On : 14-Nov-2016, 12:44
 Operator : UM/MA
 Sample : HSTDICC0100
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 14 14:56:49 2016
 Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN111416.M
 Quant Title :
 QLast Update : Mon Nov 14 14:54:35 2016
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) T HMX	0.895	510210	116.942 ug/L
3) T RDX	1.691	656559	116.912 ug/L
4) T 1,3,5-Trinitrobenzene	2.651	1142356	106.249 ug/L
5) T 1,3-Dinitrobenzene	3.532	1804675	107.456 ng/ml
6) T 3,5-Dinitroaniline	3.932	1475978	109.988 ug/L
7) T Nitrobenzene	4.721	1027126	105.279 ug/L
8) T Tetryl	6.260	842046	105.473 ug/L
9) T 2,4,6-Trinitrotoluene	6.487	1137913	107.211 ug/L
12) T 2,4-Dinitrotoluene	8.144	1231134	80.923 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN111416\
Data File : HN007783.D
Signal(s) : vwd1A.ch
Acq On : 14-Nov-2016, 12:44
Operator : UM/MA
Sample : HSTDICC0100
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 14:56:49 2016
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN111416.M
Quant Title :
QLast Update : Mon Nov 14 14:54:35 2016
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

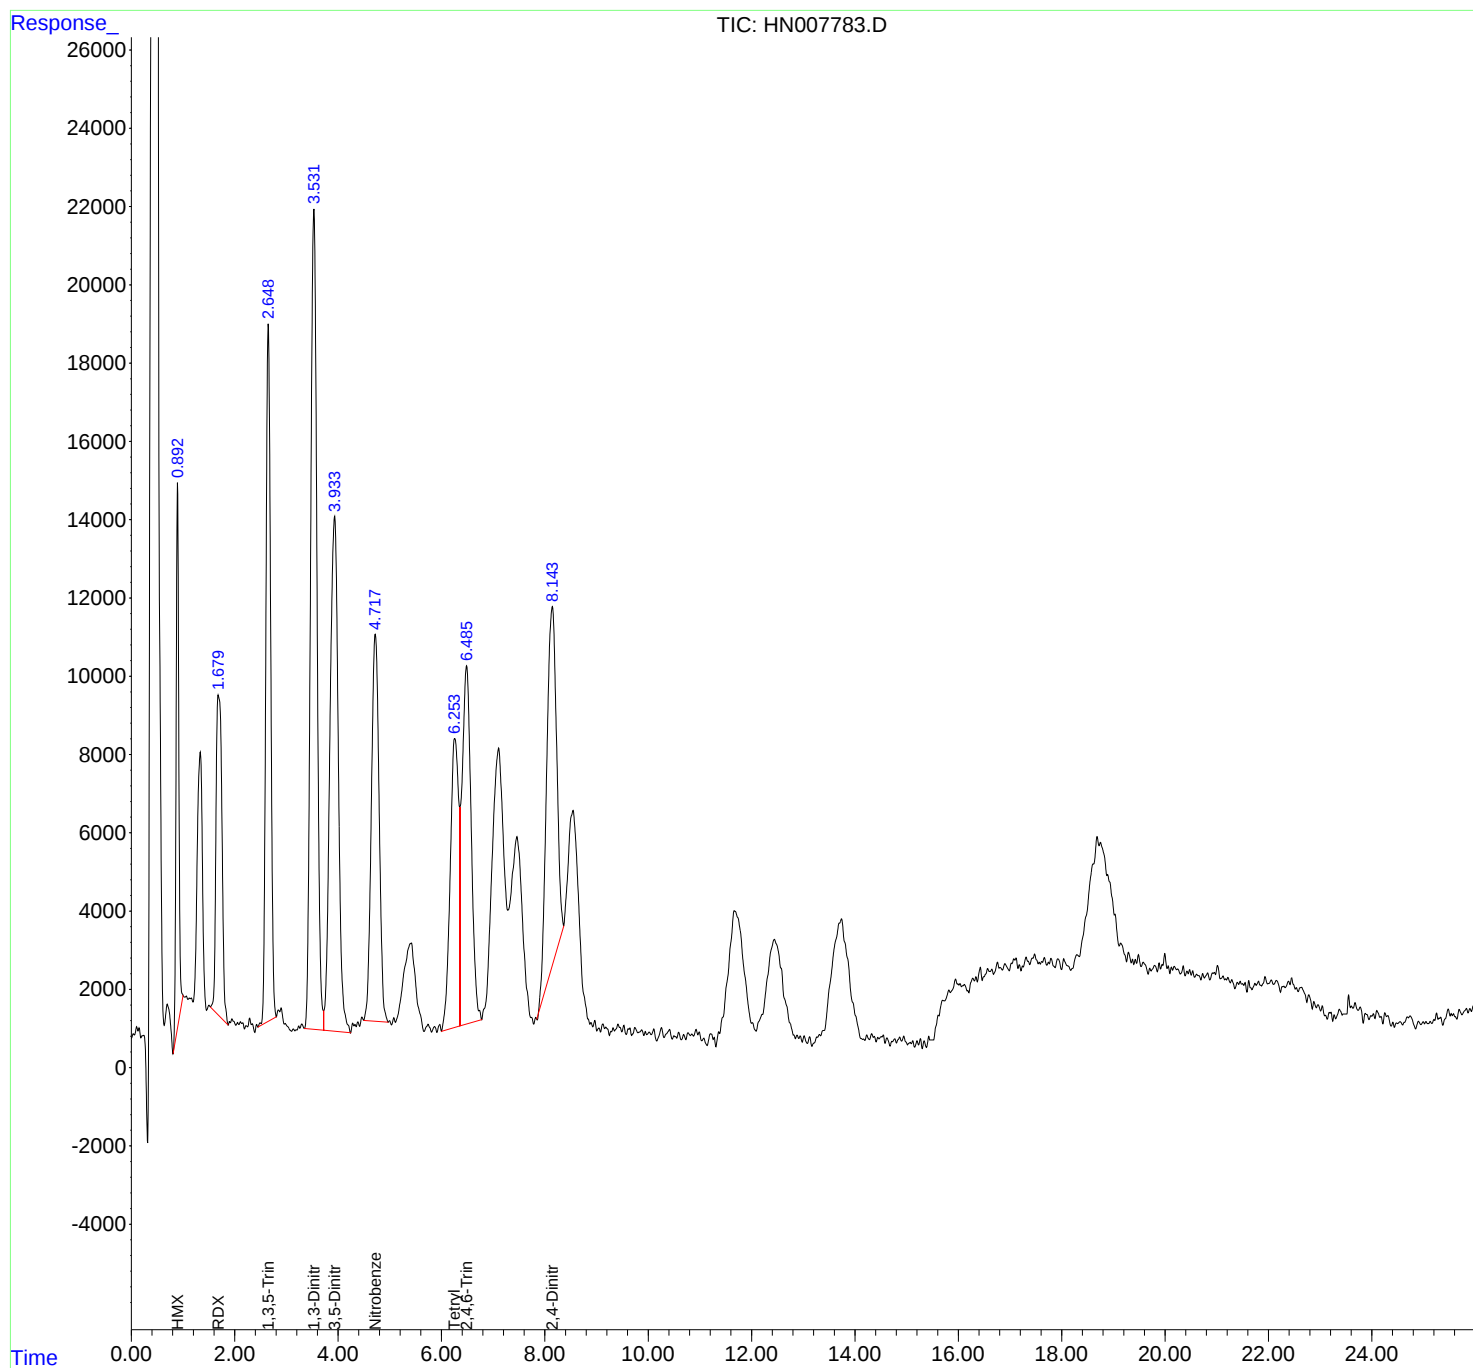


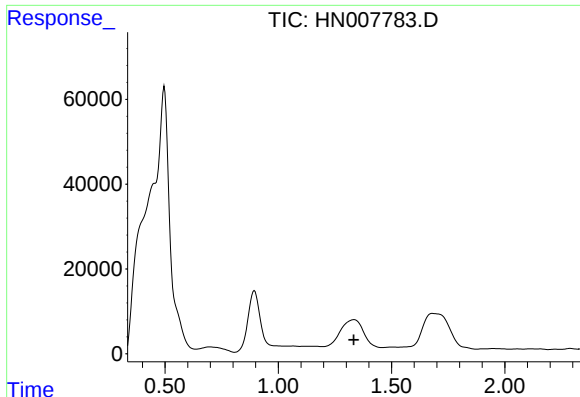

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 1.333 min
Response: 0
Conc: N.D.

Instrument :
HPLC_N
ClientSampleId :

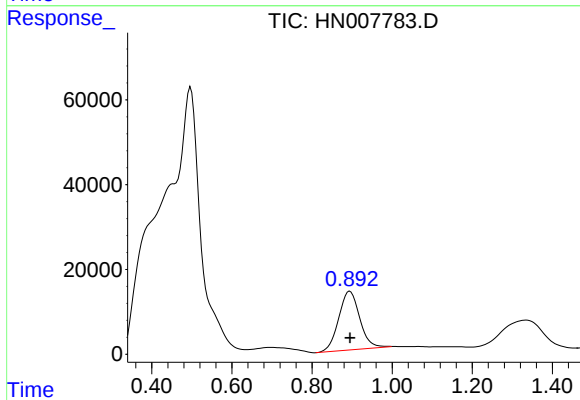


#2 HMX

R.T.: 0.895 min
Delta R.T.: 0.000 min
Response: 510210
Conc: 116.94 ug/L

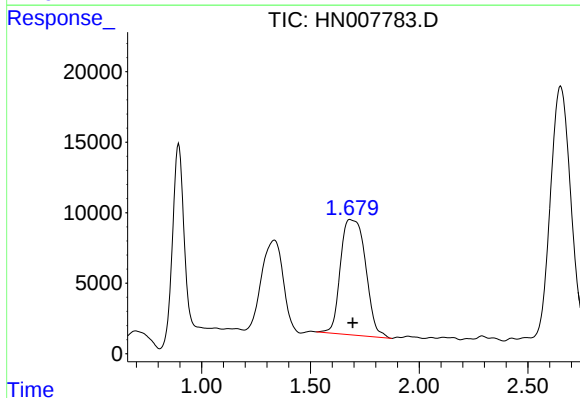


#3 RDX

R.T.: 1.691 min
Delta R.T.: -0.003 min
Response: 656559
Conc: 116.91 ug/L

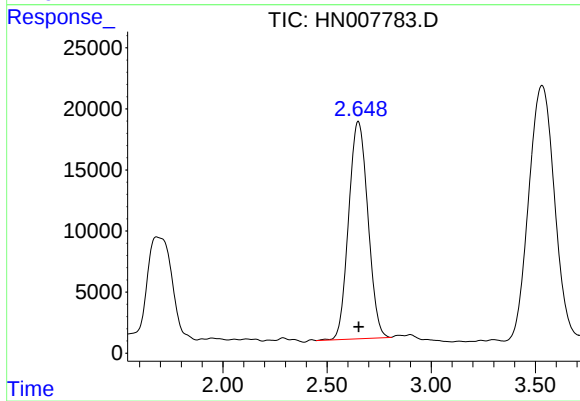

#4 1,3,5-Trinitrobenzene


R.T.: 2.651 min
Delta R.T.: -0.002 min
Response: 1142356
Conc: 106.25 ug/L

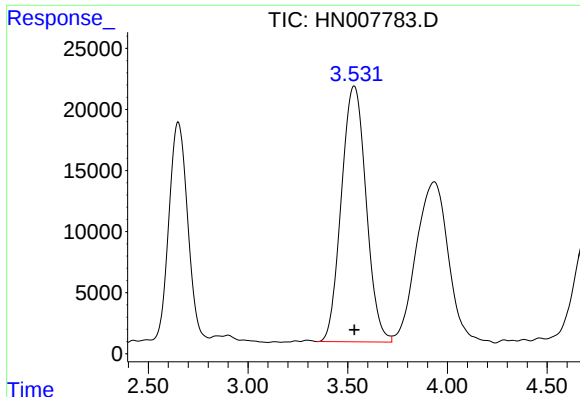

#5 1,3-Dinitrobenzene


R.T.: 3.532 min
Delta R.T.: -0.002 min
Response: 1804675
Conc: 107.46 ng/ml

Instrument :
HPLC_N
ClientSampleId :

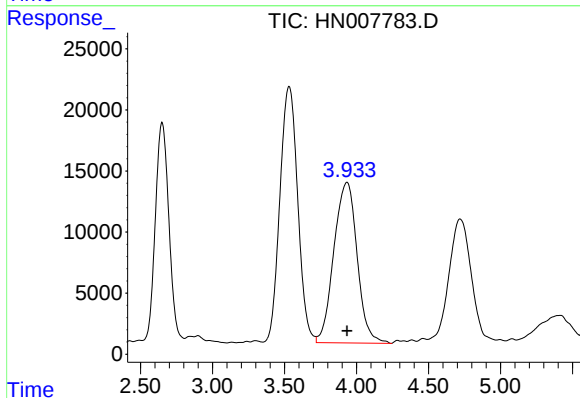


#6 3,5-Dinitroaniline

R.T.: 3.932 min
Delta R.T.: -0.003 min
Response: 1475978
Conc: 109.99 ug/L

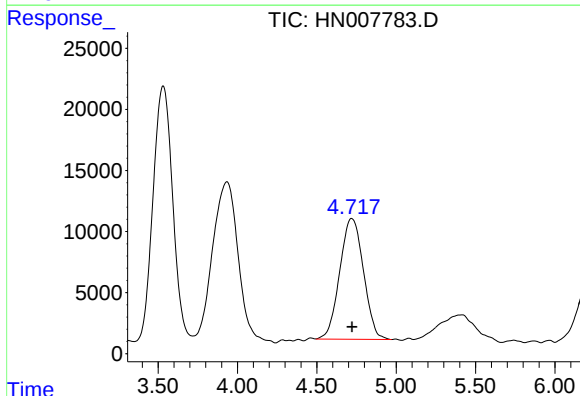


#7 Nitrobenzene

R.T.: 4.721 min
Delta R.T.: -0.002 min
Response: 1027126
Conc: 105.28 ug/L

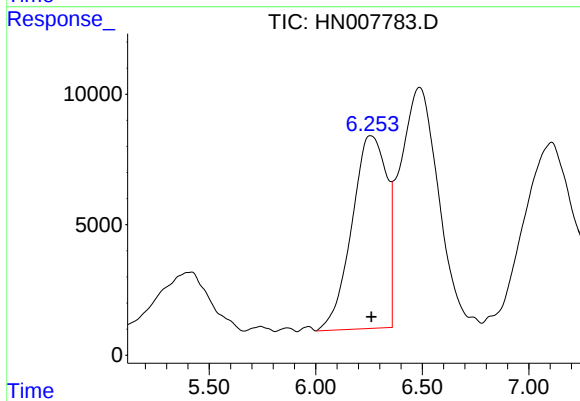

#8 Tetryl


R.T.: 6.260 min
Delta R.T.: -0.002 min
Response: 842046
Conc: 105.47 ug/L

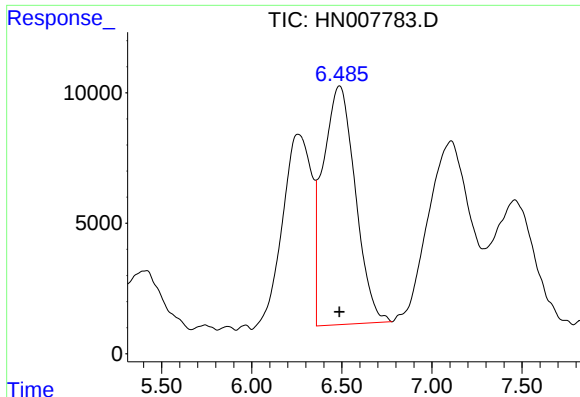

#9 2,4,6-Trinitrotoluene

R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 1137913
Conc: 107.21 ug/L

Instrument :
HPLC_N
ClientSampleId :

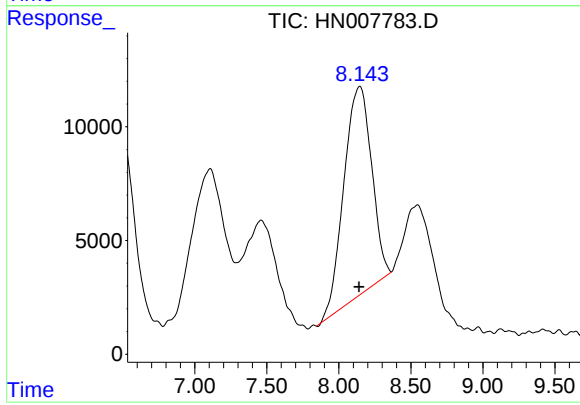

#12 2,4-Dinitrotoluene

R.T.: 8.144 min
Delta R.T.: 0.004 min
Response: 1231134
Conc: 80.92 ug/L