

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN111416\
 Data File : HN007801.D
 Signal(s) : vwd1A.ch
 Acq On : 14-Nov-2016, 19:15
 Operator : UM/MA
 Sample : H5556-01DL 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 15 00:43:40 2016
 Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN111416.M
 Quant Title :
 QLast Update : Mon Nov 14 15:03:45 2016
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

2) T	HMX	0.894	1332879	292.656 ug/L
3) T	RDX	1.706f	2759615	472.554 ug/L
4) T	1,3,5-Trinitrobenzene	2.651	2757972	252.691 ug/L
5) T	1,3-Dinitrobenzene	3.533	5930575	346.330 ng/ml
7) T	Nitrobenzene	4.722	4079414	412.037 ug/L
9) T	2,4,6-Trinitrotoluene	6.494	3988876	364.084 ug/L
10) T	2-Amino-4,6-dinitroto...	7.106	7316262	664.870 ug/L
11) T	4-Amino-2,6-dinitroto...	7.451	1747247	240.457 ug/L
13) T	2,6-Dinitrotoluene	8.548	2347434	279.269 ug/L
14) T	2-Nitrotoluene	11.712	3581423	539.454 ug/L
15) T	4-Nitrotoluene	12.459	1739816	323.322 ug/L
16) T	3-Nitrotoluene	13.731	1767358	267.247 ug/L

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN111416\
Data File : HN007801.D
Signal(s) : vwd1A.ch
Acq On : 14-Nov-2016, 19:15
Operator : UM/MA
Sample : H5556-01DL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 15 00:43:40 2016
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN111416.M
Quant Title :
QLast Update : Mon Nov 14 15:03:45 2016
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

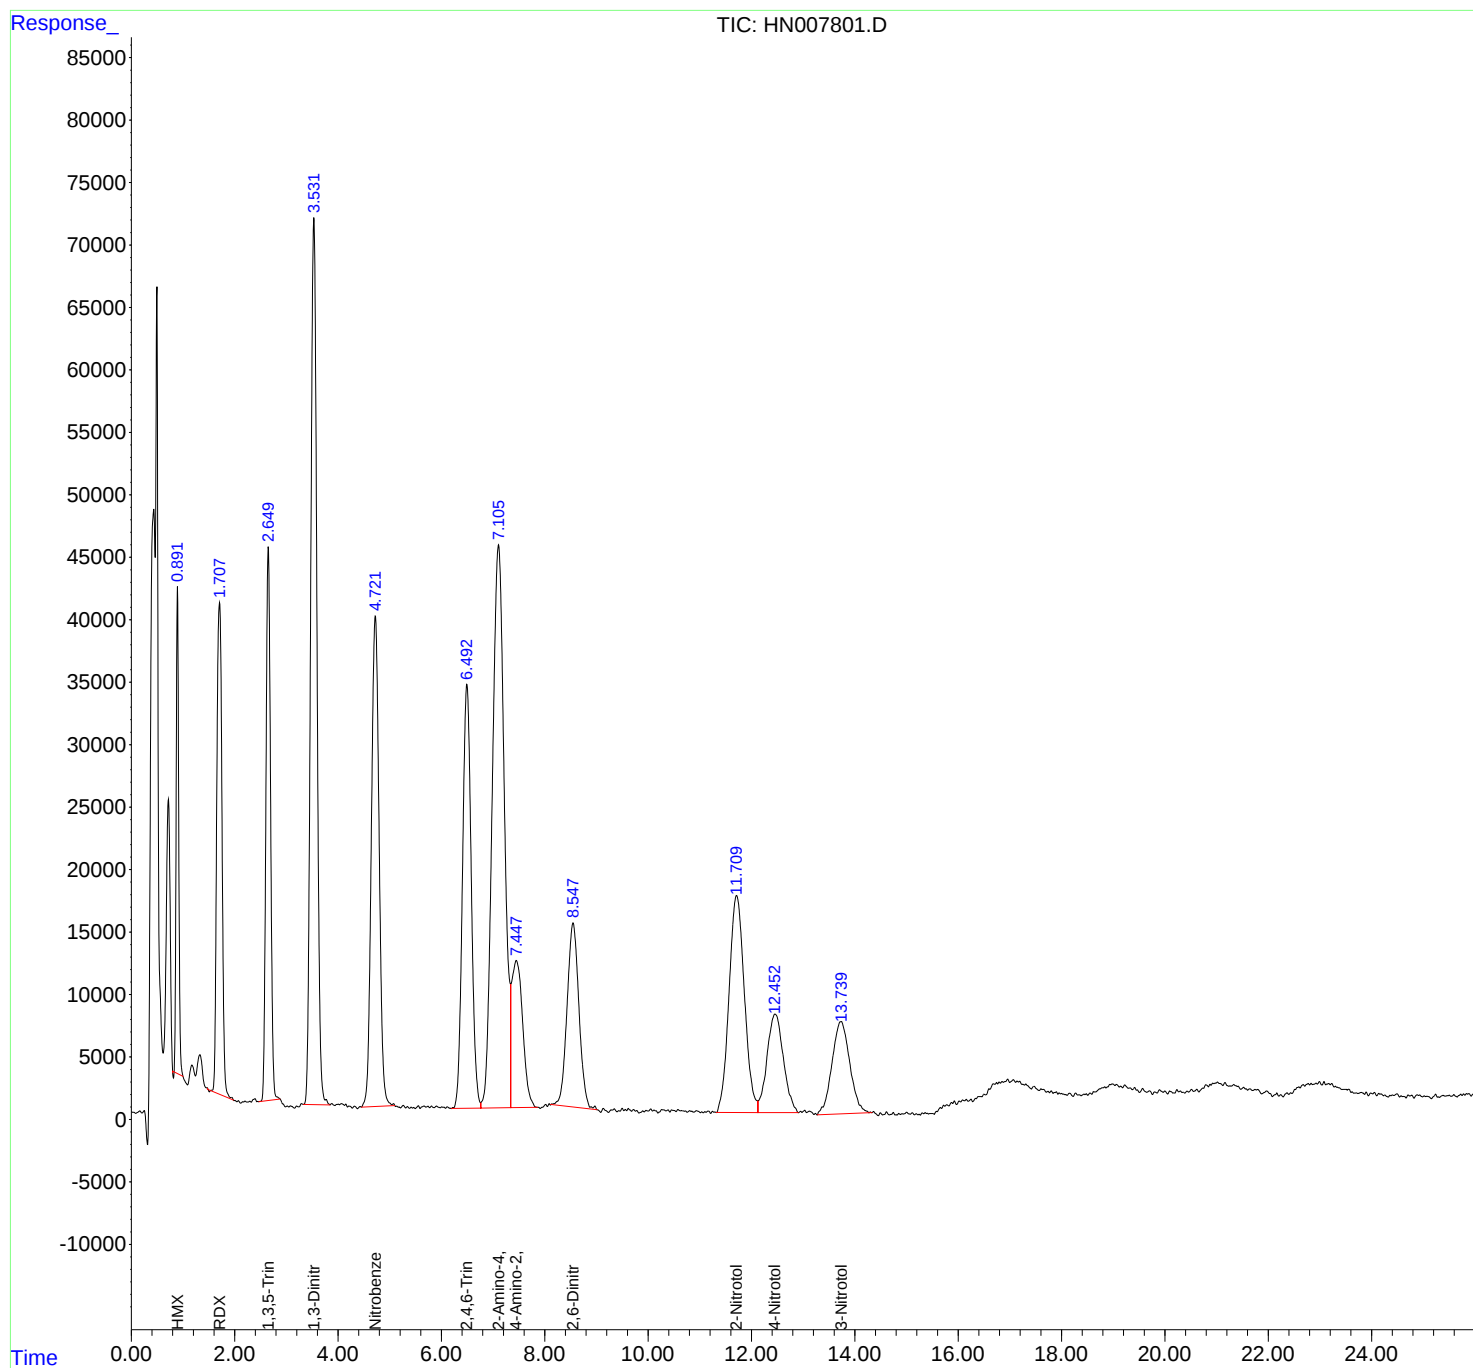


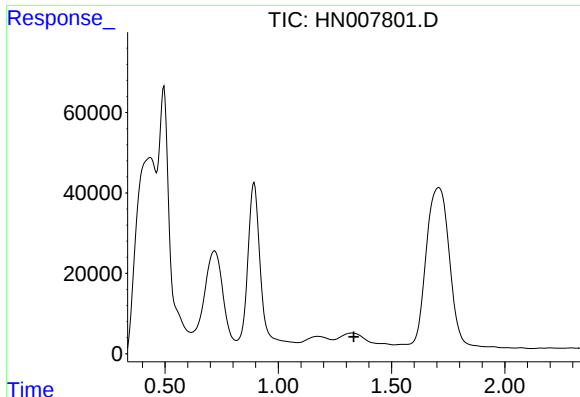

#1 4-Nitroaniline


R.T.: 0.000 min
Exp R.T.: 1.333 min
Response: 0
Conc: N.D.

Instrument :
HPLC_N
ClientSampleId :

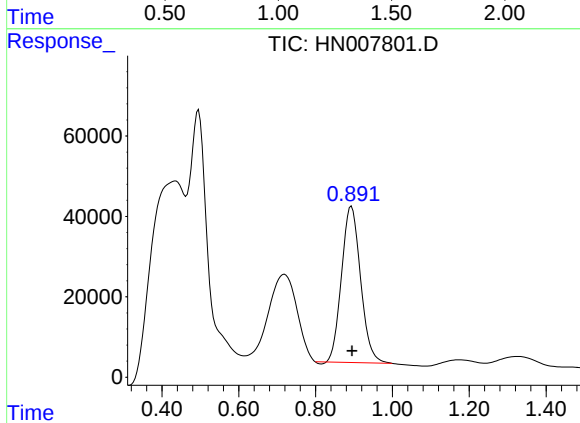


#2 HMX

R.T.: 0.894 min
Delta R.T.: -0.002 min
Response: 1332879
Conc: 292.66 ug/L

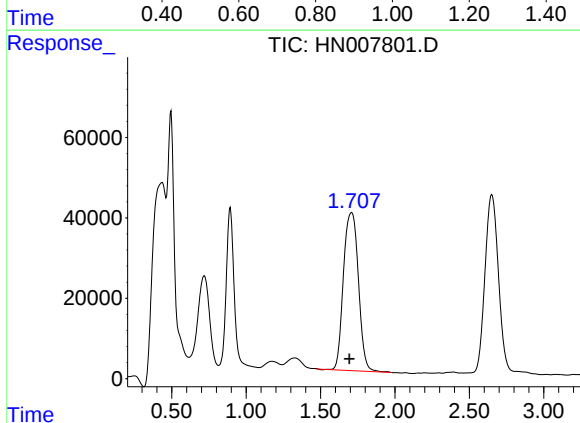


#3 RDX

R.T.: 1.706 min
Delta R.T.: 0.012 min
Response: 2759615
Conc: 472.55 ug/L

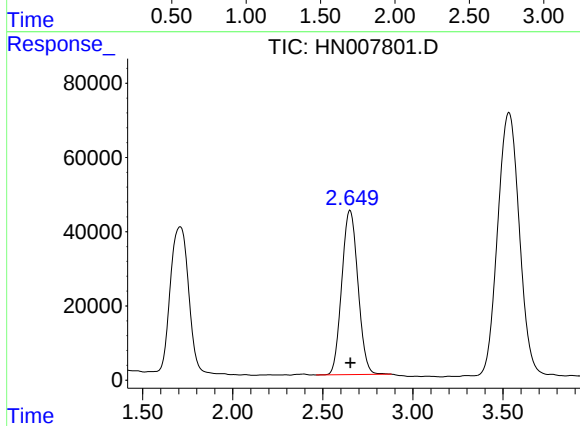

#4 1,3,5-Trinitrobenzene


R.T.: 2.651 min
Delta R.T.: -0.002 min
Response: 2757972
Conc: 252.69 ug/L

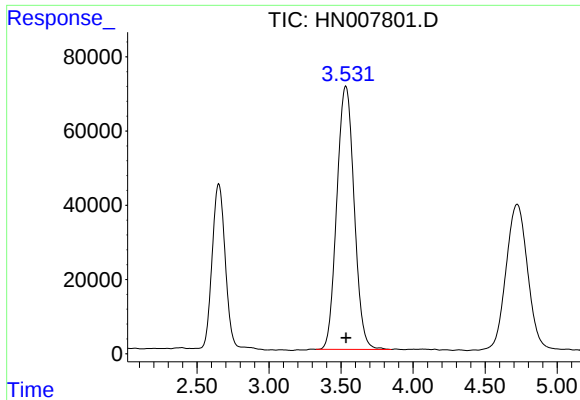

#5 1,3-Dinitrobenzene


R.T.: 3.533 min
Delta R.T.: -0.002 min
Response: 5930575
Conc: 346.33 ng/ml

Instrument :
HPLC_N
ClientSampleId :

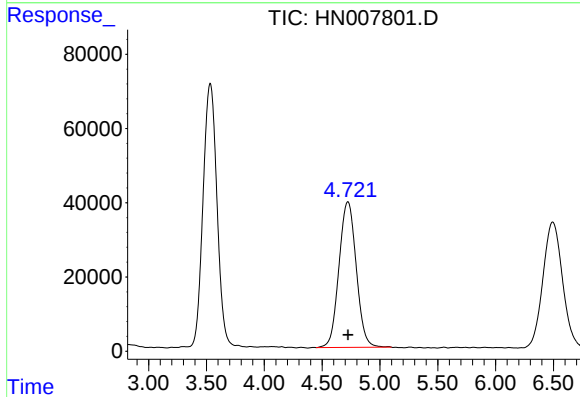


#7 Nitrobenzene

R.T.: 4.722 min
Delta R.T.: 0.000 min
Response: 4079414
Conc: 412.04 ug/L

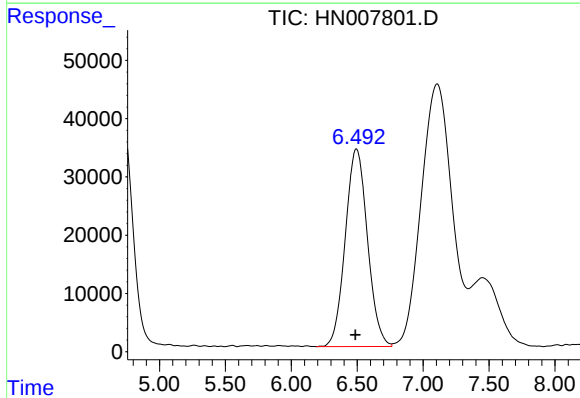


#9 2,4,6-Trinitrotoluene

R.T.: 6.494 min
Delta R.T.: 0.007 min
Response: 3988876
Conc: 364.08 ug/L

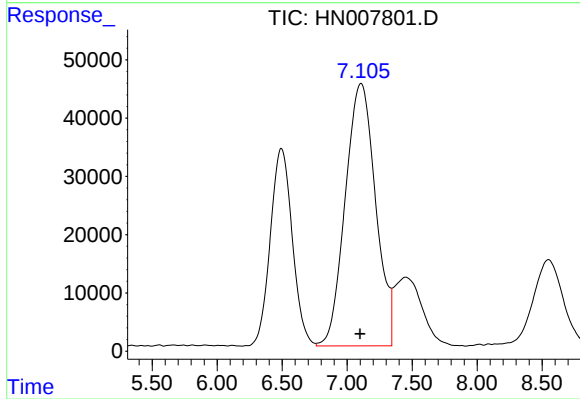

#10 2-Amino-4,6-dinitrotoluene


R.T.: 7.106 min
Delta R.T.: 0.005 min
Response: 7316262
Conc: 664.87 ug/L

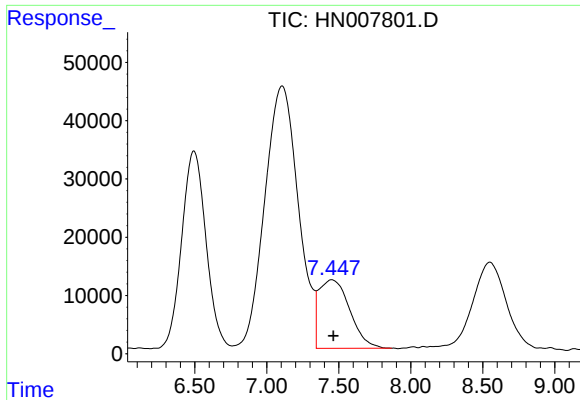

#11 4-Amino-2,6-dinitrotoluene


R.T.: 7.451 min
Delta R.T.: -0.010 min
Response: 1747247
Conc: 240.46 ug/L

Instrument :
HPLC_N
ClientSampleId :

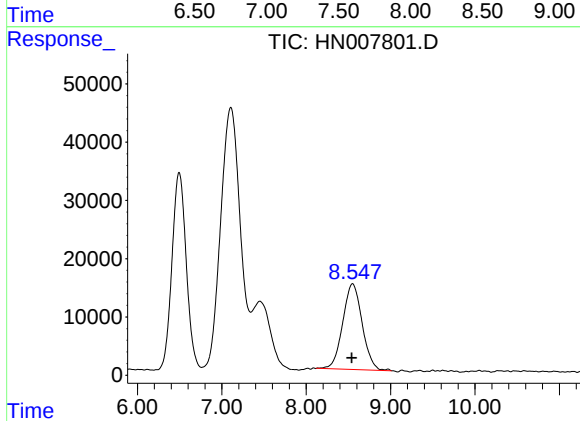


#13 2,6-Dinitrotoluene

R.T.: 8.548 min
Delta R.T.: 0.008 min
Response: 2347434
Conc: 279.27 ug/L

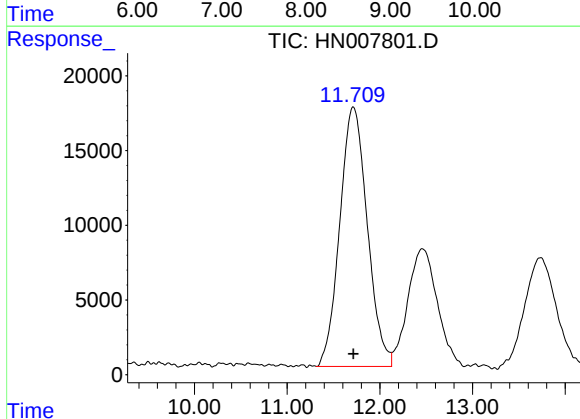


#14 2-Nitrotoluene

R.T.: 11.712 min
Delta R.T.: 0.000 min
Response: 3581423
Conc: 539.45 ug/L

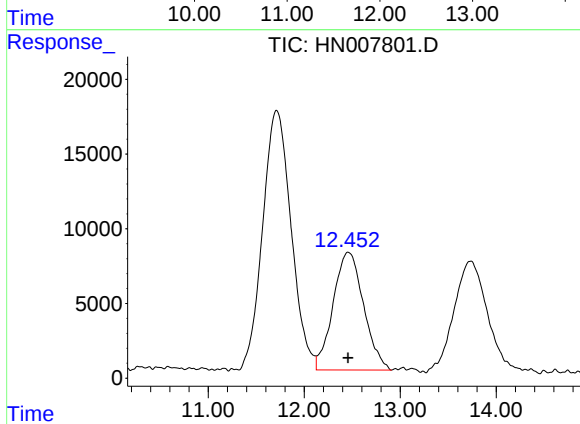

#15 4-Nitrotoluene

R.T.: 12.459 min
Delta R.T.: 0.001 min
Response: 1739816
Conc: 323.32 ug/L

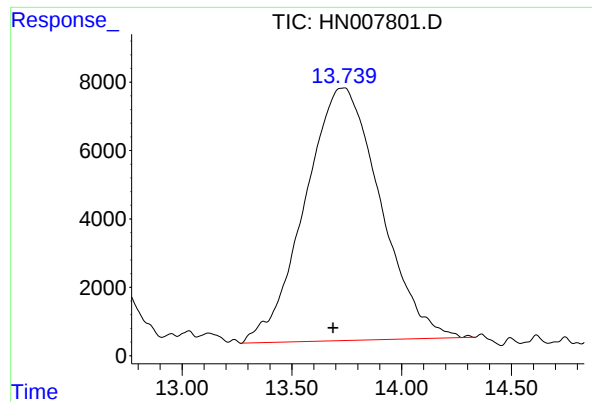

#16 3-Nitrotoluene

R.T.: 13.731 min
Delta R.T.: 0.044 min
Response: 1767358
Conc: 267.25 ug/L

Instrument :
HPLC_N
ClientSampleId :