

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007127.D\VWD1A.CH Vial: 7
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007127.D\VWD1A.CH
 Acq On : 02-Dec-2014, 13:37 Operator: TP
 Sample : PB80633BL Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Dec 3 6:22 2014 Quant Results File: HN120214.RES

Instrument :
 HPLC_N
 ClientSampleId :
 PB80633BL

Manual Integrations
 APPROVED

ugo
 12/8/2014 4:32:34 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN120214.M
 Title :
 Last Update : Tue Dec 02 14:25:16 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	2031654	485.013 ug/L m

Target Compounds

 Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN007127.D HN120214.M Wed Dec 31 17:29:59 2014

Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007127.D\VWD1A.CH Vial: 7
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007127.D\VWD1A.CH
 Acq On : 02-Dec-2014, 13:37 Operator: TP
 Sample : PB80633BL Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Dec 3 6:22 2014 Quant Results File: HN120214.RES



Instrument :
 HPLC_N
 ClientSampleId :
 PB80633BL


Manual Integrations
 APPROVED

ugo
 12/8/2014 4:32:34 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN120214.M
 Title :
 Last Update : Tue Dec 02 14:25:16 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

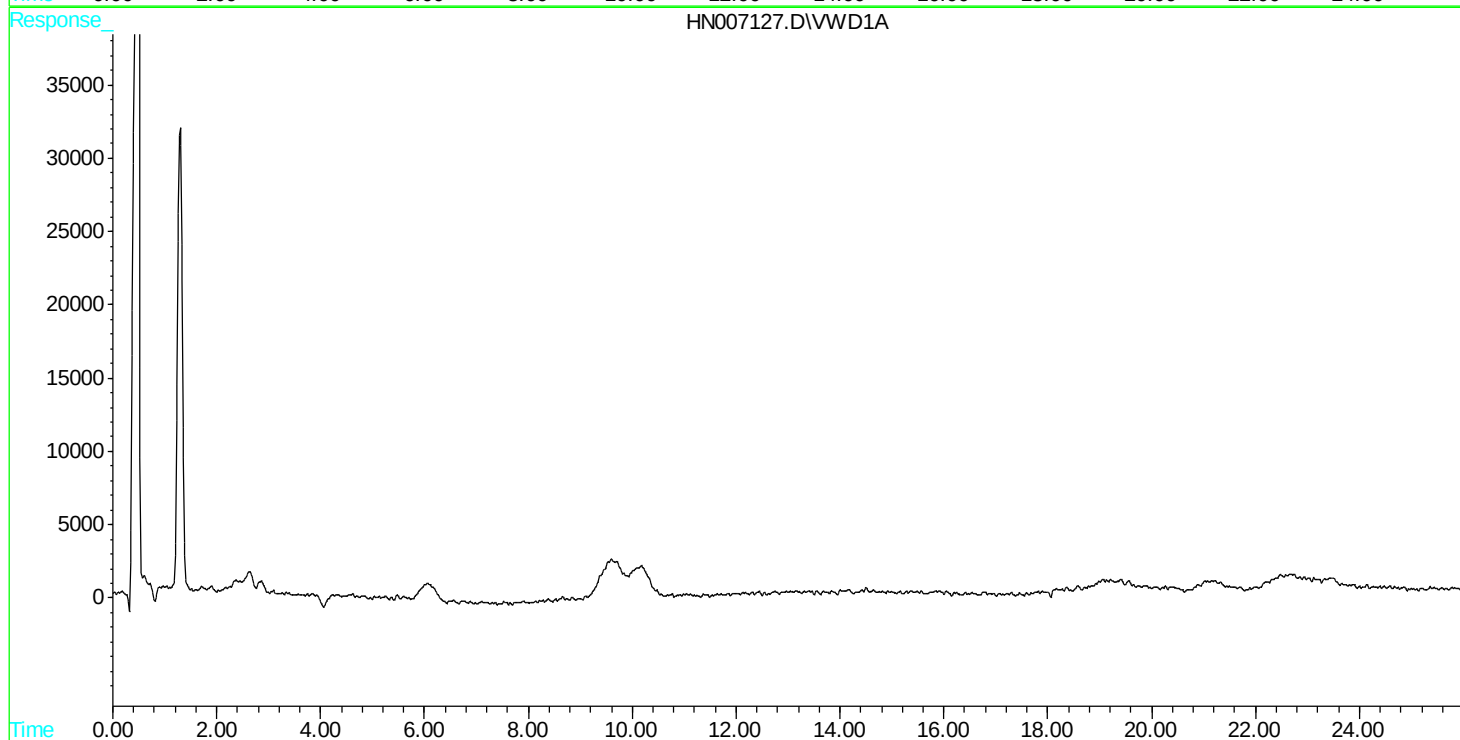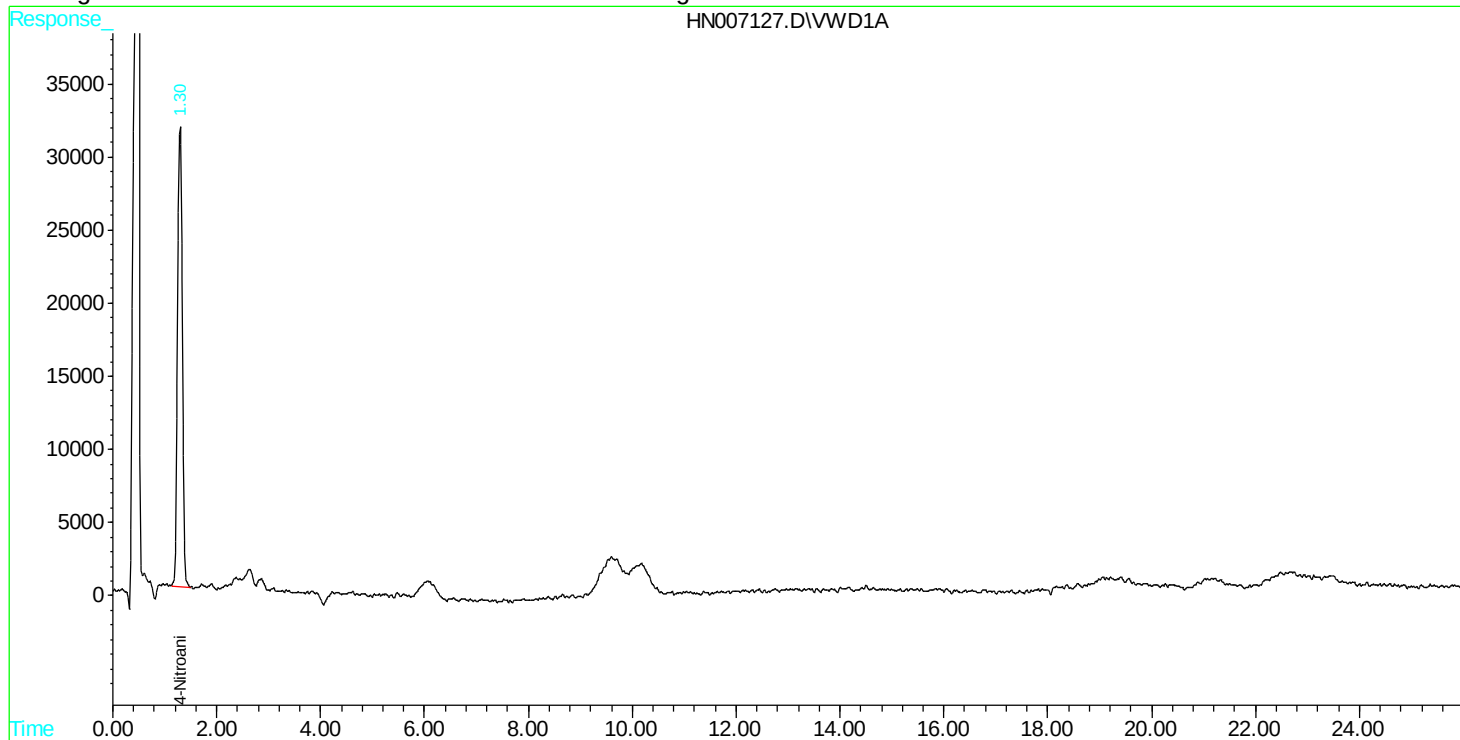

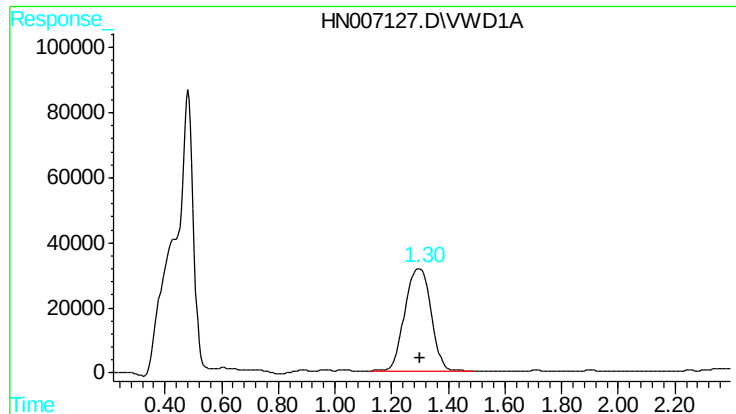

#1 4-Nitroaniline

R.T.: 1.295 min
Delta R.T.: -0.004 min
Response: 2031654
Conc: 485.01 ug/L m

Instrument :
HPLC_N
ClientSampleId :
PB80633BL

Manual Integrations
APPROVED

ugo
12/8/2014 4:32:34 PM