

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007138.D\VWD1A.CH Vial: 17
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007138.D\VWD1A.CH
 Acq On : 02-Dec-2014, 17:25 Operator: TP
 Sample : HSTDICC0.5 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Dec 3 6:01 2014 Quant Results File: HN1202NG.RES

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICC0.5

Manual Integrations
 APPROVED

ugo
 12/8/2014 4:32:54 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
 Title :
 Last Update : Wed Nov 26 06:13:45 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	2073249	0.511 ng/ul
Target Compounds			
2) T Nitroglycerin	6.13	4388726	0.505 ng/ulm

 Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN007138.D HN1202NG.M Wed Dec 31 17:33:49 2014

Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007138.D\VWD1A.CH Vial: 17
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007138.D\VWD1A.CH
 Acq On : 02-Dec-2014, 17:25 Operator: TP
 Sample : HSTDICC0.5 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Dec 3 6:01 2014 Quant Results File: HN1202NG.RES



Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICC0.5


Manual Integrations
 APPROVED

ugo
 12/8/2014 4:32:54 PM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
 Title :
 Last Update : Wed Nov 26 06:13:45 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

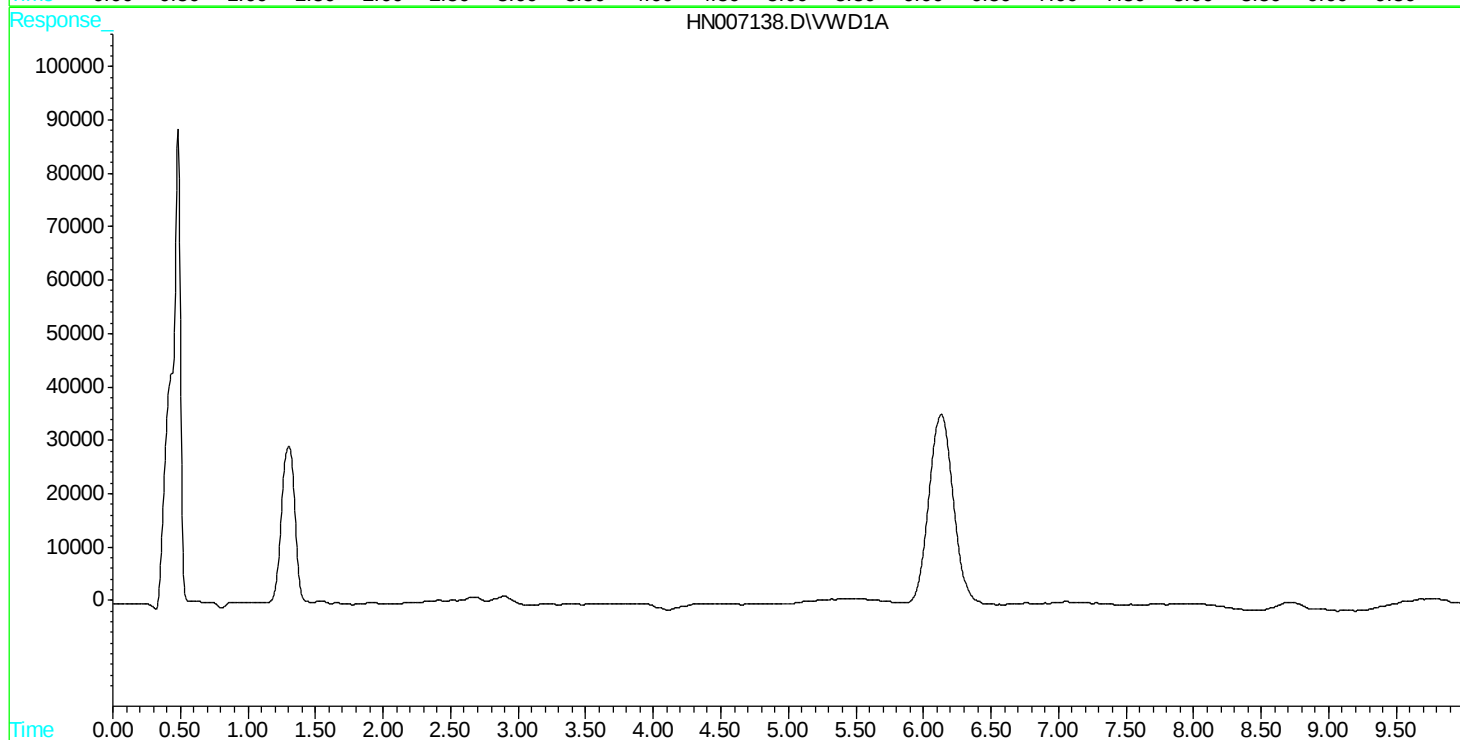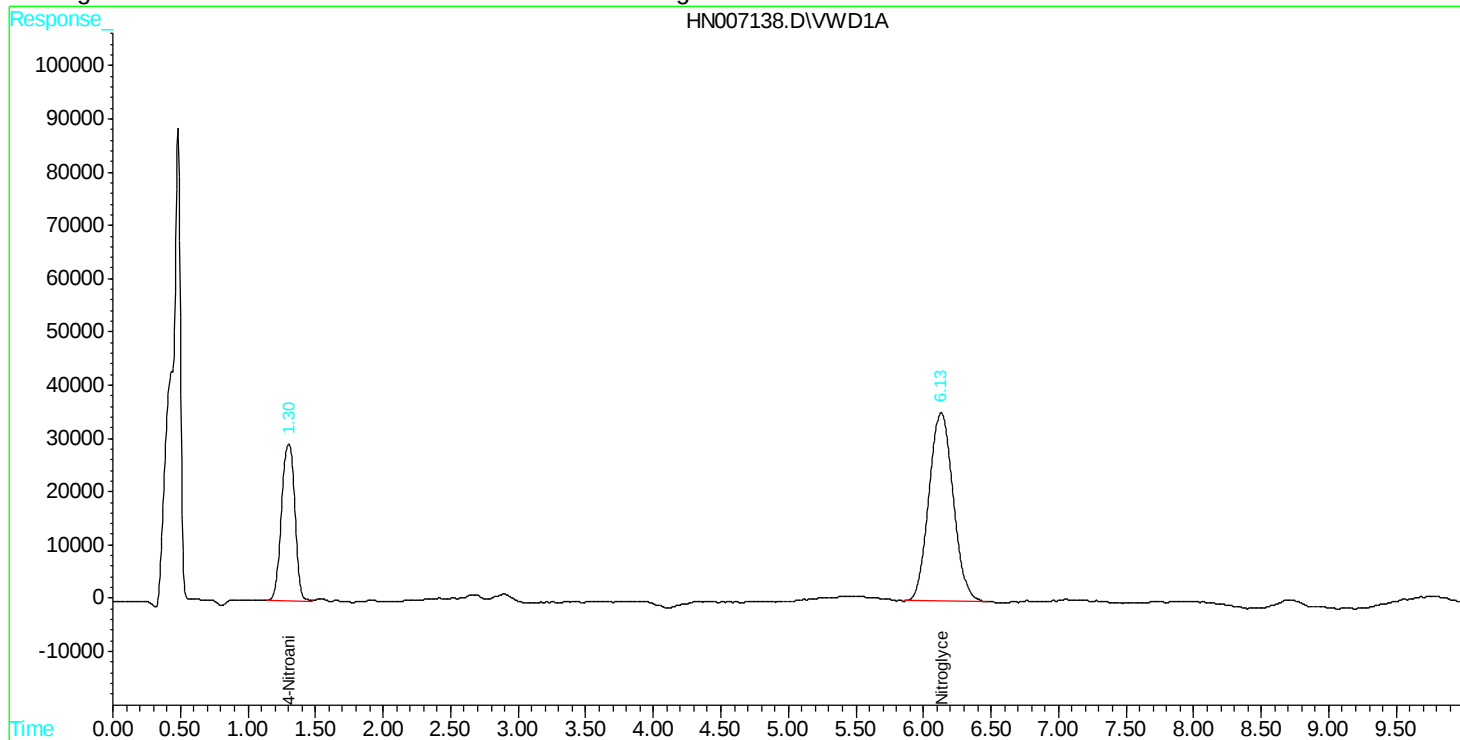

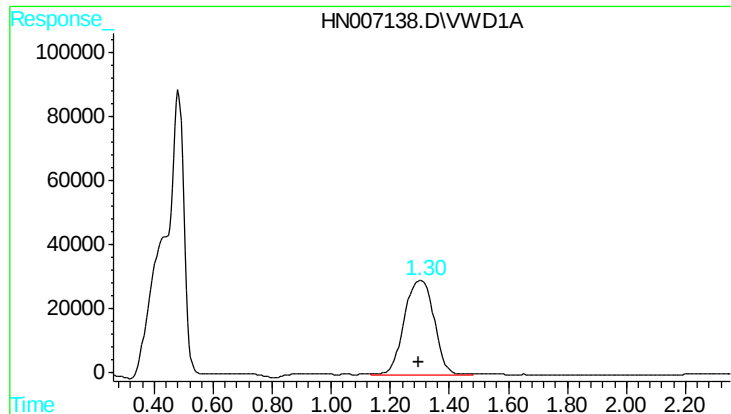


#1 4-Nitroaniline

R.T.: 1.304 min
Delta R.T.: 0.006 min
Response: 2073249
Conc: 0.51 ng/u1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC0.5

Manual Integrations
APPROVED

ugo
12/8/2014 4:32:54 PM

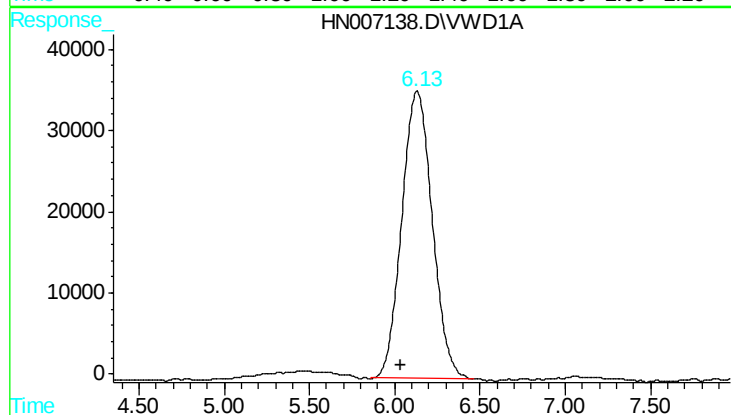

#2 Nitroglycerin

R.T.: 6.129 min
Delta R.T.: 0.094 min
Response: 4388726
Conc: 0.51 ng/u1 m