

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007139.D\VWD1A.CH Vial: 18
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007139.D\VWD1A.CH
 Acq On : 02-Dec-2014, 17:37 Operator: TP
 Sample : HSTDICV005 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Dec 3 6:06 2014 Quant Results File: HN1202NG.RES

Instrument :
 HPLC_N
 ClientSampleId :
 ICVHN120214NG

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
 Title :
 Last Update : Wed Dec 03 06:03:01 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.31	20644084	5.073 ng/ul
Target Compounds			
2) T Nitroglycerin	6.04	43631001	5.052 ng/ul

 Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.



HN007139.D HN1202NG.M Wed Dec 31 17:34:08 2014


Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007139.D\VWD1A.CH Vial: 18
Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007139.D\VWD1A.CH
Acq On : 02-Dec-2014, 17:37 Operator: TP
Sample : HSTDICV005 Inst : G1314A
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Dec 3 6:06 2014 Quant Results File: HN1202NG.RES

Instrument :
HPLC_N
ClientSampleId :
ICVHN120214NG

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
Title :
Last Update : Wed Dec 03 06:03:01 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

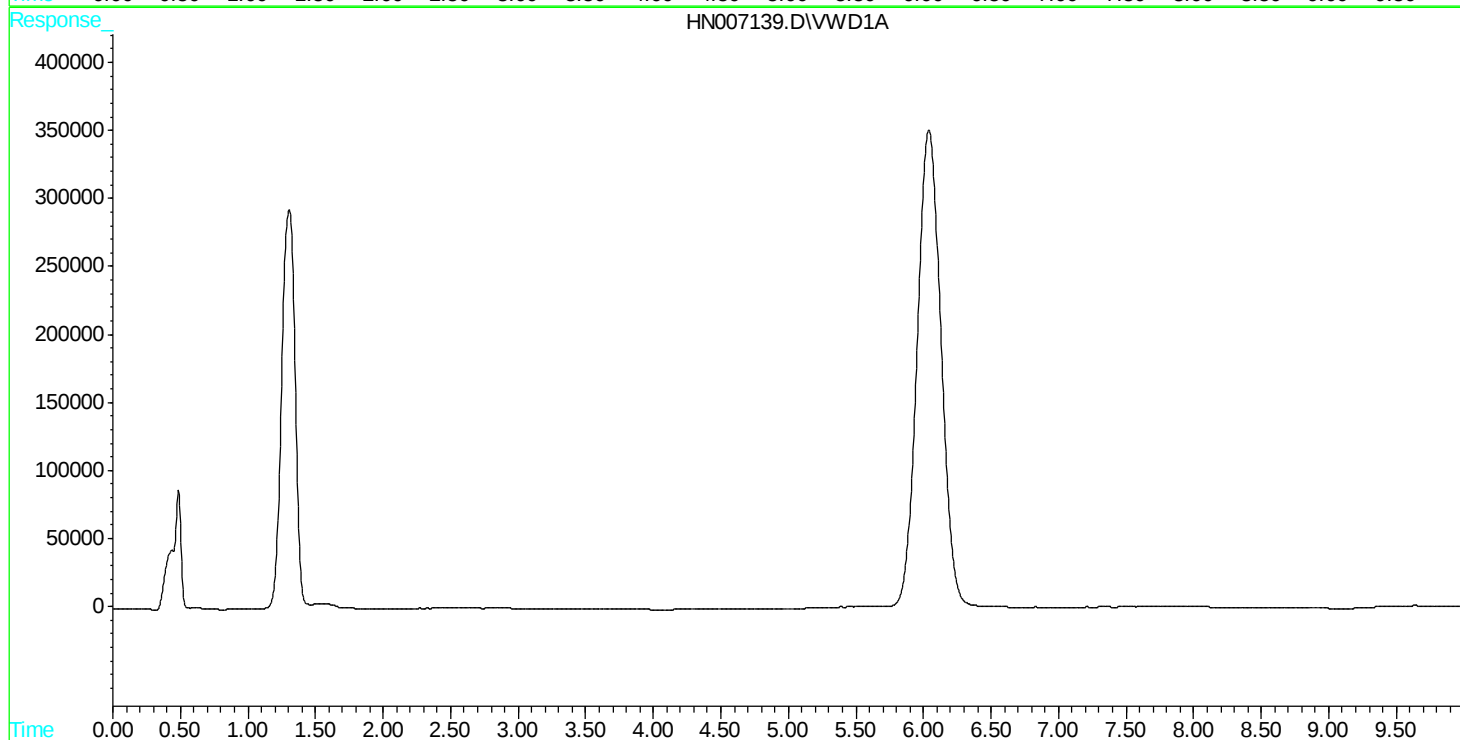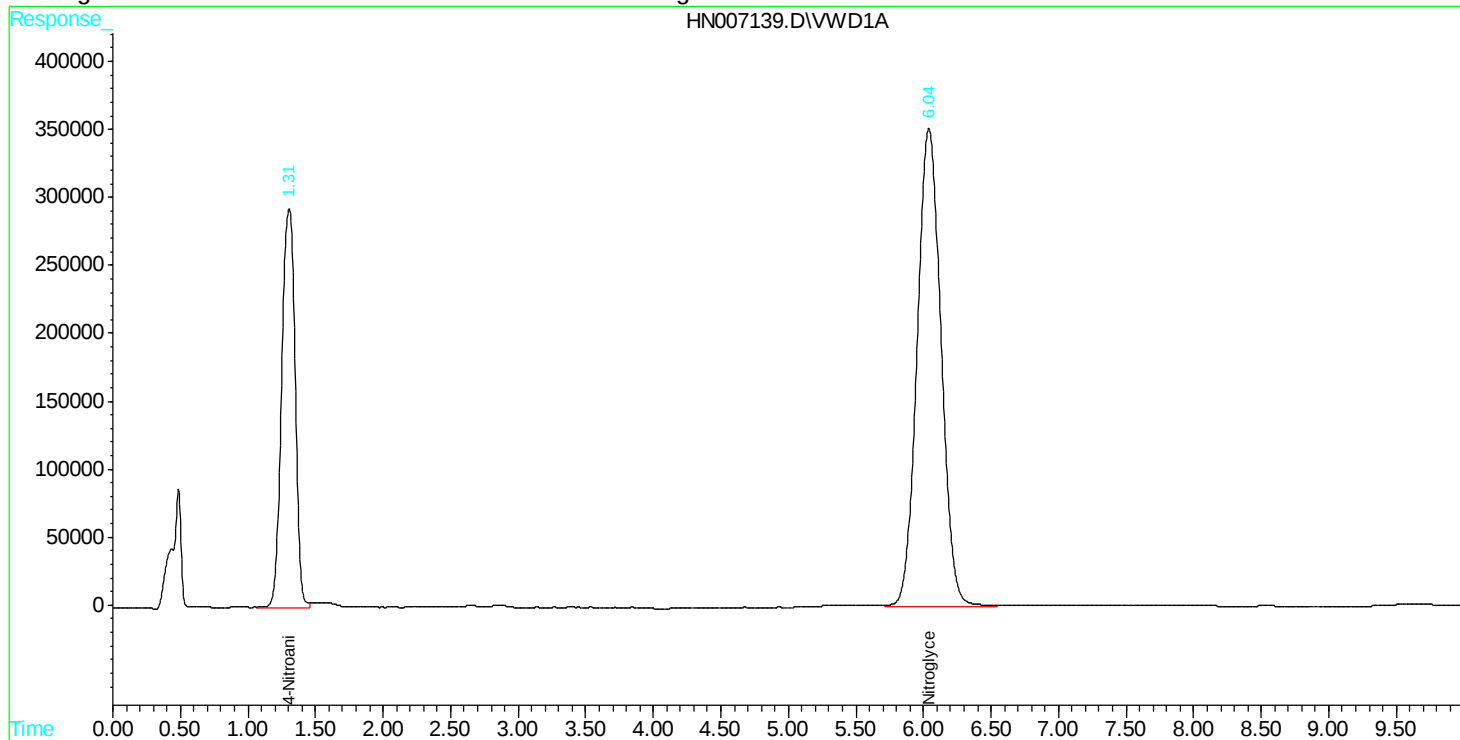


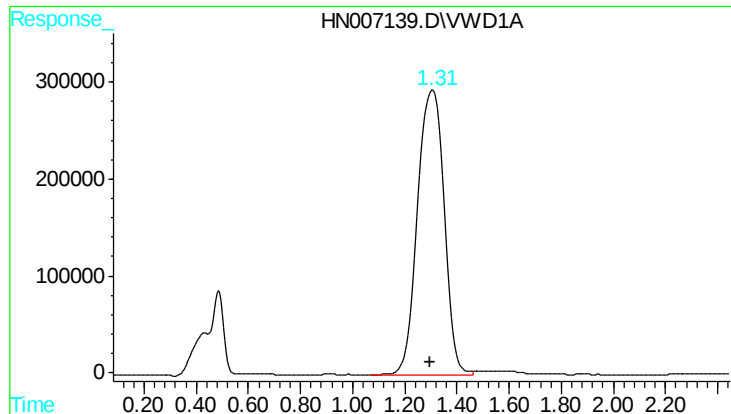

#1 4-Nitroaniline

R.T.: 1.307 min
Delta R.T.: 0.009 min
Response: 20644084
Conc: 5.07 ng/u1

Instrument :
HPLC_N
ClientSampleId :
ICVHN120214NG

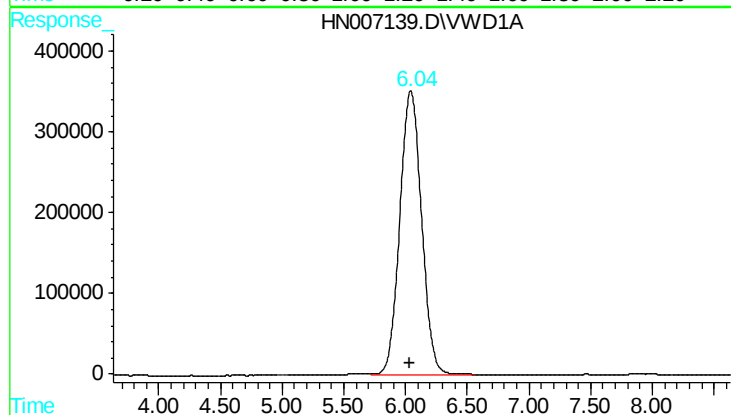

#2 Nitroglycerin

R.T.: 6.042 min
Delta R.T.: 0.006 min
Response: 43631001
Conc: 5.05 ng/u1