

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007143.D\VWD1A.CH Vial: 15
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007143.D\VWD1A.CH
 Acq On : 02-Dec-2014, 18:25 Operator: TP
 Sample : HSTDICCC005 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Dec 3 6:07 2014 Quant Results File: HN1202NG.RES

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
 Title :
 Last Update : Wed Dec 03 06:03:01 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	20428573	5.020 ng/ul
Target Compounds			
2) T Nitroglycerin	6.02	43174969	4.999 ng/ul

 Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN007143.D HN1202NG.M Wed Dec 31 17:35:48 2014



Quantitation Report


Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007143.D\VWD1A.CH Vial: 15
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN120214\HN007143.D\VWD1A.CH
 Acq On : 02-Dec-2014, 18:25 Operator: TP
 Sample : HSTDICCC005 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Dec 3 6:07 2014 Quant Results File: HN1202NG.RES

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
 Title :
 Last Update : Wed Dec 03 06:03:01 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

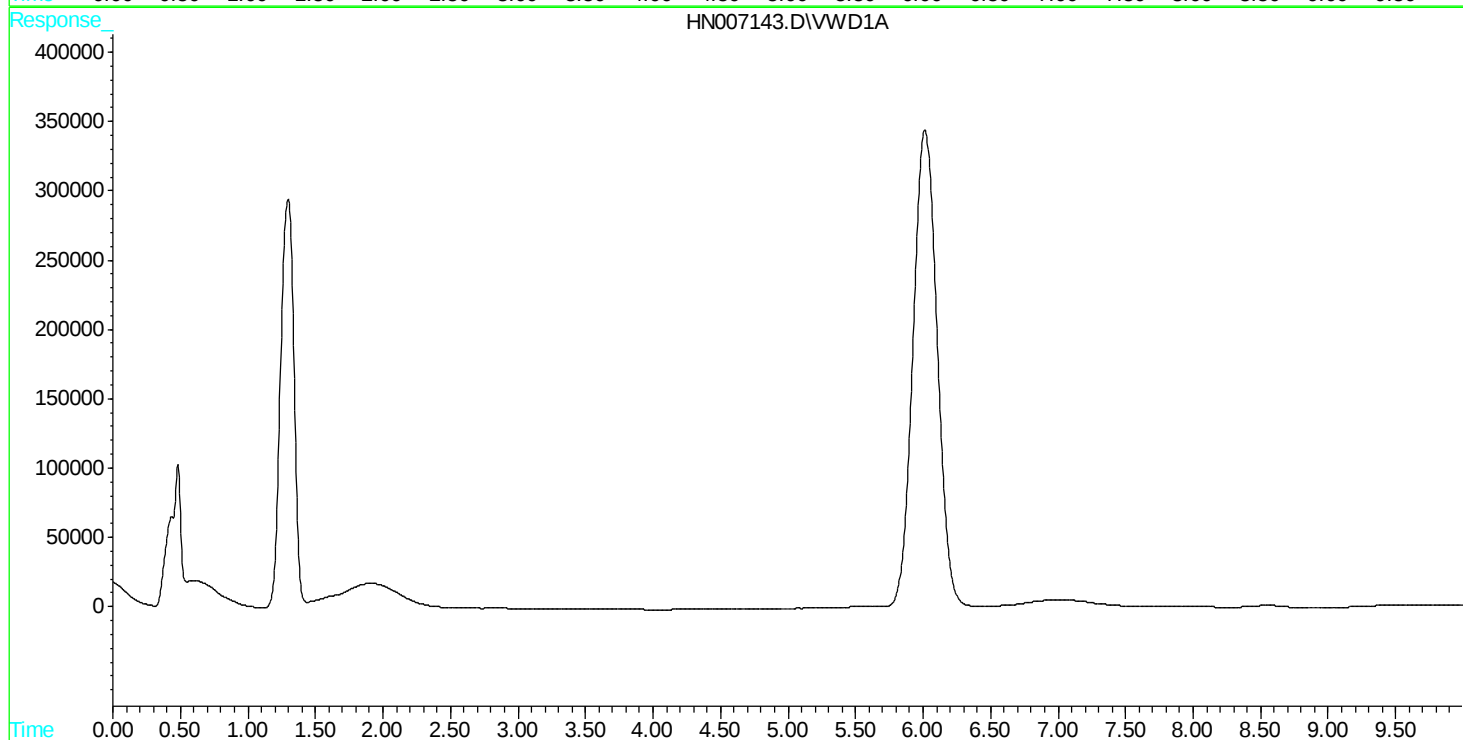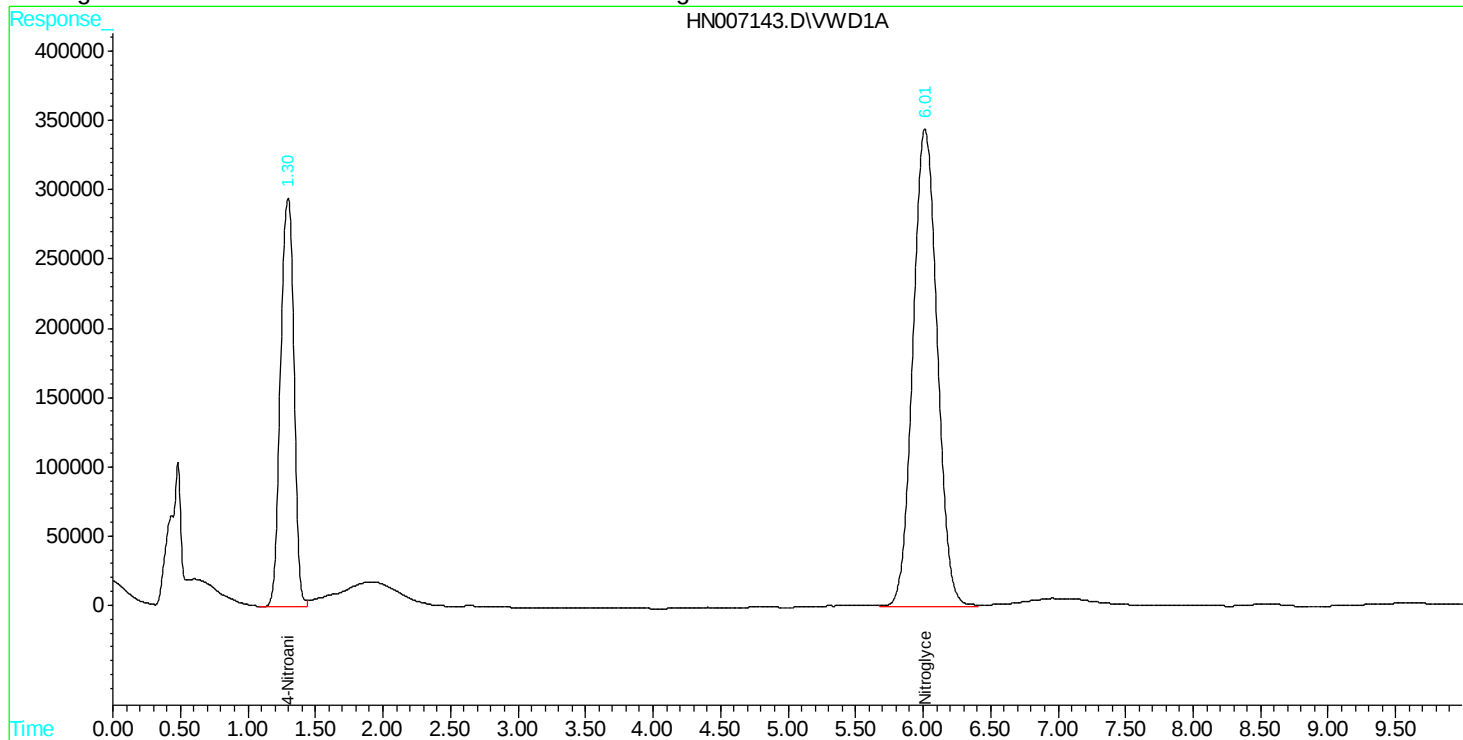


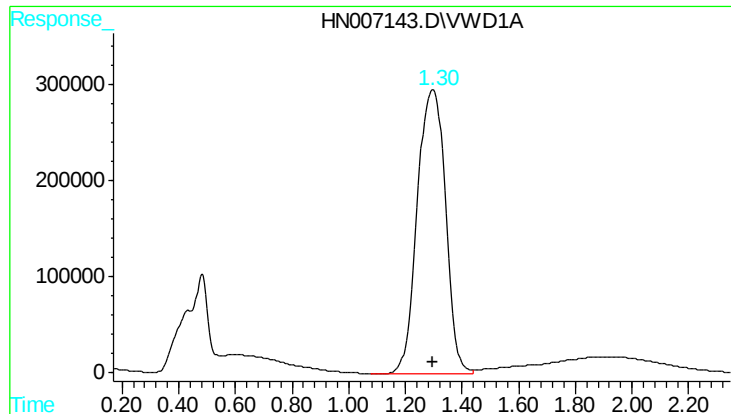

#1 4-Nitroaniline

R.T.: 1.298 min
Delta R.T.: 0.000 min
Response: 20428573
Conc: 5.02 ng/u1

Instrument :
HPLC_N
ClientSampleId :
HSTDICCC005

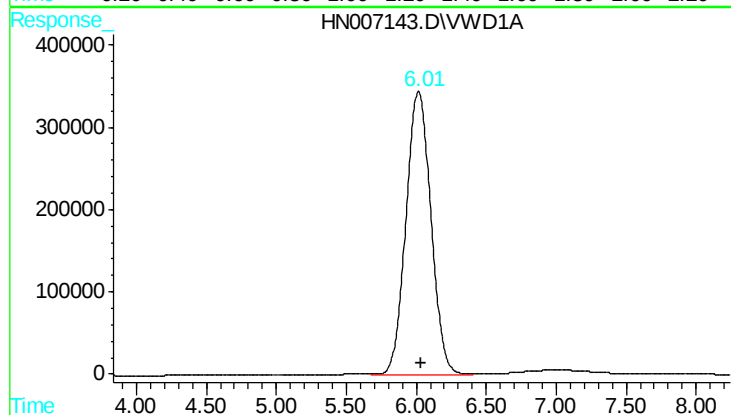

#2 Nitroglycerin

R.T.: 6.016 min
Delta R.T.: -0.019 min
Response: 43174969
Conc: 5.00 ng/u1