

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN120415\
 Data File : HN007627.D
 Signal(s) : vwd1A.ch
 Acq On : 04-Dec-2015, 16:21
 Operator : UM/MA
 Sample : SSTDICC010
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 SSTDICC010

Integration File: AUTOINT1.E
 Quant Time: Dec 04 17:12:07 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN1204NG.M
 Quant Title :
 QLast Update : Fri Dec 04 16:28:03 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 u1
 Signal Phase : ZORBAX Extend-C18
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.355	39205972	9.453 ng/u1
Target Compounds			
2) T Nitroglycerin	6.132	80757825	9.430 ng/u1

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN120415\
Data File : HN007627.D
Signal(s) : vwd1A.ch
Acq On : 04-Dec-2015, 16:21
Operator : UM/MA
Sample : SSTDICC010
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC010

Integration File: AUTOINT1.E
Quant Time: Dec 04 17:12:07 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN1204NG.M
Quant Title :
QLast Update : Fri Dec 04 16:28:03 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

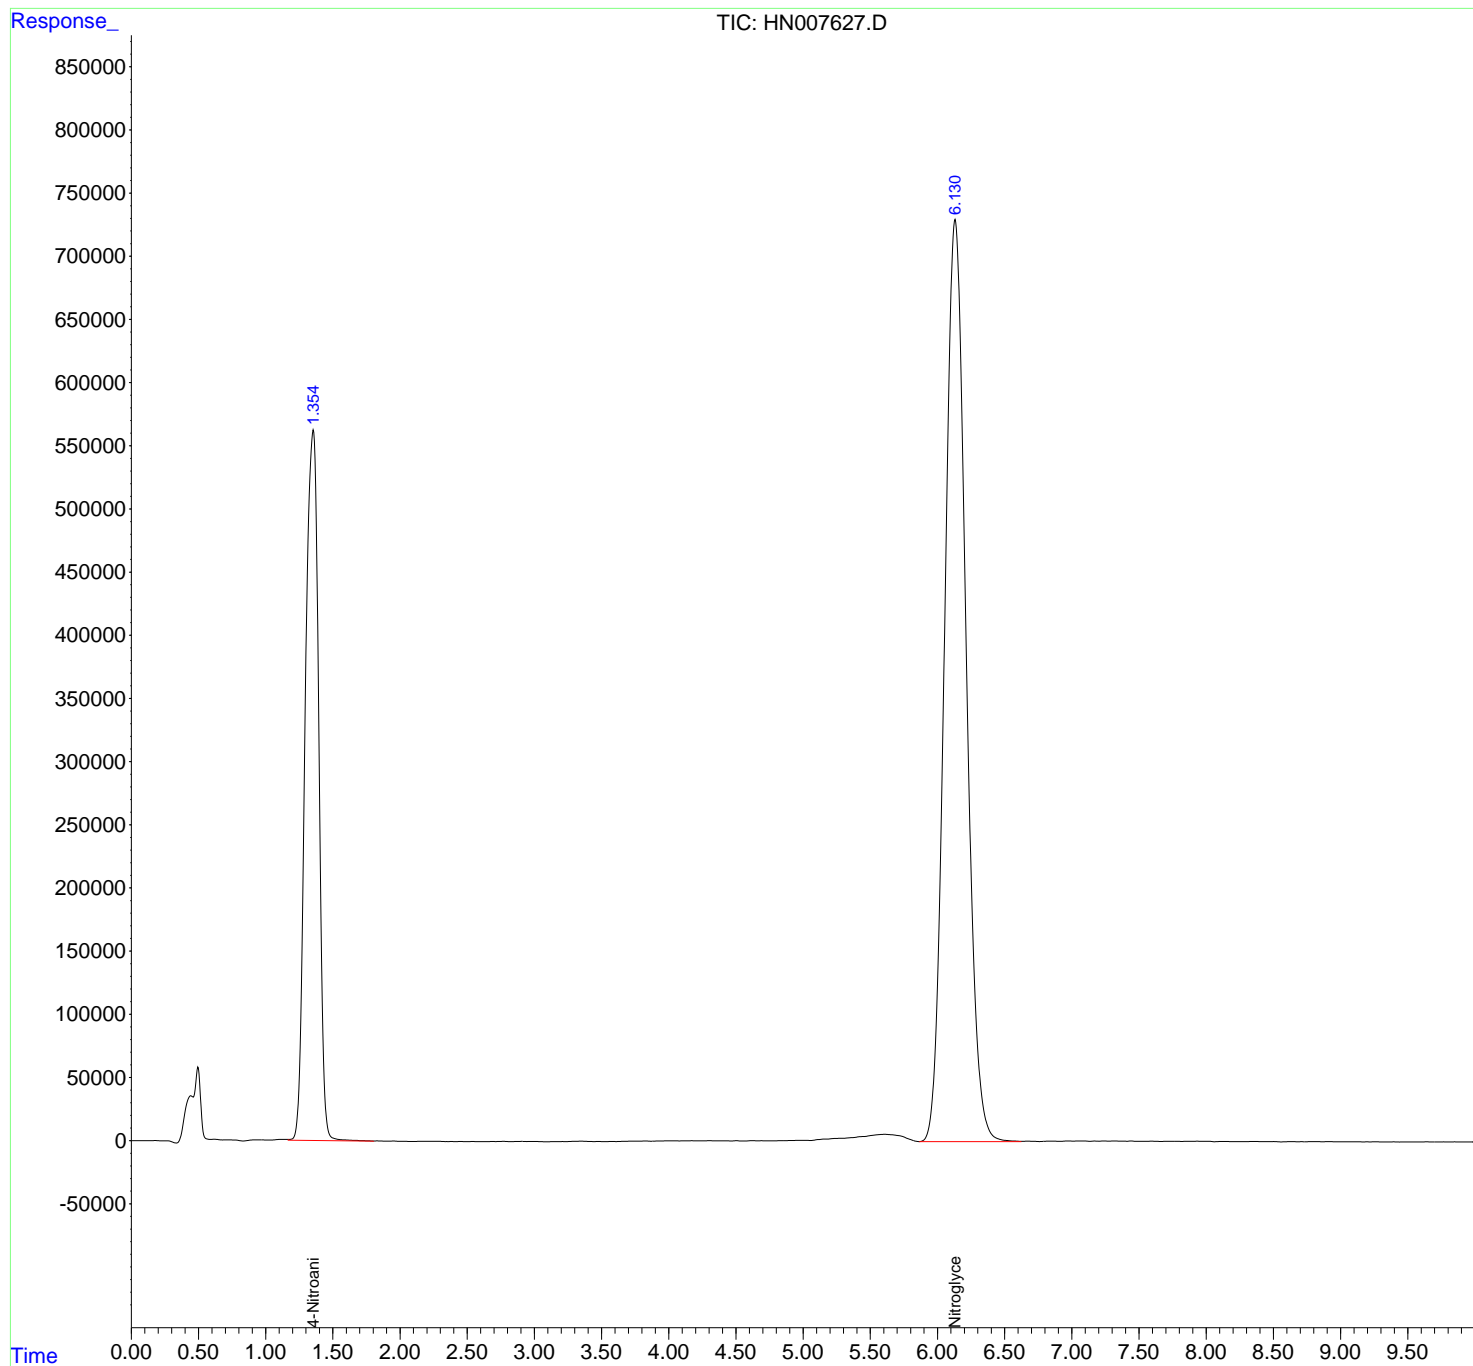


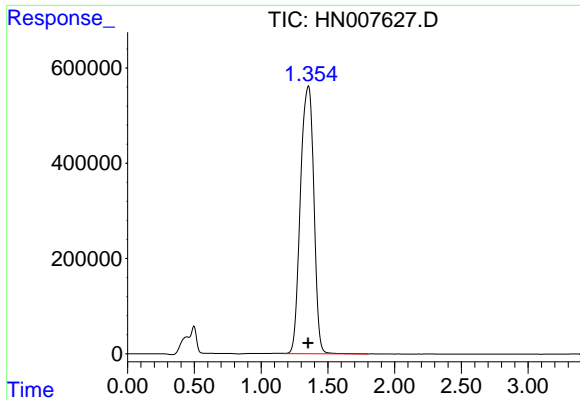

#1 4-Nitroaniline

R.T.: 1.355 min
Delta R.T.: 0.003 min
Response: 39205972
Conc: 9.45 ng/u1

Instrument :
HPLC_N
ClientSampleId :
SSTDIC010

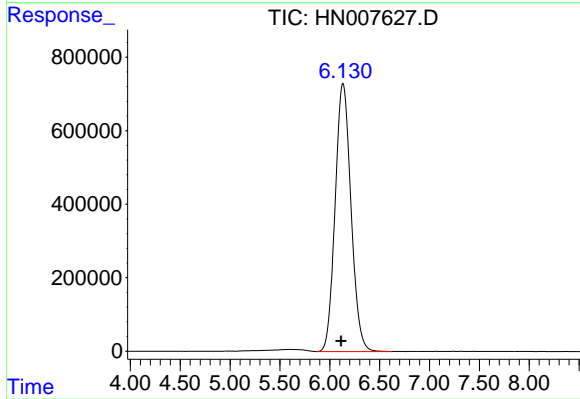

#2 Nitroglycerin

R.T.: 6.132 min
Delta R.T.: 0.020 min
Response: 80757825
Conc: 9.43 ng/u1