

Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN121014\HN007152.D Vial: 5  
Acq On : 10-Dec-2014, 19:46 Operator: TP  
Sample : BL-LOD/LOQ-WATER Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile : autoint1.e  
Quant Time: Dec 11 3:58 2014 Quant Results File: HN120214.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
BL-LOD/LOQ-WATER

Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN120214.M  
Title :  
Last Update : Tue Dec 02 14:51:46 2014  
Response via : Initial Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
Signal Phase : ZORBAX Extend-C18  
Signal Info : 4.6 X 100mm 3.5-Micron 80A

| Compound                    | R.T. | Response | Conc Units     |
|-----------------------------|------|----------|----------------|
| -----                       |      |          |                |
| System Monitoring Compounds |      |          |                |
| 1) S 4-Nitroaniline         | 1.31 | 657003   | 156.845 ug/L m |
| Target Compounds            |      |          |                |

-----  
Analyst Signature: \_\_\_\_\_ Analyst Name: \_\_\_\_\_ Date: \_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #: \_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #: \_\_\_\_\_

\_\_\_OTHER: \_\_\_\_\_ Compound #: \_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN007152.D HN120214.M Fri Dec 12 13:39:10 2014


# Quantitation Report


Data File : Z:\HPCHEM1\HPLC\_N\DATA\HN121014\HN007152.D Vial: 5  
 Acq On : 10-Dec-2014, 19:46 Operator: TP  
 Sample : BL-LOD/LOQ-WATER Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile : autoint1.e  
 Quant Time: Dec 11 3:58 2014 Quant Results File: HN120214.RES

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 BL-LOD/LOQ-WATER

Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN120214.M  
 Title :  
 Last Update : Tue Dec 02 14:51:46 2014  
 Response via : Multiple Level Calibration  
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
 Signal Phase : ZORBAX Extend-C18  
 Signal Info : 4.6 X 100mm 3.5-Micron 80A

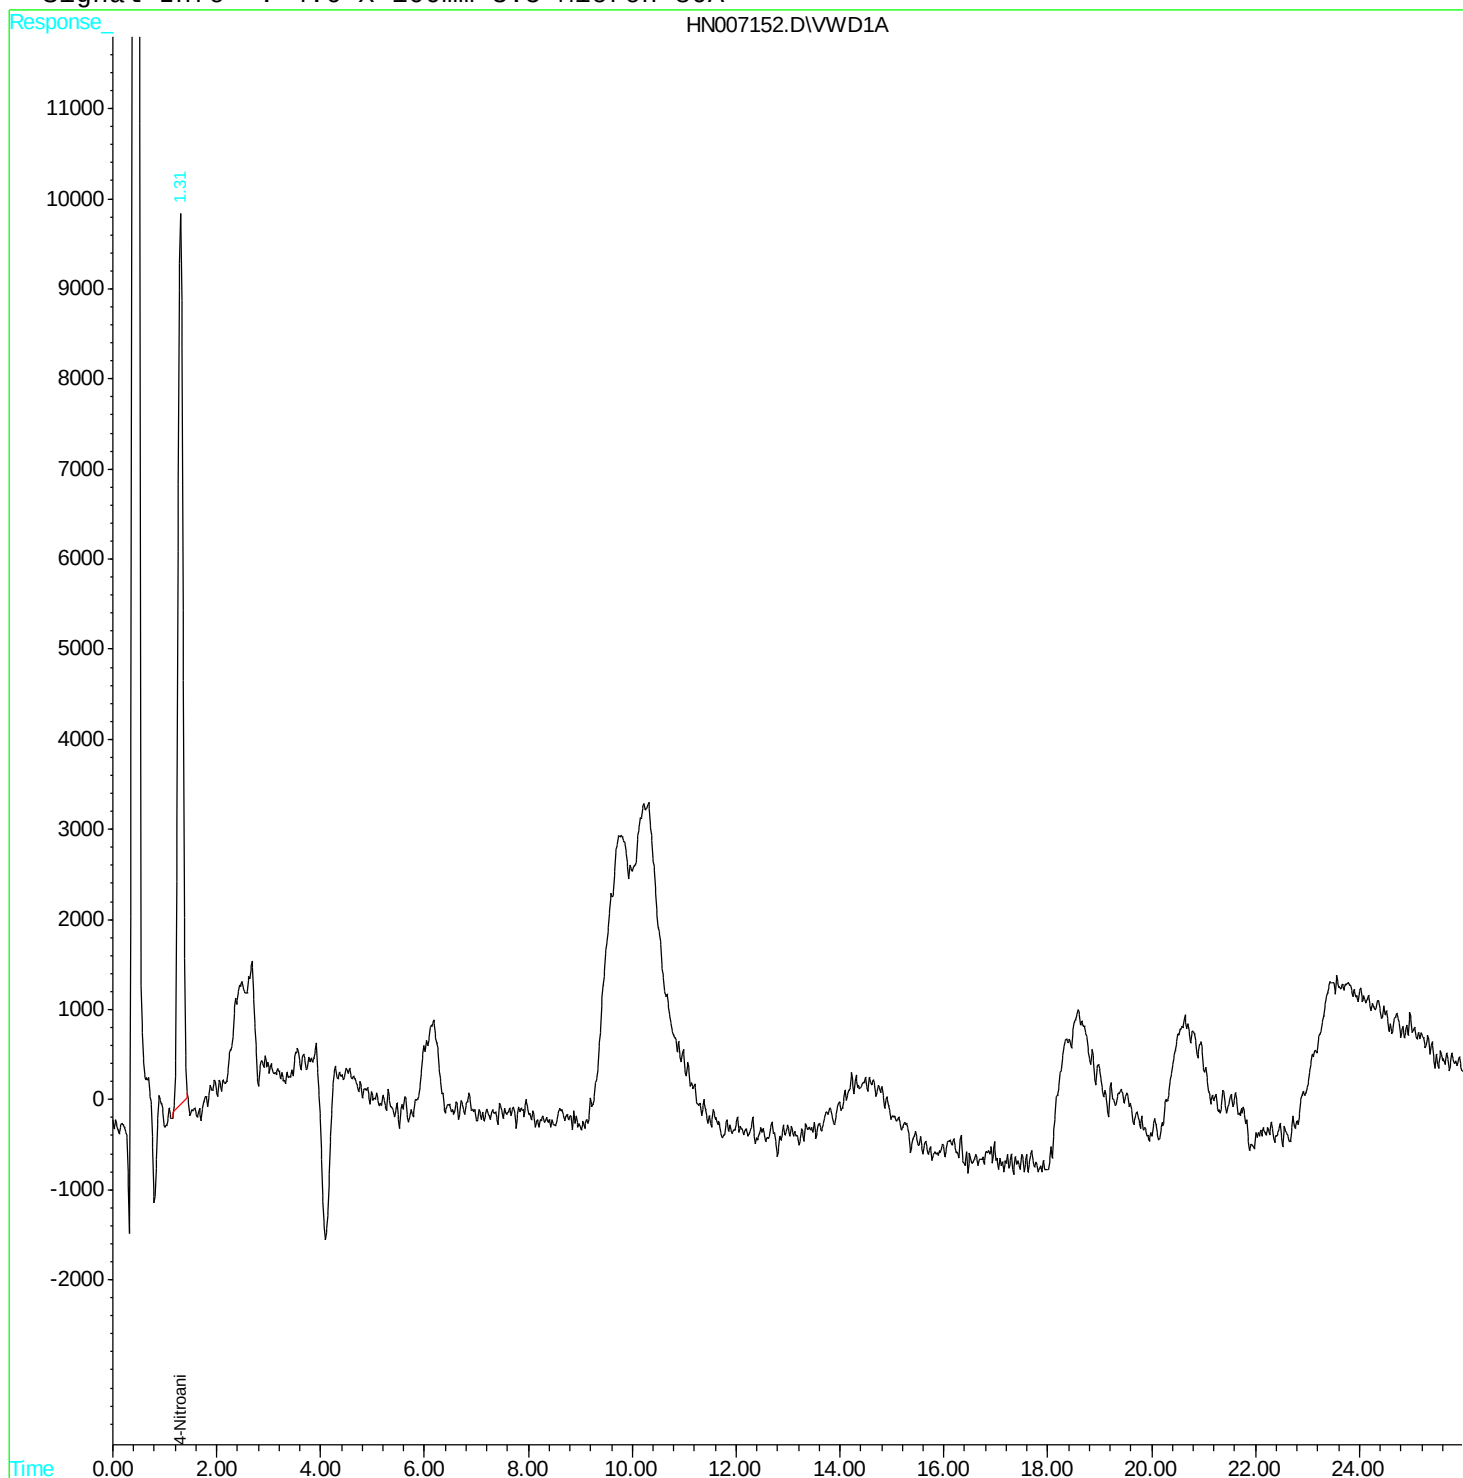

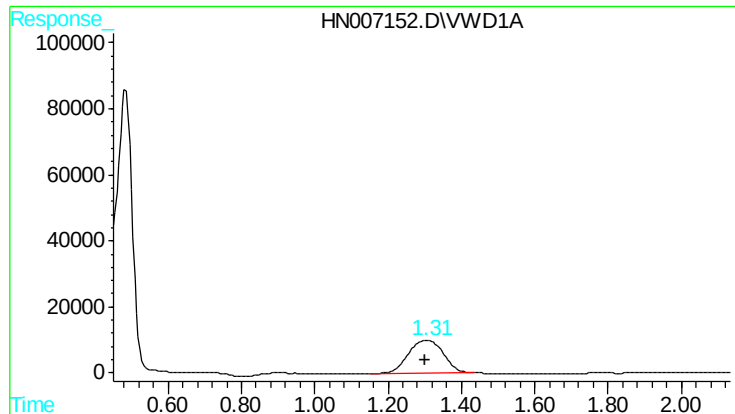

#1 4-Nitroaniline

R.T.: 1.306 min  
Delta R.T.: 0.007 min  
Response: 657003  
Conc: 156.84 ug/L m

Instrument :  
HPLC\_N  
ClientSampleId :  
BL-LOD/LOQ-WATER