

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN121014\HN007156.D Vial: 8
Acq On : 10-Dec-2014, 21:38 Operator: TP
Sample : HSTDCCC005 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Dec 11 4:08 2014 Quant Results File: HN1202NG.RES

Instrument :
HPLC_N
LabSampleId :
HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
Title :
Last Update : Wed Dec 03 06:05:17 2014
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.31	20133039	4.947 ng/ul
Target Compounds			
2) T Nitroglycerin	6.08	43154959	4.997 ng/ul

Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.


HN007156.D HN1202NG.M Fri Dec 12 13:40:08 2014


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN121014\HN007156.D Vial: 8
Acq On : 10-Dec-2014, 21:38 Operator: TP
Sample : HSTDCCC005 Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Dec 11 4:08 2014 Quant Results File: HN1202NG.RES

Instrument :
HPLC_N
LabSampleId :
HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
Title :
Last Update : Wed Dec 03 06:05:17 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

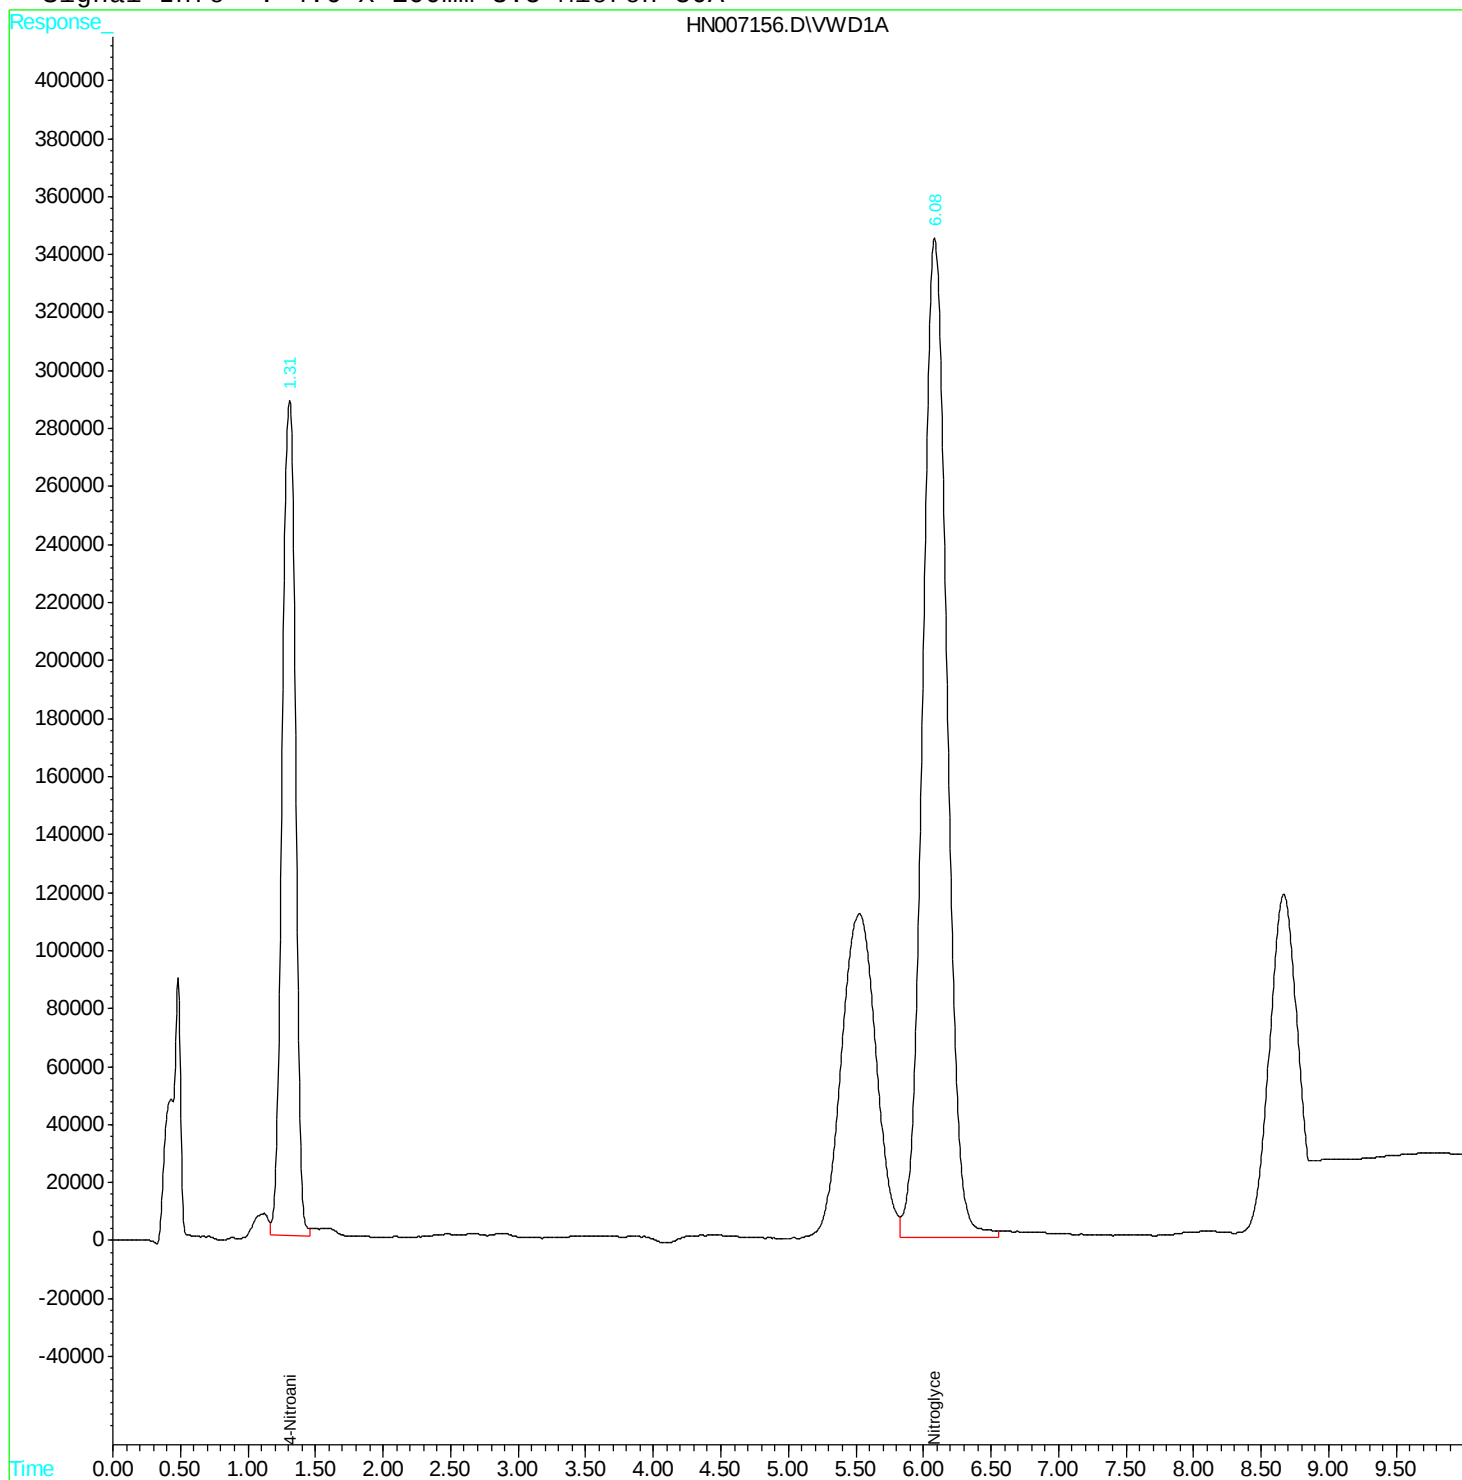


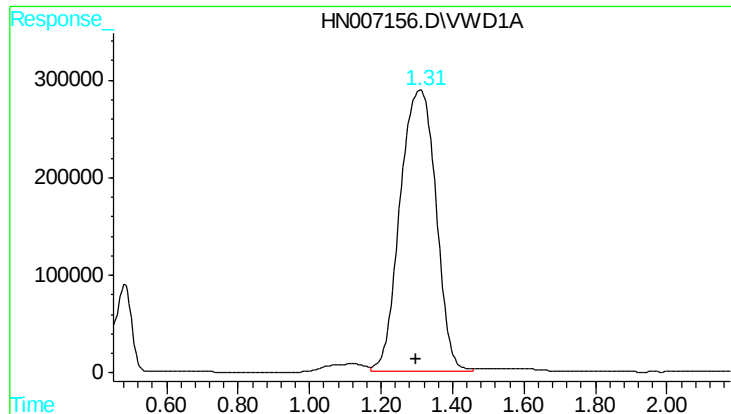

#1 4-Nitroaniline

R.T.: 1.310 min
Delta R.T.: 0.012 min
Response: 20133039
Conc: 4.95 ng/u1

Instrument :
HPLC_N
LabSampleId :
HSTDCCC005

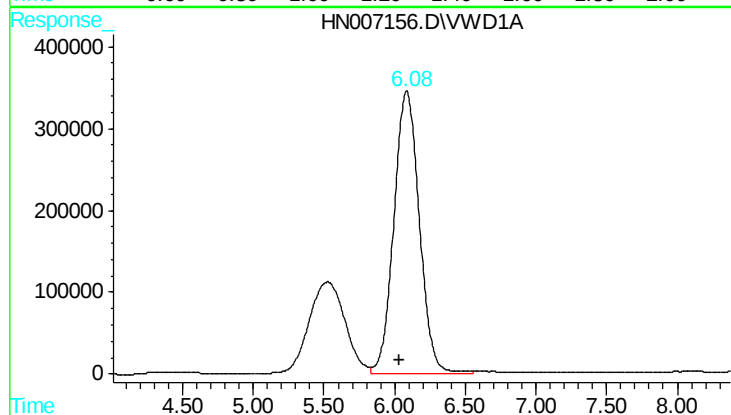

#2 Nitroglycerin

R.T.: 6.085 min
Delta R.T.: 0.050 min
Response: 43154959
Conc: 5.00 ng/u1