

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN121014\HN007160.D Vial: 12
Acq On : 10-Dec-2014, 22:26 Operator: TP
Sample : BL-LOD/LOQ-WATER Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Dec 11 4:15 2014 Quant Results File: HN1202NG.RES

Instrument :
HPLC_N
ClientSampleId :
BL-LOD/LOQ-WATER

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
Title :
Last Update : Wed Dec 03 06:05:17 2014
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.31	753587	0.185 ng/ul
Target Compounds			

Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.


HN007160.D HN1202NG.M Fri Dec 12 13:40:45 2014


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN121014\HN007160.D Vial: 12
Acq On : 10-Dec-2014, 22:26 Operator: TP
Sample : BL-LOD/LOQ-WATER Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Dec 11 4:15 2014 Quant Results File: HN1202NG.RES

Instrument :
HPLC_N
ClientSampleId :
BL-LOD/LOQ-WATER

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
Title :
Last Update : Wed Dec 03 06:05:17 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

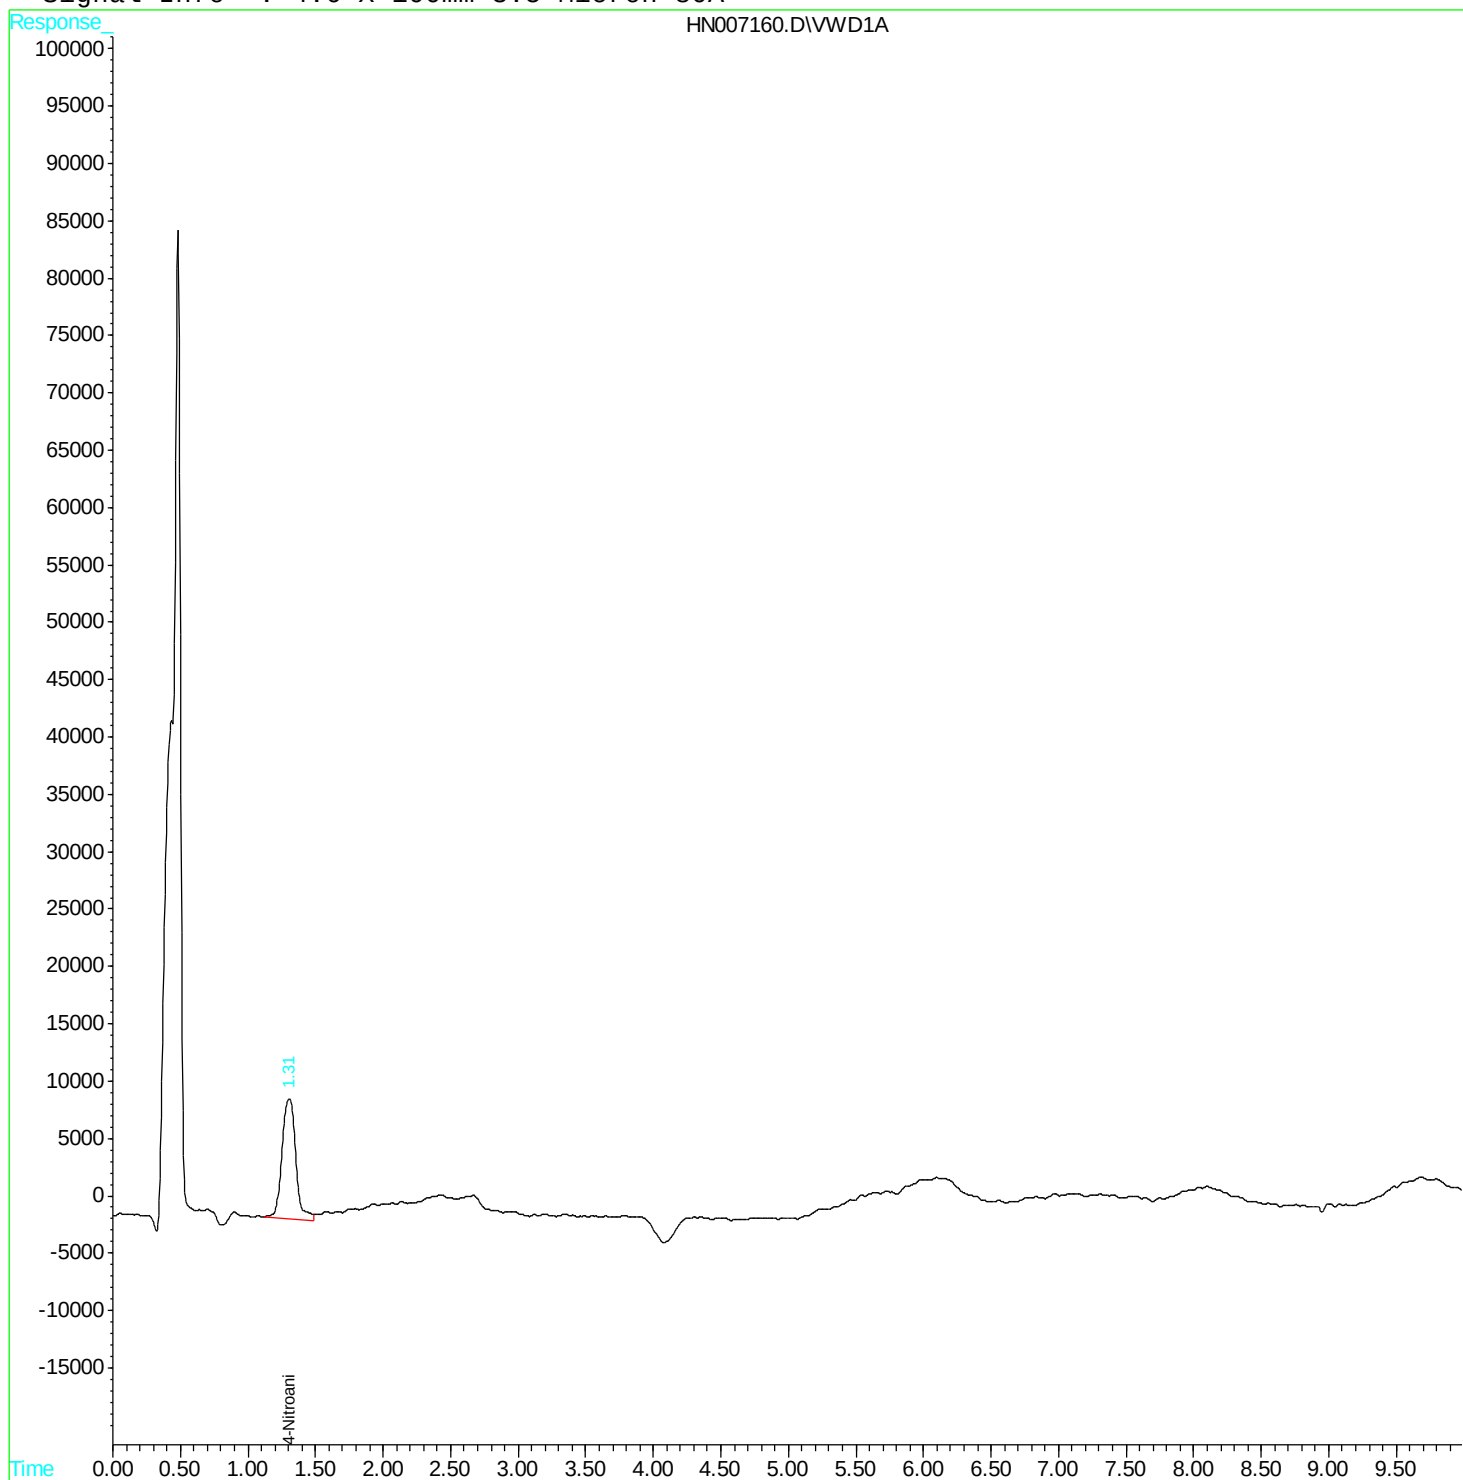

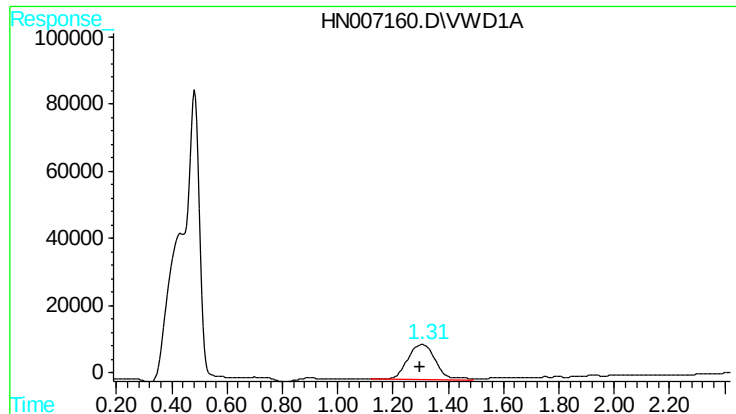

#1 4-Nitroaniline

R.T.: 1.308 min
Delta R.T.: 0.010 min
Response: 753587
Conc: 0.19 ng/ul

Instrument :
HPLC_N
ClientSampleId :
BL-LOD/LOQ-WATER