

Data File : Z:\HPCHEM1\HPLC_N\DATA\HN121014\HN007161.D Vial: 13
Acq On : 10-Dec-2014, 22:38 Operator: TP
Sample : LOQ-WATER-200ML Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Dec 11 7:33 2014 Quant Results File: HN1202NG.RES

Instrument :
HPLC_N
ClientSampleId :
LOQ-WATER-200ML

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
Title :
Last Update : Wed Dec 03 06:05:17 2014
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	680267	0.167 ng/ul
Target Compounds			
2) T Nitroglycerin	6.12	763910	0.088 ng/ulm

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____ Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.


HN007161.D HN1202NG.M Fri Dec 12 13:40:53 2014


Data File : Z:\HPCHEM1\HPLC_N\DATA\HN121014\HN007161.D Vial: 13
Acq On : 10-Dec-2014, 22:38 Operator: TP
Sample : LOQ-WATER-200ML Inst : G1314A
Misc : Multiplr: 1.00
IntFile : AUTOINT1.E
Quant Time: Dec 11 7:33 2014 Quant Results File: HN1202NG.RES

Instrument :
HPLC_N
ClientSampleId :
LOQ-WATER-200ML

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1202NG.M
Title :
Last Update : Wed Dec 03 06:05:17 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

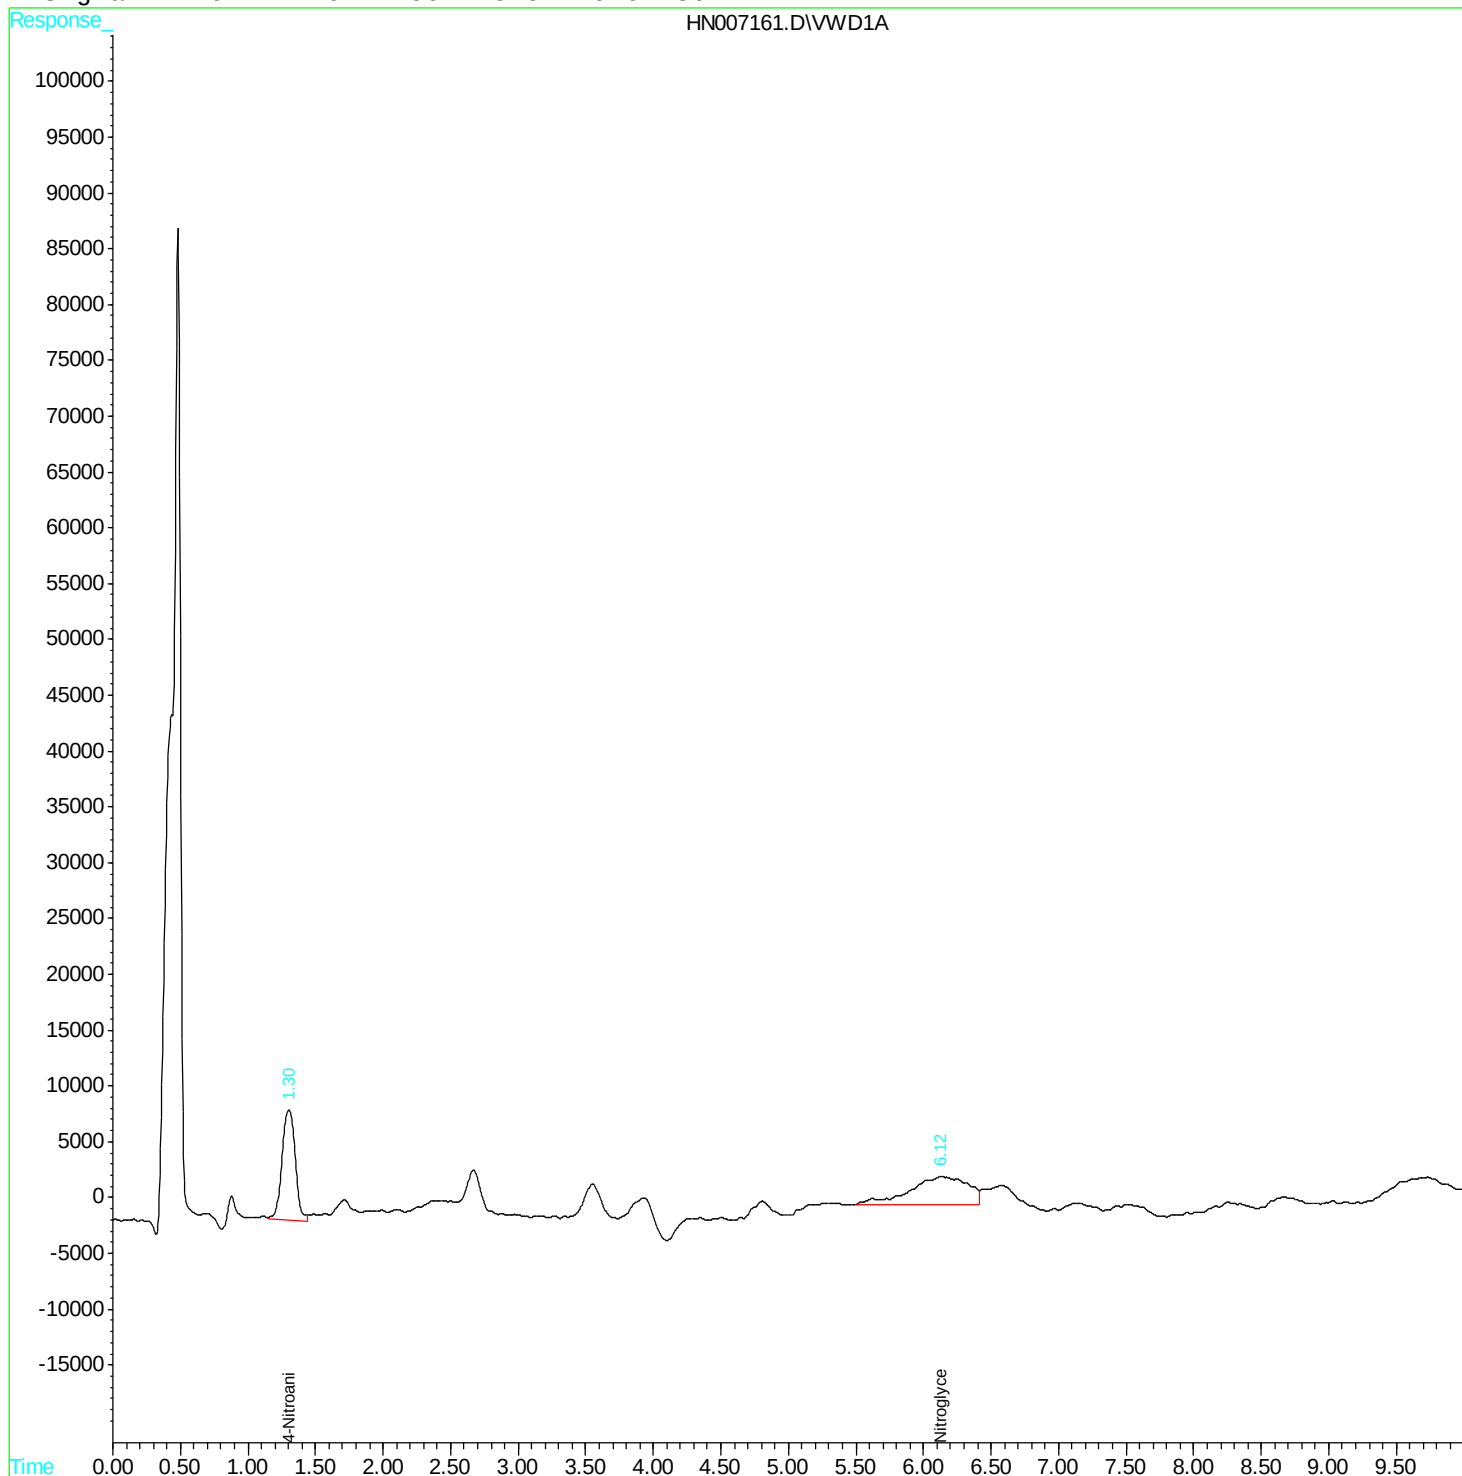


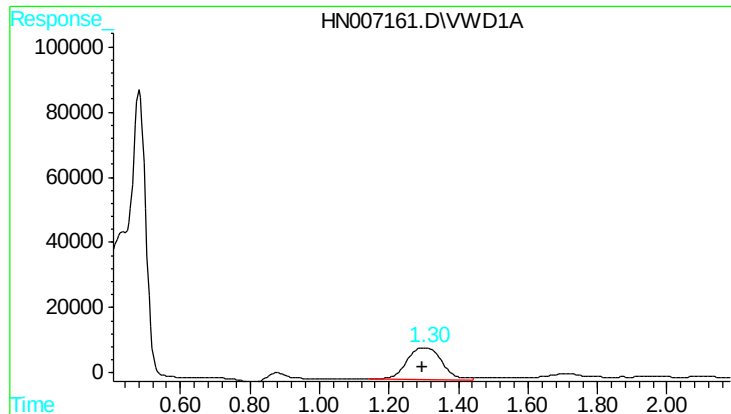

#1 4-Nitroaniline

R.T.: 1.304 min
Delta R.T.: 0.006 min
Response: 680267
Conc: 0.17 ng/ul

Instrument :
HPLC_N
ClientSampleId :
LOQ-WATER-200ML

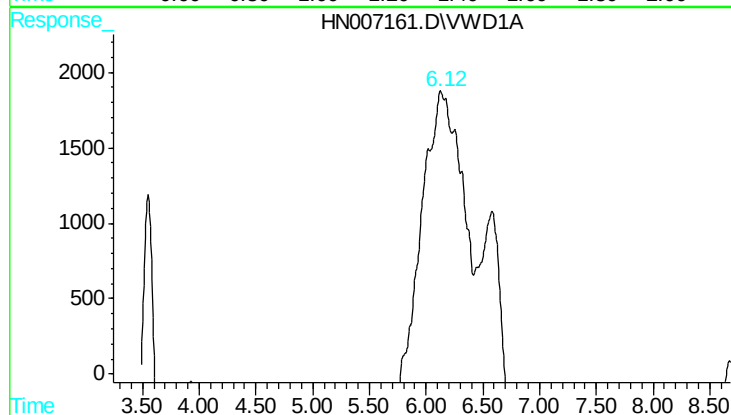

#2 Nitroglycerin

R.T.: 6.123 min
Delta R.T.: 0.088 min
Response: 763910
Conc: 0.09 ng/ul m