


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN010220\
Data File : BN009288.D
Acq On : 02 Jan 2020 10:45
Operator : JU
Sample : K6466-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0BP0

Manual Integrations
APPROVED

mohammad
1/2/2020 6:56:15 PM

Quant Time: Jan 02 12:47:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 02 12:44:14 2020
Response via : Initial Calibration

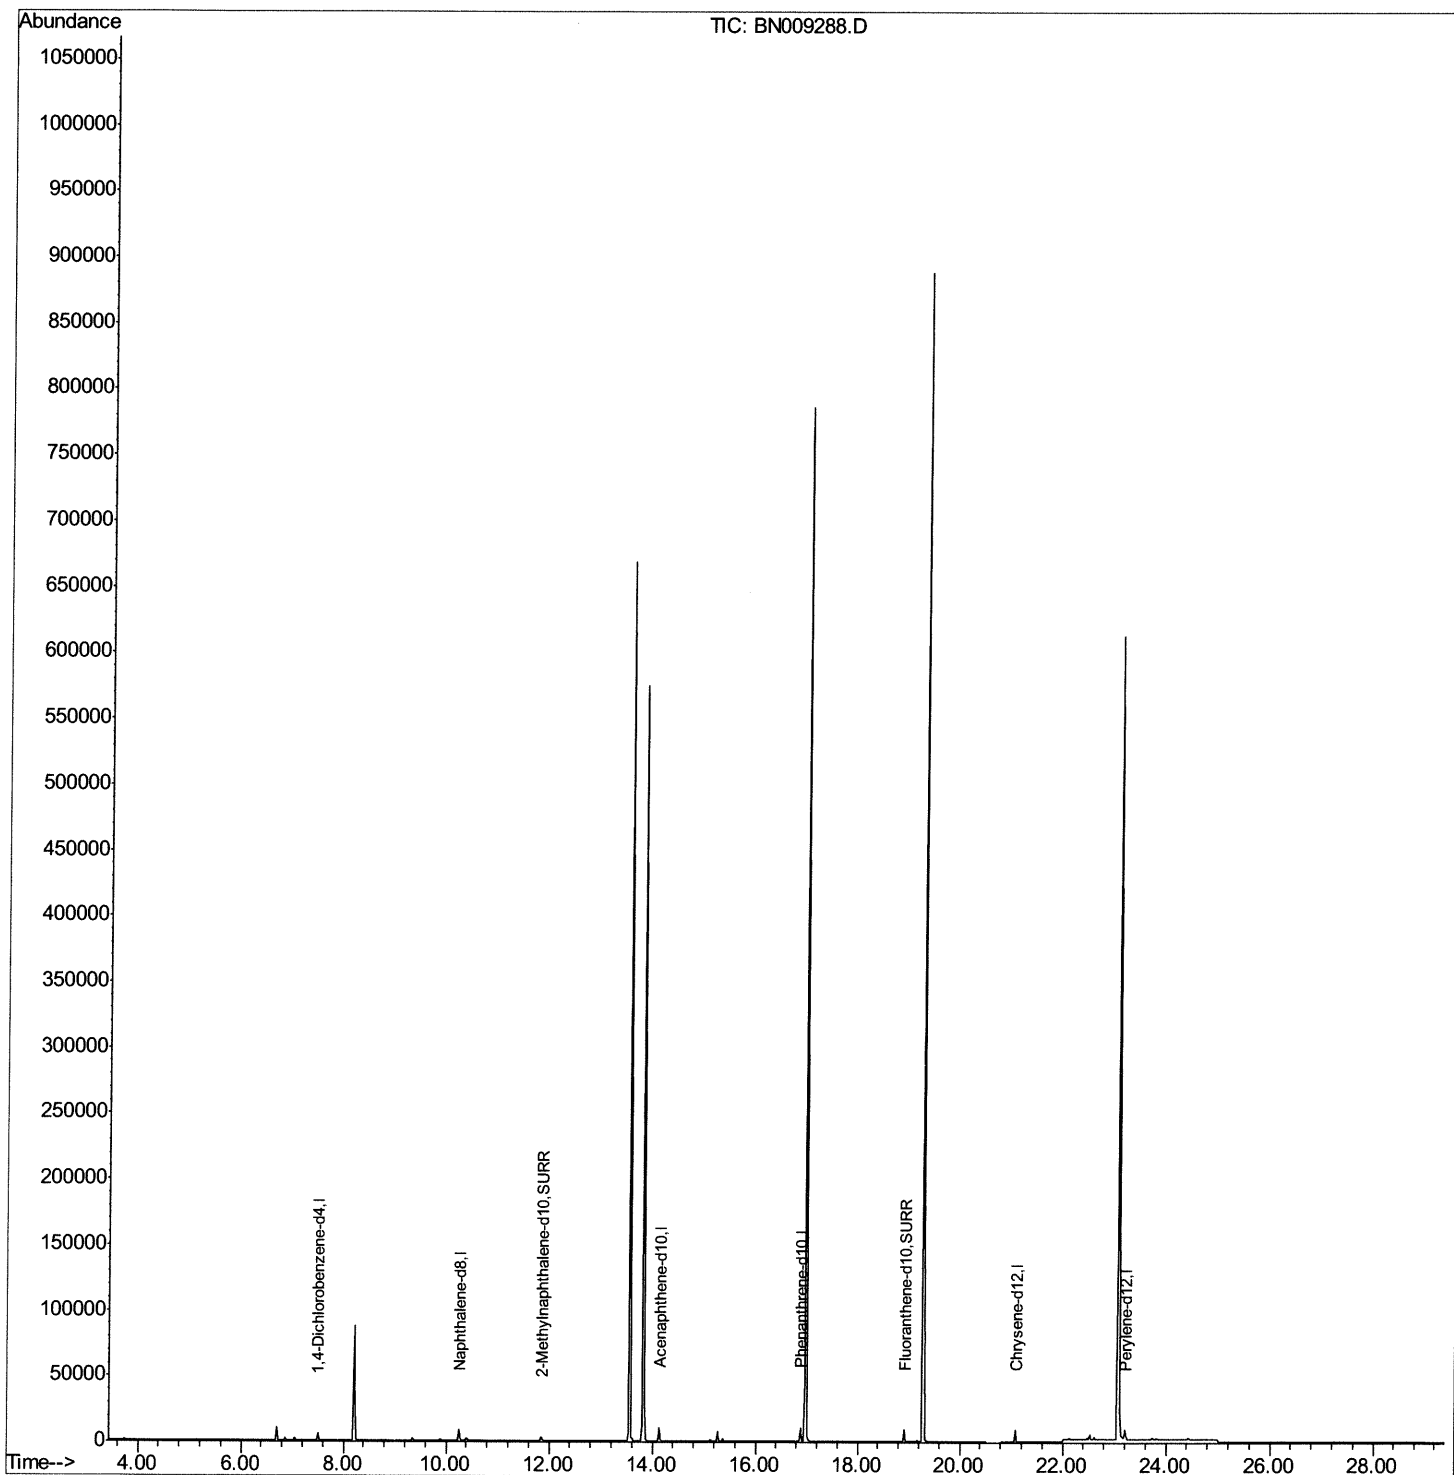

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN010220\
 Data File : BN009288.D
 Acq On : 02 Jan 2020 10:45
 Operator : JU
 Sample : K6466-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 H0BP0

Manual Integrations
APPROVED

mohammad
 1/2/2020 6:56:15 PM

Quant Time: Jan 02 12:46:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 02 12:44:14 2020
 Response via : Initial Calibration

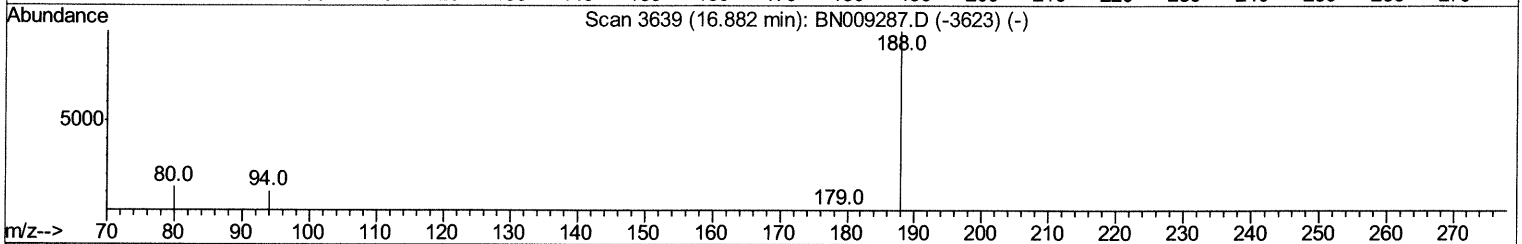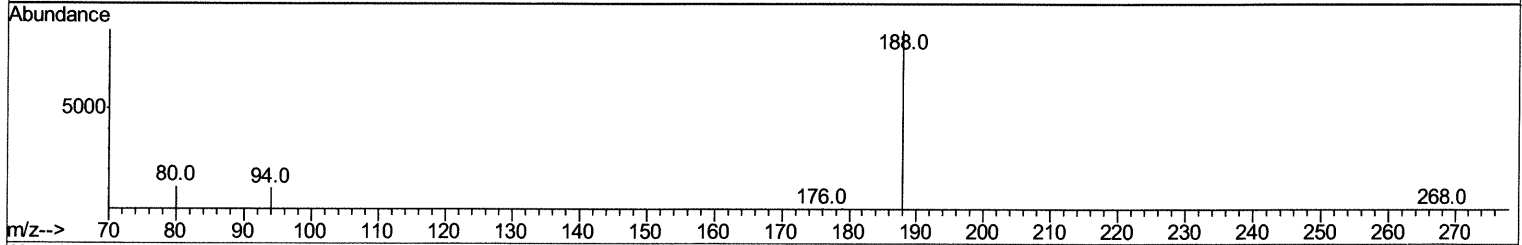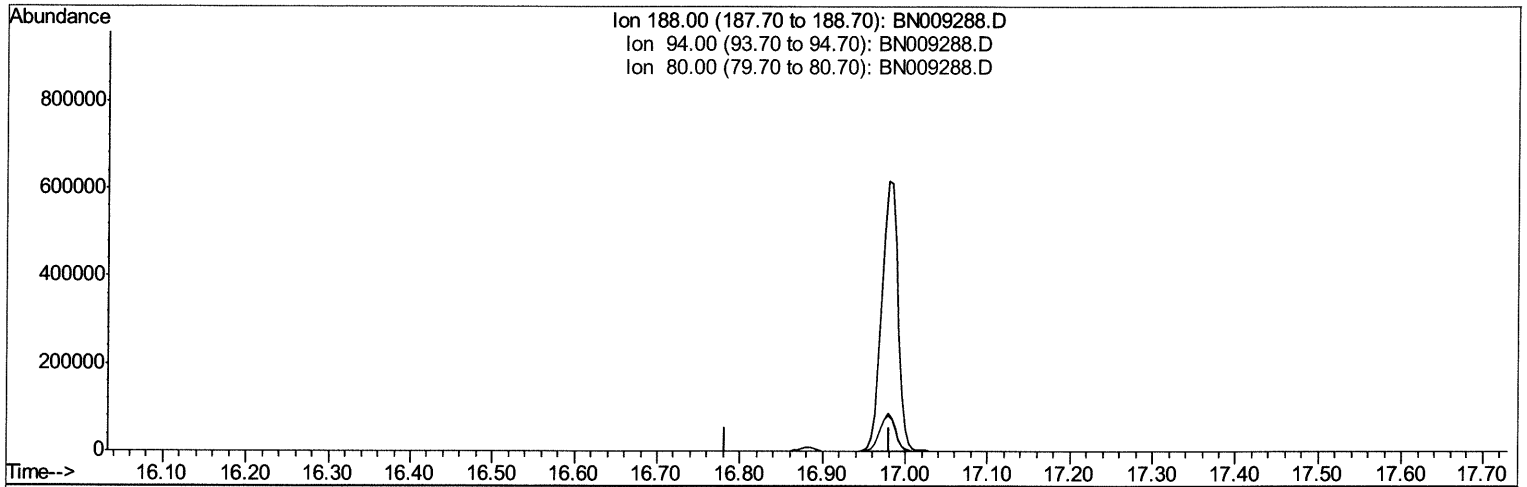

TIC: BN009288.D

(10) Phenanthrene-d10 (I)
 16.882min (-16.882) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN010220\
 Data File : BN009288.D
 Acq On : 02 Jan 2020 10:45
 Operator : JU
 Sample : K6466-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 H0BP0

Manual Integrations
APPROVED

mohammad
 1/2/2020 6:56:15 PM

Quant Time: Jan 02 12:46:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 02 12:44:14 2020
 Response via : Initial Calibration

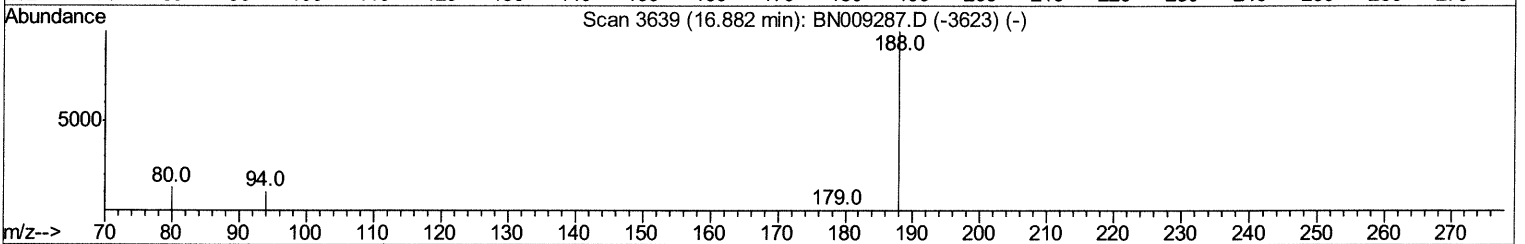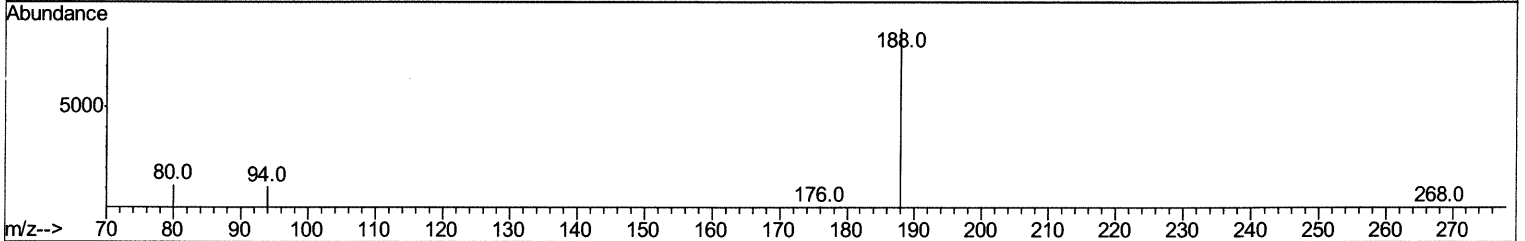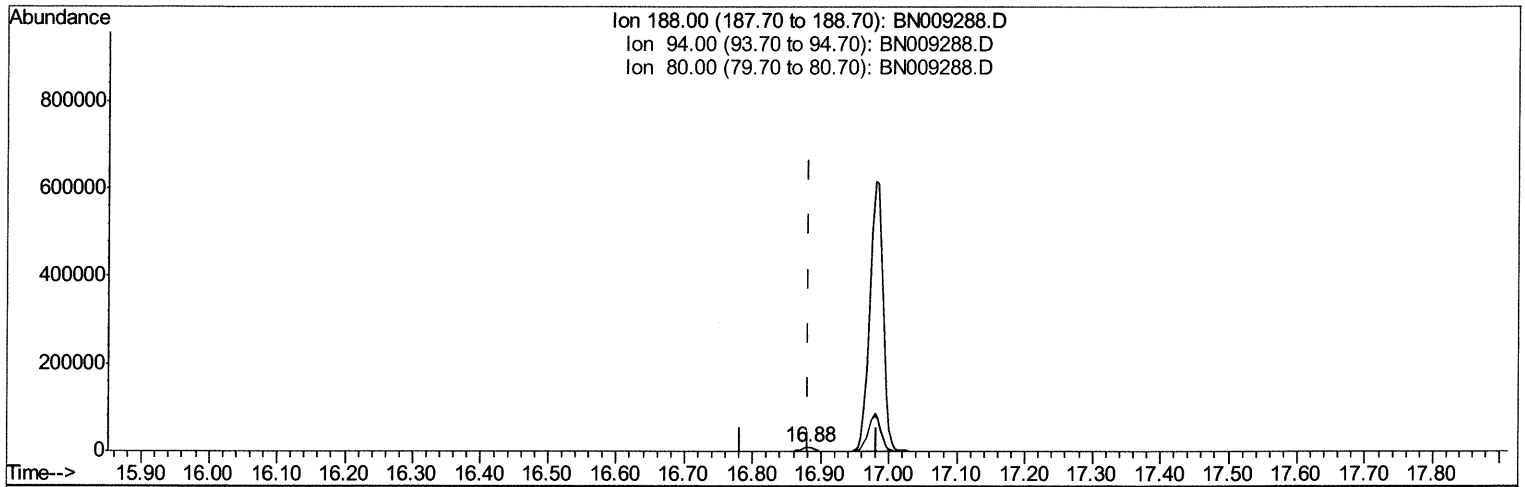

TIC: BN009288.D

(10) Phenanthrene-d10 (I)

16.882min (-0.000) 0.40ng/ul m *JU 01/13/20*

response 12090

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	11.88
80.00	13.70	13.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN010220\
 Data File : BN009288.D
 Acq On : 02 Jan 2020 10:45
 Operator : JU
 Sample : K6466-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0BP0

Manual Integrations
 APPROVED

mohammad
 1/2/2020 6:56:15 PM

Quant Time: Jan 02 12:47:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 02 12:44:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	2953	0.40	ng/ul	0.00
2) Naphthalene-d8	10.26	136	10719	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.13	164	5979	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.88	188	12090m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.08	240	8416	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	9089	0.40	ng/ul	0.00

JU 01/13/20

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.85	152	4619	0.24	ng/ul	0.00
14) Fluoranthene-d10	18.92	212	10420	0.29	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed