

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010422\
 Data File : BN018342.D
 Acq On : 04 Jan 2022 19:32
 Operator : CG/JU
 Sample : M5173-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3E5

Quant Time: Jan 05 01:02:20 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN010422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 04 13:43:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.598	152	6097	0.400	ng/ul	0.00
4) Naphthalene-d8	10.376	136	21154	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.239	164	16902	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.981	188	40671	0.400	ng/ul	0.00
17) Chrysene-d12	21.178	240	39498	0.400	ng/ul	0.00
23) Perylene-d12	23.391	264	44252	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.067	96	21426	3.881	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.976	152	13102	0.455	ng/ul	0.00
18) Fluoranthene-d10	19.016	212	53236	0.503	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.425	128	2583	0.045	ng/ul#	88
15) Phenanthrene	17.023	178	7395	0.057	ng/ul#	95
19) Fluoranthene	19.044	202	3370	0.024	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010422\
Data File : BN018342.D
Acq On : 04 Jan 2022 19:32
Operator : CG/JU
Sample : M5173-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3E5

Quant Time: Jan 05 01:02:20 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN010422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 04 13:43:36 2022
Response via : Initial Calibration




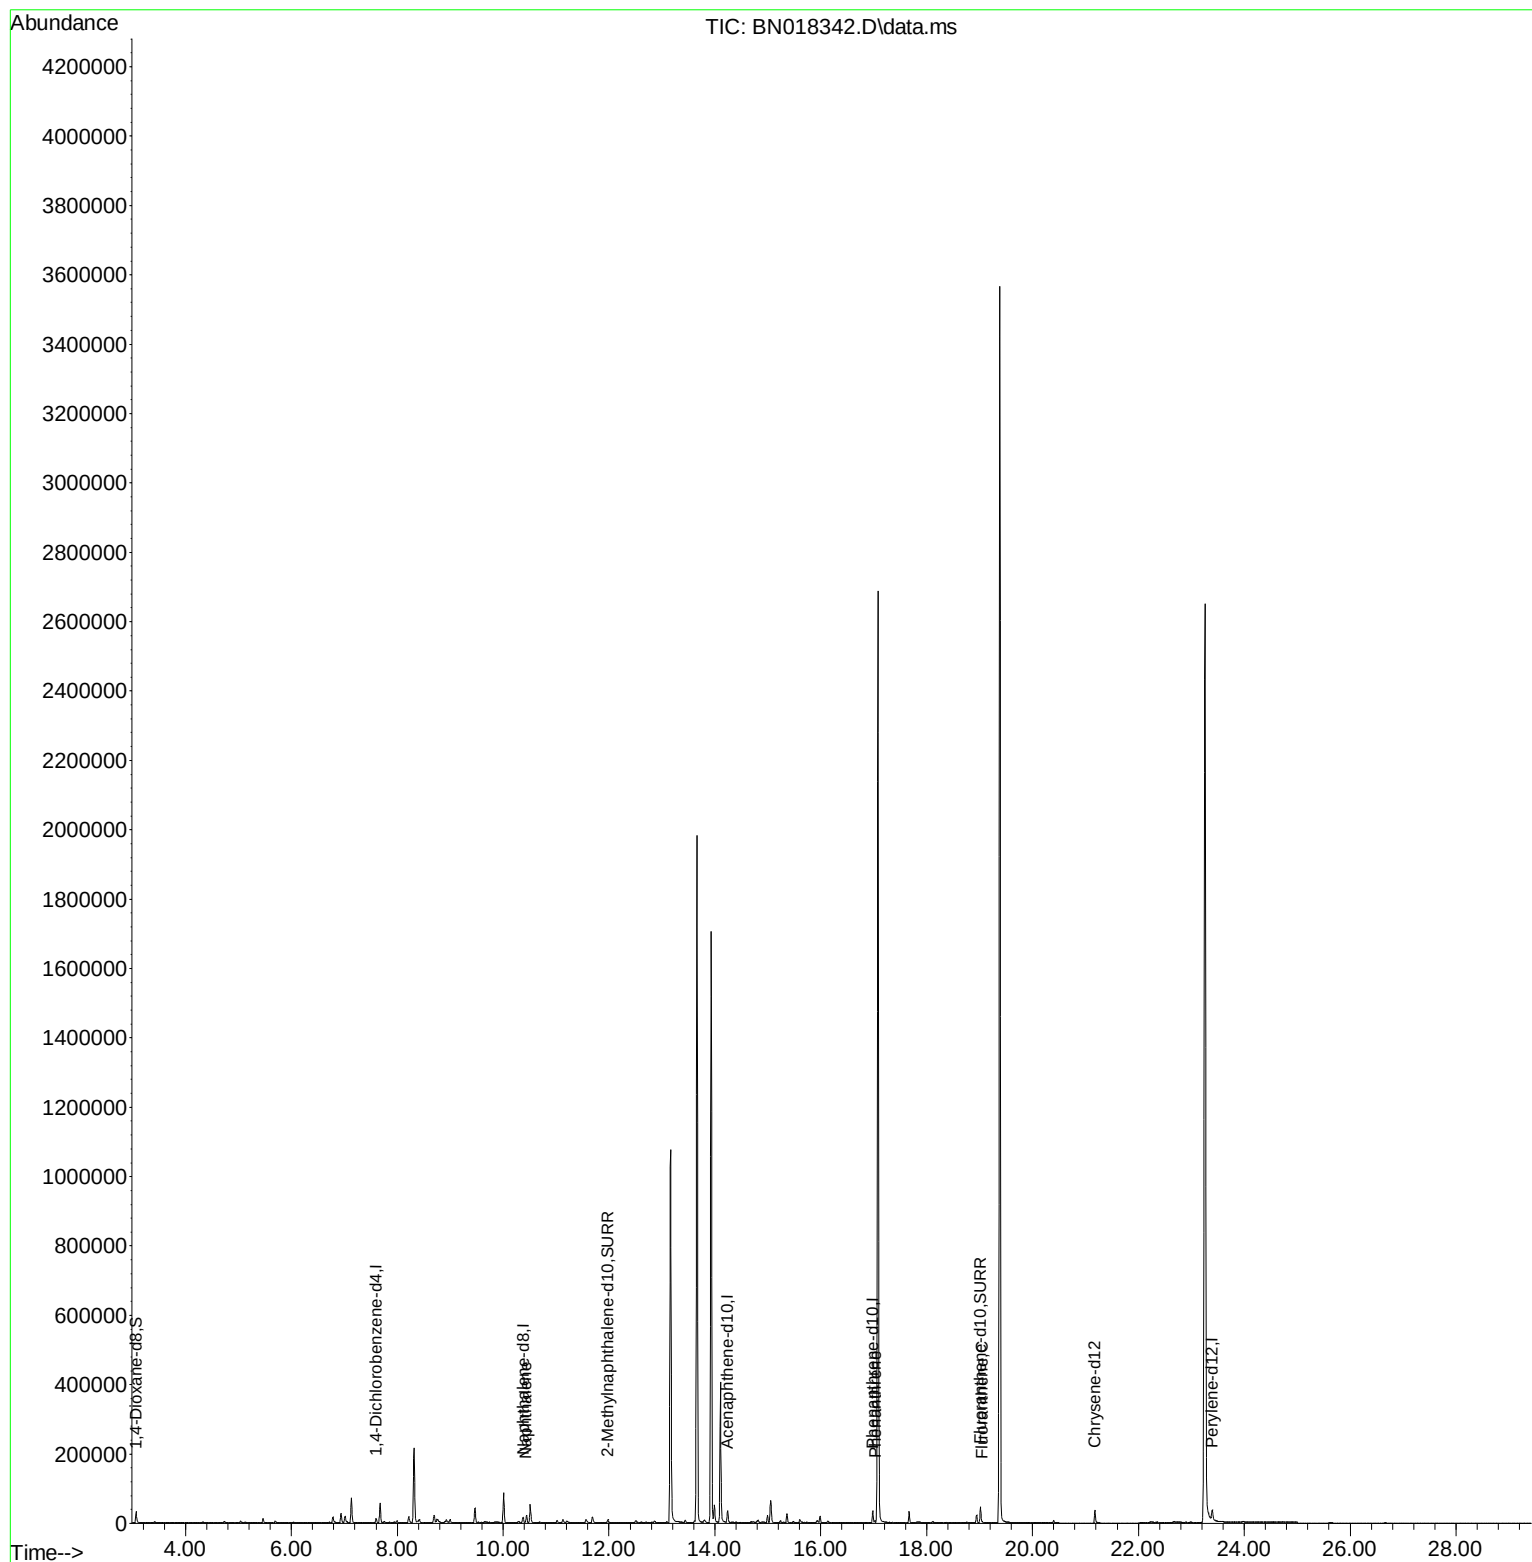


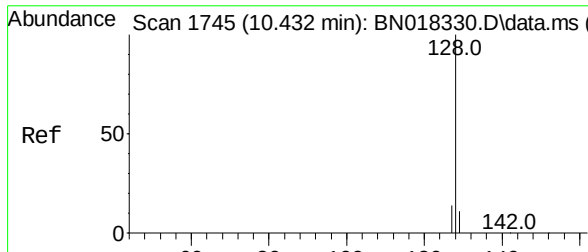

Scan 1745 (10.432 min): BN018330.D\data.ms (-1756) (-)
 Naphthalene
 Concen: 0.045 ng/ul
 RT: 10.425 min Scan# 1756
 Delta R.T. -0.007 min
 Lab File: BN018342.D
 Acq: 04 Jan 2022 19:32




Instrument :
 BNA_N
 ClientSampleId :
 BG3E5

Tgt Ion:	128	Resp:	2583
Ion	Ratio	Lower	Upper
128	100		
129	17.3	9.4	14.0#
127	17.4	11.0	16.6#

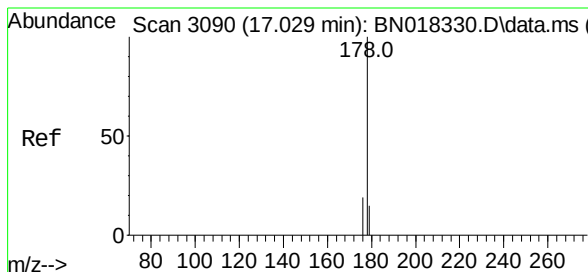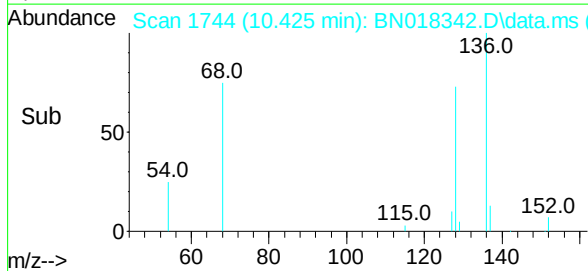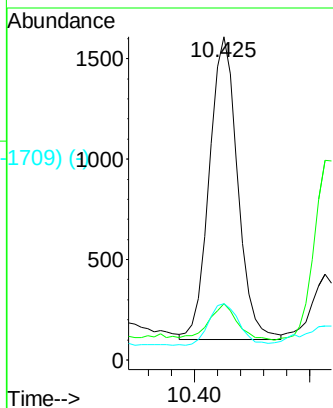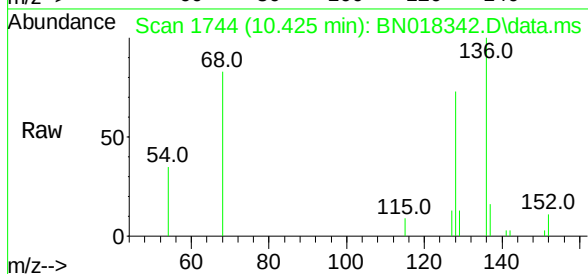


Scan 3090 (17.029 min): BN018330.D\data.ms (-30715) (-)
 Phenanthrene
 Concen: 0.057 ng/ul
 RT: 17.023 min Scan# 3089
 Delta R.T. -0.006 min
 Lab File: BN018342.D
 Acq: 04 Jan 2022 19:32

Tgt Ion:	178	Resp:	7395
Ion	Ratio	Lower	Upper
178	100		
179	18.7	12.2	18.4#
176	20.7	15.4	23.2

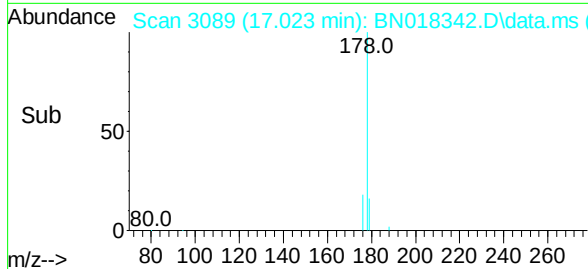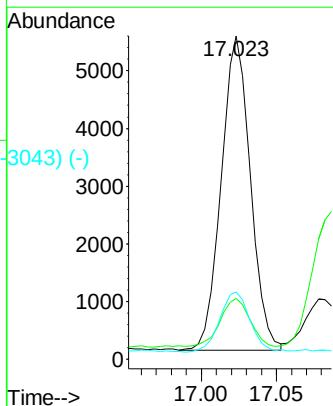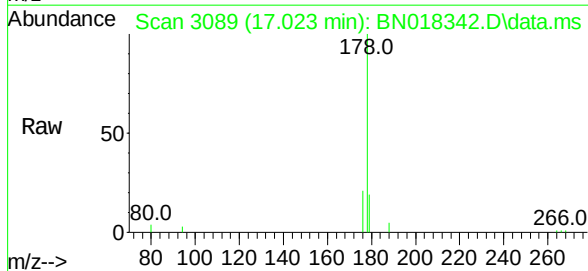

Abundance Scan 3557 (19.051 min): BN018330.D\data.ms (-3549) (-)

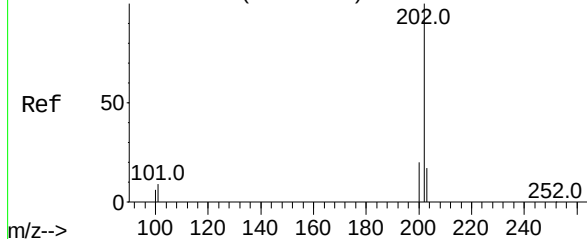

Fluoranthene

Concen: 0.024 ng/ul

RT: 19.044 min Scan#

Delta R.T. -0.006 min

Lab File: BN018342.D

Acq: 04 Jan 2022 19:32

Instrument :

BNA_N

ClientSampleId :

BG3E5

Tgt Ion:202 Resp: 3370

Ion Ratio Lower Upper

202 100

101 13.6 7.5 11.3#

100 12.1 5.4 8.2#

