

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010523\
 Data File : BN023564.D
 Acq On : 05 Jan 2023 11:52
 Operator : CG/JU
 Sample : PB149946BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK946

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023564.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	32	35	40	rBV	33064	46744	1.17%	0.105%
2	3.722	106	108	128	rBV	443442	772358	19.27%	1.737%
3	4.058	162	165	175	rVB2	11585	19099	0.48%	0.043%
4	7.105	676	683	692	rVB	646026	1001537	24.98%	2.252%
5	7.269	705	711	720	rBV	530986	816105	20.36%	1.835%
6	7.469	738	745	761	rVB	676793	1043348	26.02%	2.346%
7	7.946	819	826	834	rBV	654957	1050452	26.20%	2.362%
8	8.657	940	947	961	rBV	823458	1257328	31.36%	2.828%
9	9.116	1018	1025	1034	rBV	625812	1000426	24.95%	2.250%
10	9.840	1139	1148	1158	rBV	523744	837946	20.90%	1.884%
11	10.381	1232	1240	1250	rBV	818348	1316816	32.85%	2.961%
12	10.763	1296	1305	1313	rBV	988101	1645444	41.04%	3.700%
13	10.899	1322	1328	1340	rBV	840838	1397329	34.85%	3.142%
14	12.351	1567	1575	1580	rVB	15086	23407	0.58%	0.053%
15	12.928	1668	1673	1674	rBV2	3525	4413	0.11%	0.010%
16	13.869	1826	1833	1839	rBV4	4614	8886	0.22%	0.020%
17	14.010	1848	1857	1867	rBV	1502118	1976188	49.29%	4.444%
18	14.292	1898	1905	1916	rBV	1698662	2354138	58.72%	5.294%
19	14.598	1950	1957	1966	rBV	1565831	2296435	57.28%	5.164%
20	14.798	1984	1991	2006	rBV	747575	1013319	25.28%	2.279%
21	15.375	2084	2089	2093	rBV4	5122	9178	0.23%	0.021%
22	15.592	2116	2126	2133	rBV	2205248	3037232	75.76%	6.830%
23	15.710	2140	2146	2158	rBV	688359	866705	21.62%	1.949%
24	15.834	2163	2167	2170	rVB2	8978	10476	0.26%	0.024%
25	15.998	2191	2195	2200	rVB5	2958	4154	0.10%	0.009%
26	16.639	2300	2304	2309	rVB5	2650	4226	0.11%	0.010%
27	16.816	2330	2334	2340	rVB3	5953	8467	0.21%	0.019%
28	17.022	2366	2369	2374	rVB5	2601	4596	0.11%	0.010%
29	17.139	2384	2389	2392	rBV3	3923	5939	0.15%	0.013%
30	17.186	2392	2397	2400	rBV6	3718	5678	0.14%	0.013%
31	17.269	2406	2411	2413	rBV6	3611	5255	0.13%	0.012%
32	17.351	2418	2425	2435	rBV	2066661	2866240	71.49%	6.446%
33	17.451	2435	2442	2456	rBV	2328774	3298396	82.27%	7.418%
34	17.892	2512	2517	2522	rBV6	5396	10326	0.26%	0.023%
35	18.316	2587	2589	2592	rVB3	5519	4054	0.10%	0.009%
36	18.833	2673	2677	2682	rBV5	6092	8640	0.22%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010523\
Data File : BN023564.D
Acq On : 05 Jan 2023 11:52
Operator : CG/JU
Sample : PB149946BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK946

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Title : SVOA CALIBRATION

37	19.310	2753	2758	2764	rBV	28956	45160	1.13%	0.102%
38	19.375	2766	2769	2773	rBV	24589	32266	0.80%	0.073%
39	19.745	2826	2832	2846	rBV	2977838	3954339	98.63%	8.893%
40	20.716	2995	2997	3000	rVB3	24191	21044	0.52%	0.047%
41	21.539	3132	3137	3145	rBV	2481335	3199701	79.81%	7.196%
42	23.810	3516	3523	3535	rBV2	1974061	4009075	100.00%	9.016%
43	23.968	3543	3550	3560	rVB2	1627686	3174767	79.19%	7.140%




Sum of corrected areas: 44467632

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010523\
Data File : BN023564.D
Acq On : 05 Jan 2023 11:52
Operator : CG/JU
Sample : PB149946BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK946

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

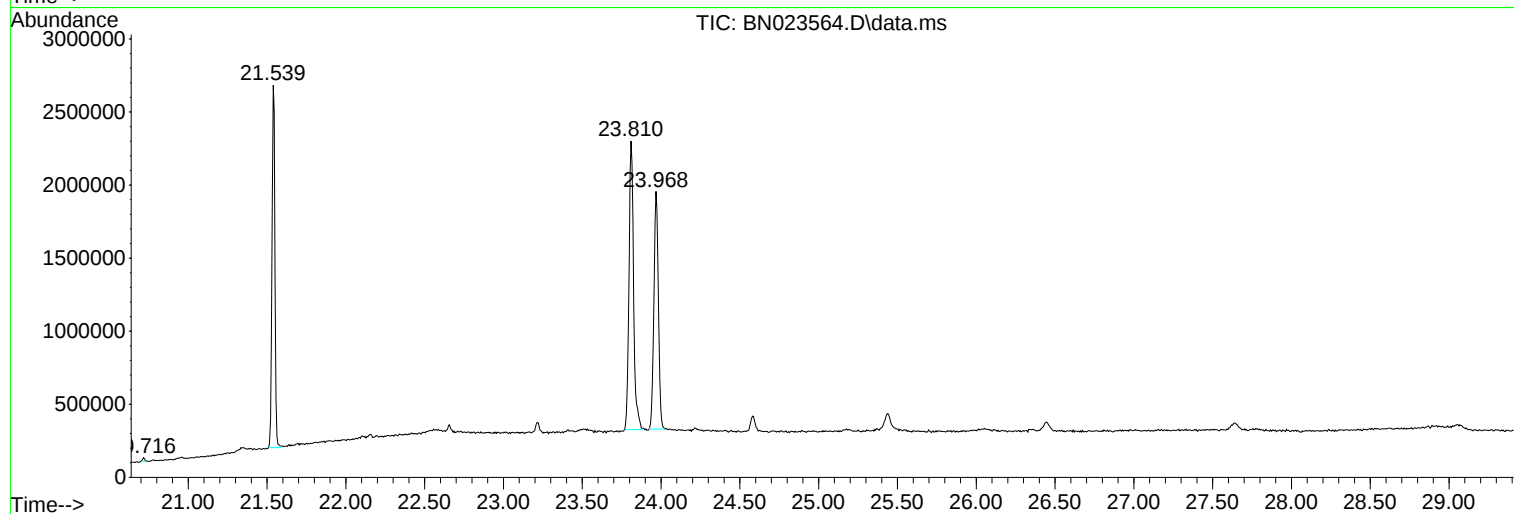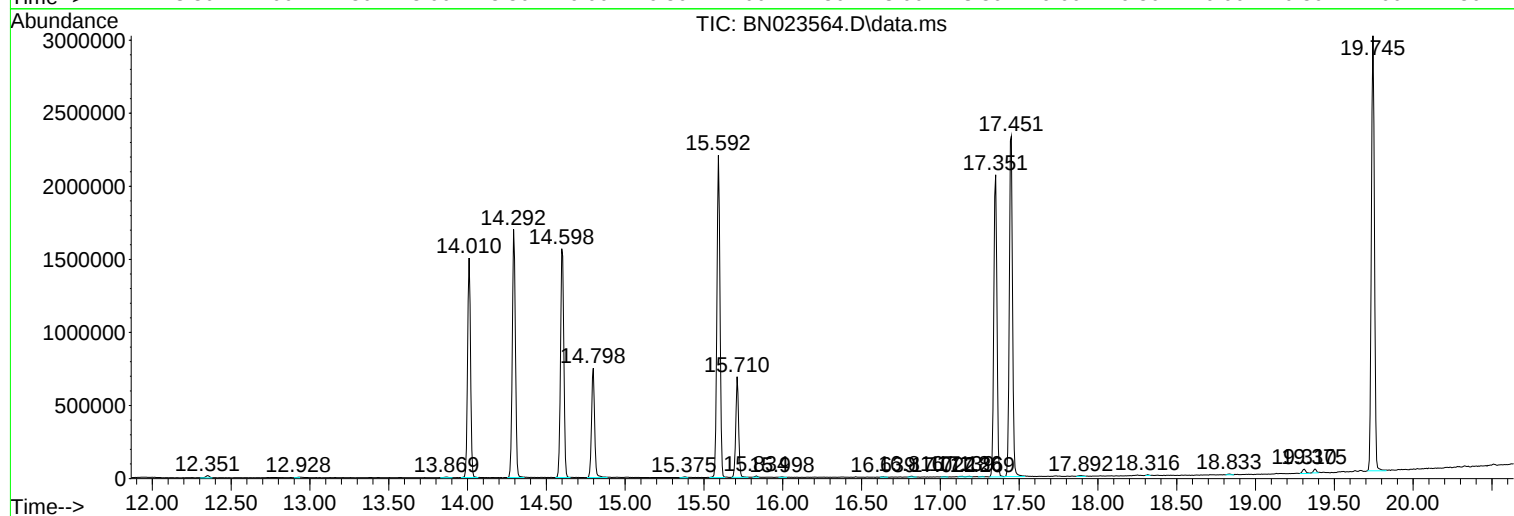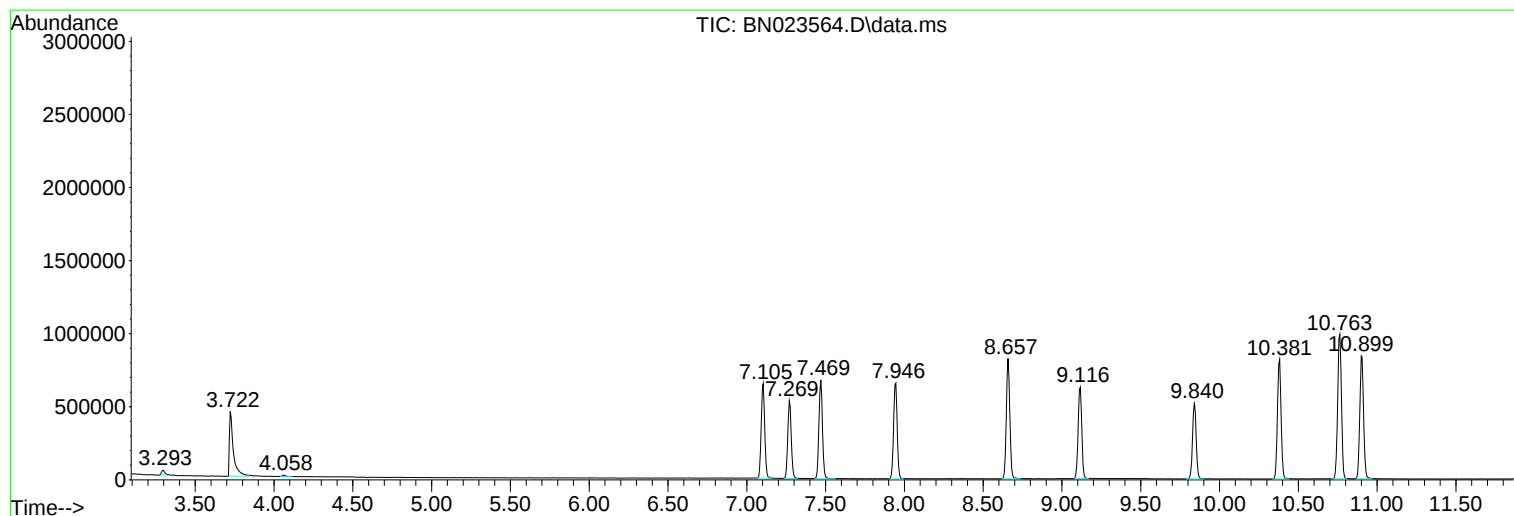

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010523\
Data File : BN023564.D
Acq On : 05 Jan 2023 11:52
Operator : CG/JU
Sample : PB149946BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK946

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010523\
Data File : BN023564.D
Acq On : 05 Jan 2023 11:52
Operator : CG/JU
Sample : PB149946BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK946

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc