

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010523\
 Data File : BN023567.D
 Acq On : 05 Jan 2023 14:34
 Operator : CG/JU
 Sample : PB149947BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK947

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	44	rVB	36935	58306	1.37%	0.129%
2	3.722	104	108	128	rBV	488672	860281	20.20%	1.901%
3	4.058	162	165	170	rBV2	11268	14356	0.34%	0.032%
4	7.099	675	682	692	rVB	730274	1101644	25.87%	2.434%
5	7.269	704	711	719	rBV	593496	891477	20.94%	1.970%
6	7.463	738	744	752	rBV	716797	1133774	26.63%	2.505%
7	7.940	818	825	834	rBV	614444	957759	22.49%	2.116%
8	8.652	940	946	956	rBV	862249	1369931	32.17%	3.027%
9	9.110	1017	1024	1036	rVB	690225	1086509	25.52%	2.400%
10	9.840	1139	1148	1160	rBV	566461	909632	21.36%	2.010%
11	10.375	1231	1239	1249	rBV	900413	1422182	33.40%	3.142%
12	10.757	1297	1304	1313	rBV	909051	1498317	35.19%	3.310%
13	10.898	1321	1328	1339	rBV	924188	1502962	35.30%	3.321%
14	12.345	1570	1574	1579	rBV2	15065	22841	0.54%	0.050%
15	12.898	1661	1668	1670	rBV7	4327	8685	0.20%	0.019%
16	13.845	1822	1829	1830	rBV5	4845	6423	0.15%	0.014%
17	14.010	1846	1857	1866	rBV	1598854	2115587	49.68%	4.674%
18	14.292	1898	1905	1915	rBV	1811092	2525835	59.32%	5.580%
19	14.598	1950	1957	1967	rBV	1472504	2073979	48.71%	4.582%
20	14.798	1984	1991	2008	rBV	776932	1089080	25.58%	2.406%
21	15.375	2084	2089	2094	rBV3	7579	11612	0.27%	0.026%
22	15.592	2116	2126	2135	rBV	2321093	3241124	76.11%	7.161%
23	15.710	2139	2146	2156	rBV	730328	927624	21.78%	2.049%
24	15.828	2162	2166	2172	rVB3	10229	14252	0.33%	0.031%
25	15.904	2172	2179	2182	rBV6	2128	4388	0.10%	0.010%
26	15.998	2189	2195	2201	rVB5	6417	11517	0.27%	0.025%
27	16.463	2270	2274	2279	rBV5	3917	5725	0.13%	0.013%
28	16.639	2300	2304	2309	rVB5	5424	8118	0.19%	0.018%
29	16.816	2328	2334	2338	rBV	11754	16523	0.39%	0.037%
30	17.133	2384	2388	2393	rBV3	4376	5103	0.12%	0.011%
31	17.186	2393	2397	2401	rVV4	6237	9844	0.23%	0.022%
32	17.263	2406	2410	2414	rBV6	4502	5587	0.13%	0.012%
33	17.351	2418	2425	2435	rBV	1789672	2552980	59.95%	5.640%
34	17.445	2435	2441	2460	rVV	2452215	3555408	83.50%	7.855%
35	17.733	2487	2490	2497	rVB8	4524	7853	0.18%	0.017%
36	17.892	2513	2517	2520	rBV3	7576	9346	0.22%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010523\
 Data File : BN023567.D
 Acq On : 05 Jan 2023 14:34
 Operator : CG/JU
 Sample : PB149947BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK947

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

37	18.016	2535	2538	2542	rVB6	5195	6479	0.15%	0.014%
38	18.316	2586	2589	2593	rBV	8200	10345	0.24%	0.023%
39	18.833	2673	2677	2681	rBV3	10510	14271	0.34%	0.032%
40	19.310	2754	2758	2763	rVB2	26989	37932	0.89%	0.084%
41	19.380	2765	2770	2773	rBV	27664	36855	0.87%	0.081%
42	19.633	2810	2813	2816	rBV3	8417	12326	0.29%	0.027%
43	19.745	2826	2832	2838	rBV	3284084	4148545	97.42%	9.165%
44	21.539	3132	3137	3149	rBV	2285976	2868633	67.37%	6.338%
45	23.810	3516	3523	3536	rVB2	2100196	4258200	100.00%	9.408%
46	23.968	3543	3550	3561	rVB2	1503979	2832720	66.52%	6.258%




Sum of corrected areas: 45262870

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010523\
Data File : BN023567.D
Acq On : 05 Jan 2023 14:34
Operator : CG/JU
Sample : PB149947BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

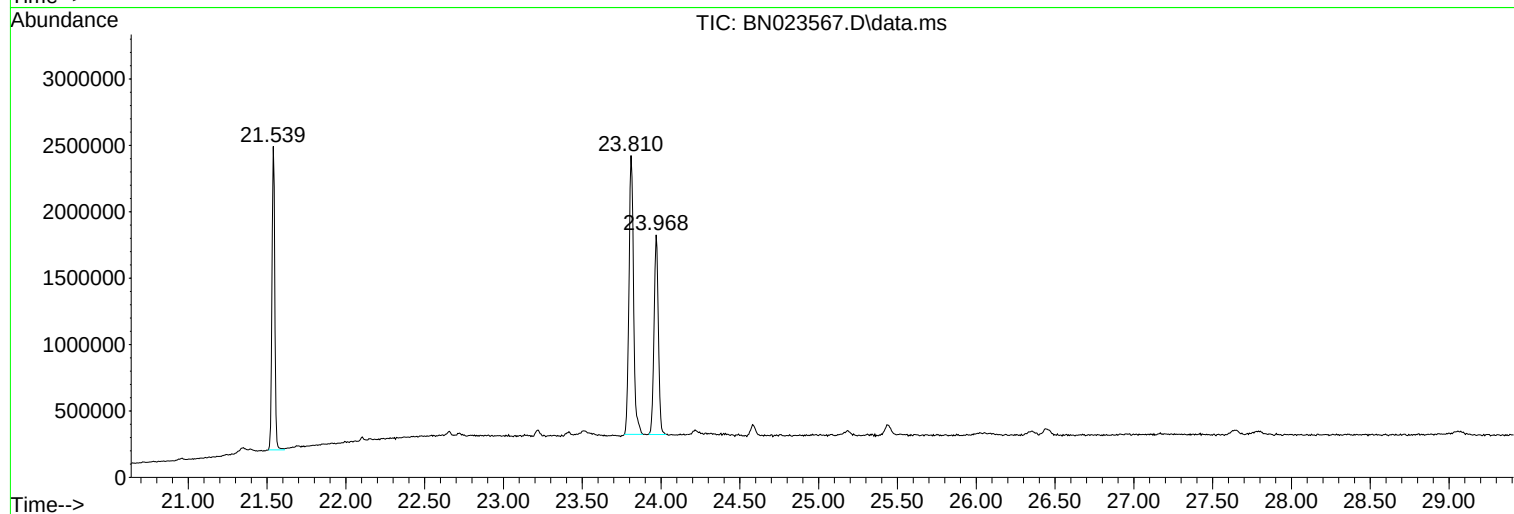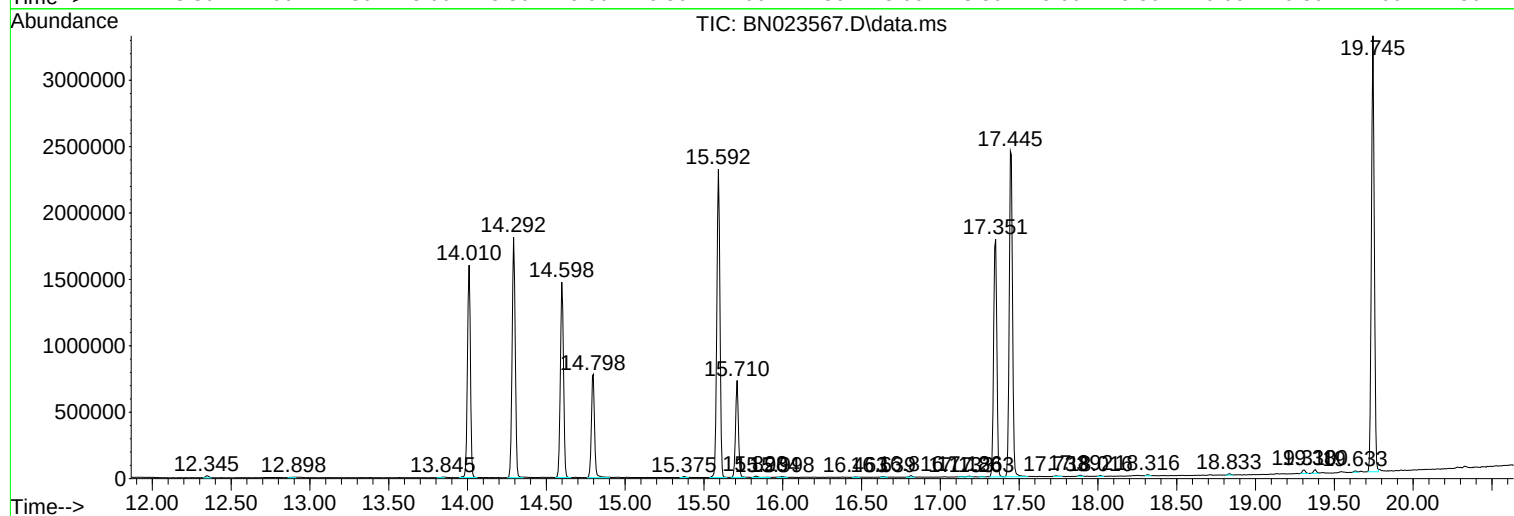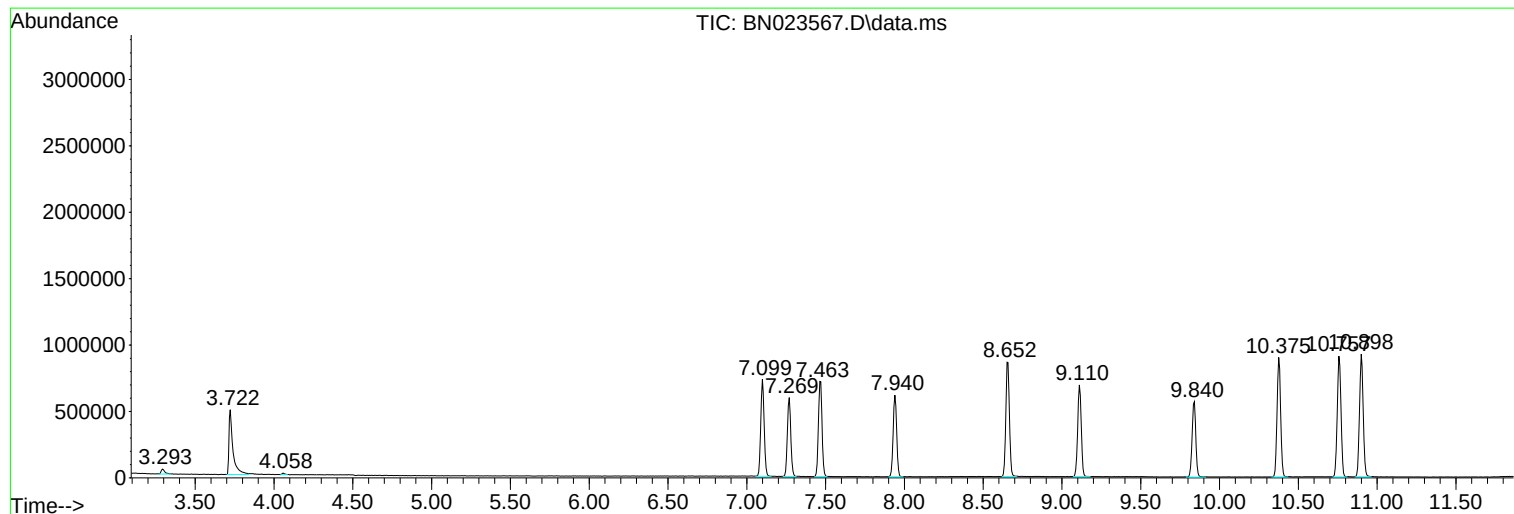

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010523\
Data File : BN023567.D
Acq On : 05 Jan 2023 14:34
Operator : CG/JU
Sample : PB149947BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010523\
Data File : BN023567.D
Acq On : 05 Jan 2023 14:34
Operator : CG/JU
Sample : PB149947BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc