

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010623\
 Data File : BN023575.D
 Acq On : 06 Jan 2023 13:35
 Operator : CG/JU
 Sample : PB149982BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK982

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023575.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	32	35	44	rVB	38346	55115	1.21%	0.115%
2	3.723	106	108	126	rBV	494936	825017	18.08%	1.727%
3	4.064	162	166	173	rVB	11587	17503	0.38%	0.037%
4	7.105	676	683	693	rVB	731497	1087471	23.83%	2.276%
5	7.275	705	712	724	rVB	568430	887682	19.45%	1.858%
6	7.469	738	745	753	rBV	735135	1120055	24.54%	2.344%
7	7.946	819	826	834	rBV	705909	1088174	23.84%	2.278%
8	8.658	940	947	957	rBV	881076	1364988	29.91%	2.857%
9	9.116	1018	1025	1034	rBV	683217	1078223	23.62%	2.257%
10	9.840	1141	1148	1160	rVB	584428	906220	19.85%	1.897%
11	10.381	1232	1240	1251	rBV	894860	1415374	31.01%	2.962%
12	10.763	1297	1305	1313	rVB	1093490	1740070	38.12%	3.642%
13	10.905	1320	1329	1345	rBV	933115	1537978	33.70%	3.219%
14	12.352	1569	1575	1585	rVB2	15101	24197	0.53%	0.051%
15	14.010	1851	1857	1870	rVB	1661643	2203293	48.27%	4.612%
16	14.293	1898	1905	1915	rBV	1824770	2564384	56.18%	5.367%
17	14.598	1950	1957	1965	rBV	1658243	2391466	52.39%	5.006%
18	14.798	1984	1991	2006	rBV	839385	1155771	25.32%	2.419%
19	15.010	2024	2027	2033	rVB6	2626	4632	0.10%	0.010%
20	15.593	2118	2126	2133	rBV	2449307	3310318	72.53%	6.929%
21	15.710	2140	2146	2155	rBV	823211	1050364	23.01%	2.198%
22	15.834	2163	2167	2171	rBV2	9958	12661	0.28%	0.027%
23	16.816	2329	2334	2339	rBV6	3996	7653	0.17%	0.016%
24	17.345	2418	2424	2431	rBV	2045322	2901051	63.56%	6.072%
25	17.445	2434	2441	2454	rBV	2682460	3774397	82.69%	7.900%
26	19.304	2753	2757	2763	rBV	32232	42666	0.93%	0.089%
27	19.375	2765	2769	2773	rVV	28165	37306	0.82%	0.078%
28	19.669	2817	2819	2823	rVB4	9868	7929	0.17%	0.017%
29	19.745	2826	2832	2846	rVV	3453222	4469276	97.92%	9.355%
30	21.539	3132	3137	3145	rBV	2515510	3092581	67.75%	6.473%
31	23.804	3515	3522	3535	rBV2	2229902	4564377	100.00%	9.554%
32	23.969	3543	3550	3560	rVB2	1535188	3038390	66.57%	6.360%




Sum of corrected areas: 47776582

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010623\
Data File : BN023575.D
Acq On : 06 Jan 2023 13:35
Operator : CG/JU
Sample : PB149982BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

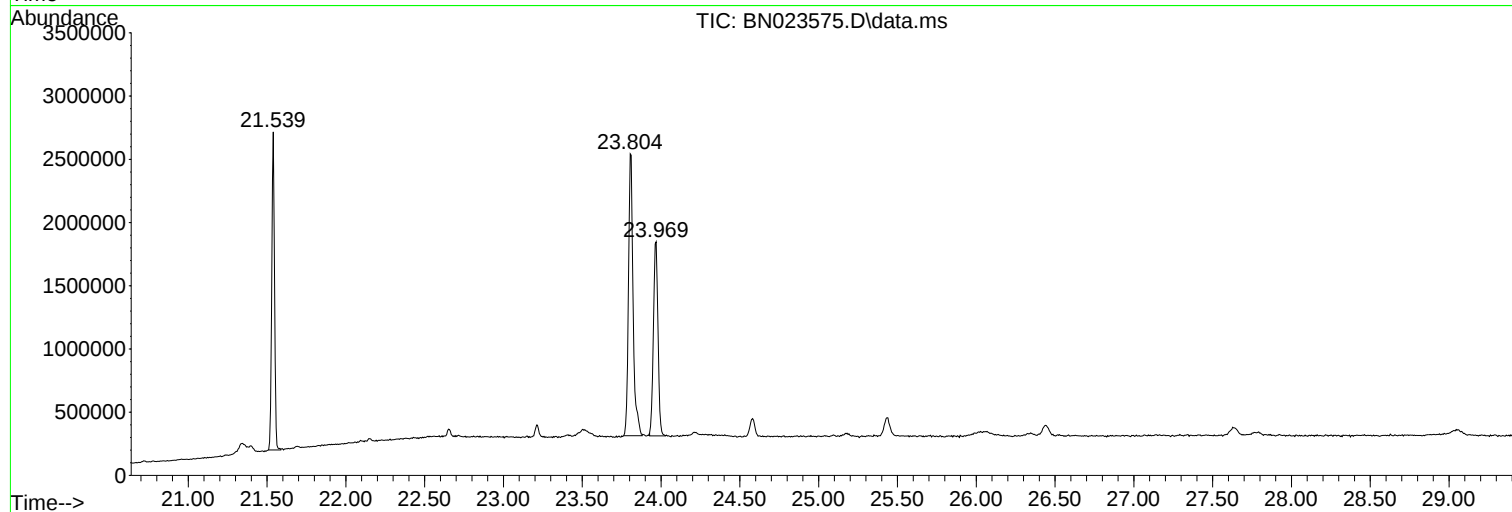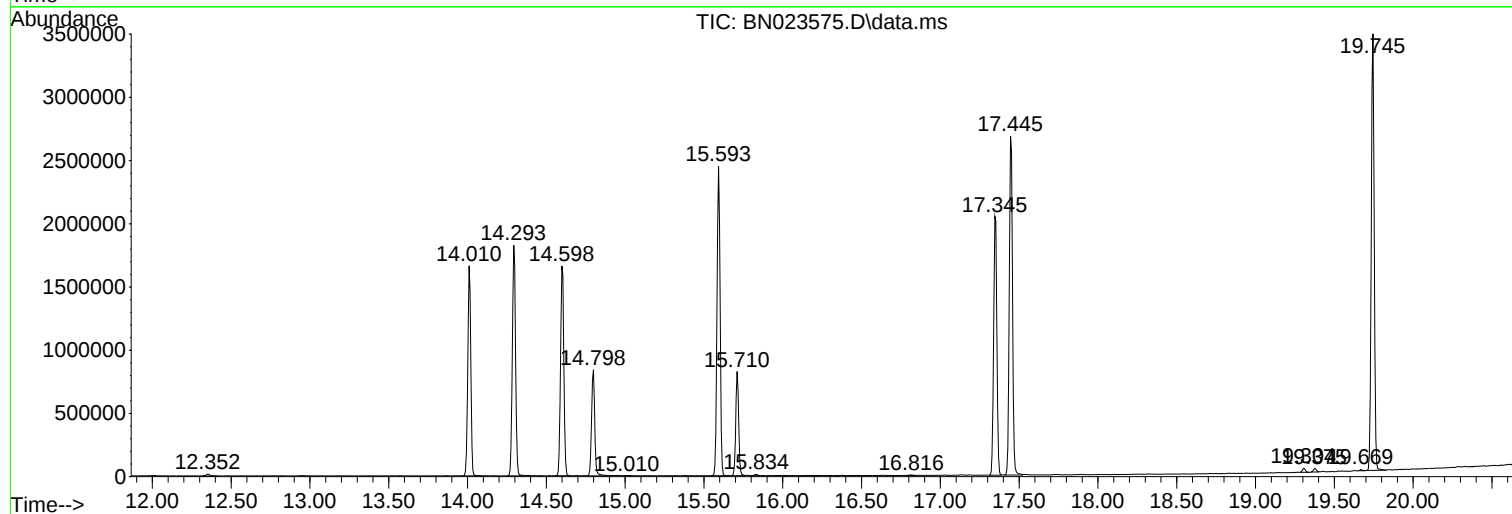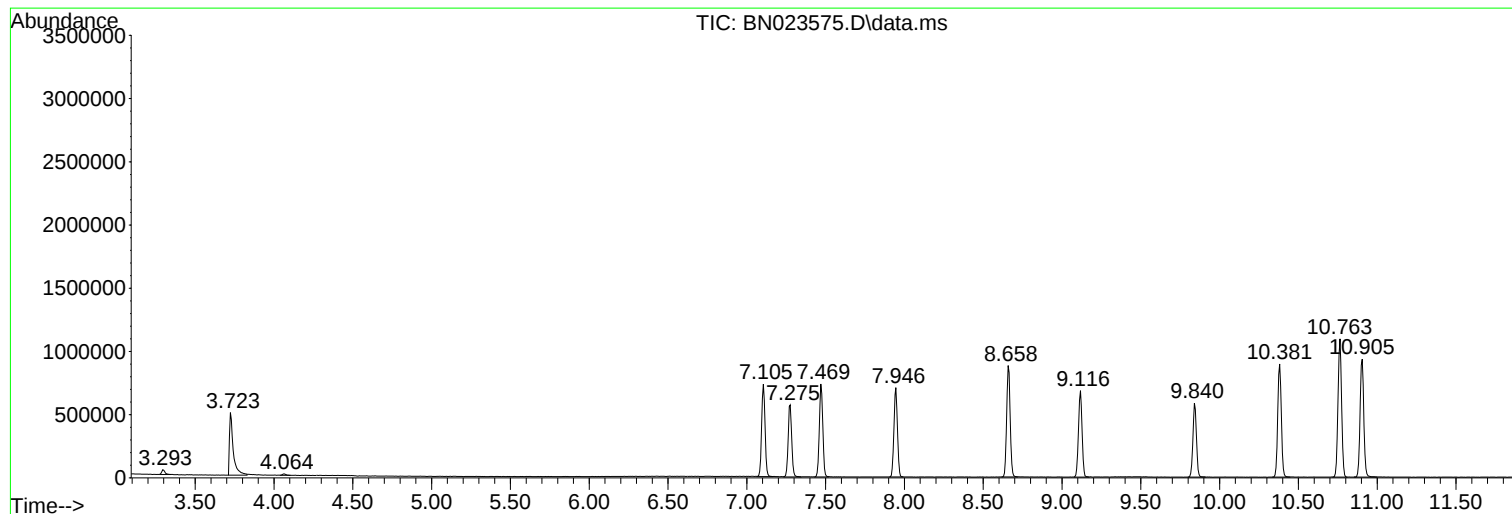

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010623\
Data File : BN023575.D
Acq On : 06 Jan 2023 13:35
Operator : CG/JU
Sample : PB149982BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010623\
Data File : BN023575.D
Acq On : 06 Jan 2023 13:35
Operator : CG/JU
Sample : PB149982BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc