

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010722\
 Data File : BN018363.D
 Acq On : 07 Jan 2022 11:02
 Operator : CG/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Jan 07 13:18:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 07 13:11:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.624	152	29804	0.400	ng	0.00
7) Naphthalene-d8	10.407	136	136194	0.400	ng	0.00
13) Acenaphthene-d10	14.256	164	66262	0.400	ng	0.00
19) Phenanthrene-d10	16.993	188	109610	0.400	ng	# 0.00
29) Chrysene-d12	21.185	240	91291	0.400	ng	# 0.00
35) Perylene-d12	23.413	264	82835	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.236	112	28056	0.470	ng	0.00
5) Phenol-d6	6.813	99	27738	0.480	ng	0.00
8) Nitrobenzene-d5	8.772	82	28507	0.352	ng	0.00
11) 2-Methylnaphthalene-d10	11.998	152	84669	0.370	ng	0.00
14) 2,4,6-Tribromophenol	15.753	330	7382	0.332	ng	0.00
15) 2-Fluorobiphenyl	12.886	172	96668	0.385	ng	0.00
27) Fluoranthene-d10	19.033	212	121975	0.350	ng	0.00
31) Terphenyl-d14	19.639	244	79389	0.342	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.170	88	6551	0.385	ng	# 56
3) n-Nitrosodimethylamine	3.502	42	10118	0.413	ng	92
6) bis(2-Chloroethyl)ether	7.061	93	31693	0.447	ng	99
9) Naphthalene	10.445	128	138478	0.411	ng	99
10) Hexachlorobutadiene	10.749	225	25531	0.272	ng	# 100
12) 2-Methylnaphthalene	12.069	142	86002	0.398	ng	98
16) Acenaphthylene	13.964	152	98581	0.423	ng	100
17) Acenaphthene	14.319	154	73298	0.428	ng	100
18) Fluorene	15.309	166	81736	0.405	ng	99
20) 4,6-Dinitro-2-methylph...	15.423	198	1169	0.564	ng	# 91
21) 4-Bromophenyl-phenylether	16.202	248	23204	0.349	ng	90
22) Hexachlorobenzene	16.312	284	32046	0.378	ng	# 91
23) Atrazine	16.470	200	12690	0.317	ng	91
24) Pentachlorophenol	16.665	266	3780	0.320	ng	100
25) Phenanthrene	17.030	178	122909	0.425	ng	100
26) Anthracene	17.127	178	95479	0.419	ng	100
28) Fluoranthene	19.063	202	133054	0.393	ng	# 96
30) Pyrene	19.425	202	130376	0.364	ng	99
32) Benzo(a)anthracene	21.174	228	96697	0.395	ng	99
33) Chrysene	21.227	228	125761	0.428	ng	98
34) Bis(2-ethylhexyl)phtha...	21.121	149	44175	0.388	ng	# 94
36) Indeno(1,2,3-cd)pyrene	25.675	276	94730	0.479	ng	# 91
37) Benzo(b)fluoranthene	22.742	252	110257	0.419	ng	# 96
38) Benzo(k)fluoranthene	22.786	252	105610	0.424	ng	# 96
39) Benzo(a)pyrene	23.317	252	96361	0.421	ng	# 96
40) Dibenzo(a,h)anthracene	25.696	278	67848	0.481	ng	# 95
41) Benzo(g,h,i)perylene	26.363	276	92601	0.469	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010722\
Data File : BN018363.D
Acq On : 07 Jan 2022 11:02
Operator : CG/JU
Sample : SSTDICC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.4


Quant Time: Jan 07 13:18:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 07 13:11:58 2022
Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.624 min Scan# 493
 Delta R.T. 0.000 min
 Lab File: BN018363.D
 Acq: 07 Jan 2022 11:02

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4







Tgt Ion:152 Resp: 29804
 Ion Ratio Lower Upper
 152 100
 150 159.2 121.7 182.5
 115 63.8 43.8 65.8



#2
 1,4-Dioxane
 Concen: 0.385 ng
 RT: 3.170 min Scan# 10
 Delta R.T. 0.000 min
 Lab File: BN018363.D
 Acq: 07 Jan 2022 11:02

Tgt Ion: 88 Resp: 6551
 Ion Ratio Lower Upper
 88 100
 43 31.5 69.7 104.5#
 58 72.5 83.8 125.8#







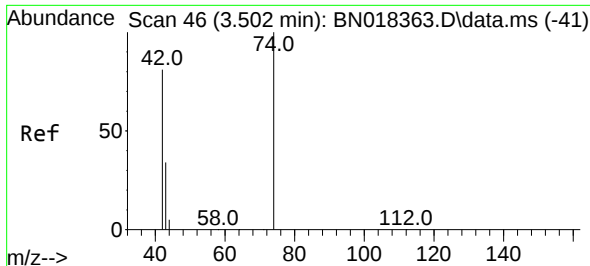

#3
n-Nitrosodimethylamine
Concen: 0.413 ng
RT: 3.502 min Scan# 41
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 42 Resp: 10118
Ion Ratio Lower Upper
42 100
74 125.3 108.6 163.0
44 6.5 5.8 8.8

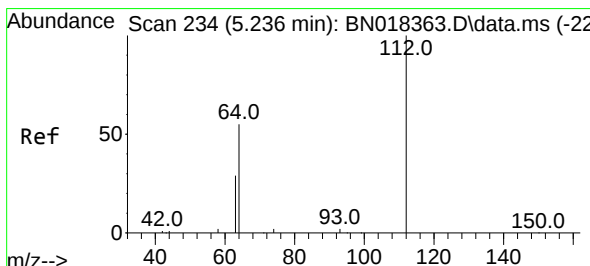

#4
2-Fluorophenol
Concen: 0.470 ng
RT: 5.236 min Scan# 234
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion: 112 Resp: 28056
Ion Ratio Lower Upper
112 100
64 60.3 48.0 72.0
63 32.0 25.3 37.9









#5
Phenol-d6
Concen: 0.480 ng
RT: 6.813 min Scan# 405
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 99 Resp: 27738
Ion Ratio Lower Upper
99 100
42 20.8 16.3 24.5
71 34.2 26.8 40.2



#6
bis(2-Chloroethyl)ether
Concen: 0.447 ng
RT: 7.061 min Scan# 432
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion: 93 Resp: 31693
Ion Ratio Lower Upper
93 100
63 78.2 61.7 92.5
95 33.4 26.2 39.4









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.407 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	136	Resp:	136194
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.8	13.2
54	5.4	5.0	7.6
68	4.8	4.4	6.6



#8
Nitrobenzene-d5
Concen: 0.352 ng
RT: 8.772 min Scan# 604
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:	82	Resp:	28507
Ion	Ratio	Lower	Upper
82	100		
128	34.0	33.7	50.5
54	51.5	36.6	55.0





#9
Naphthalene

Concen: 0.411 ng
RT: 10.445 min Scan# 736
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02





Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4

Tgt Ion:128 Resp: 138478
Ion Ratio Lower Upper
128 100
129 10.8 8.7 13.1
127 13.4 10.4 15.6







#10

Hexachlorobutadiene

Concen: 0.272 ng
RT: 10.749 min Scan# 760
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:225 Resp: 25531
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.1 51.0 76.6



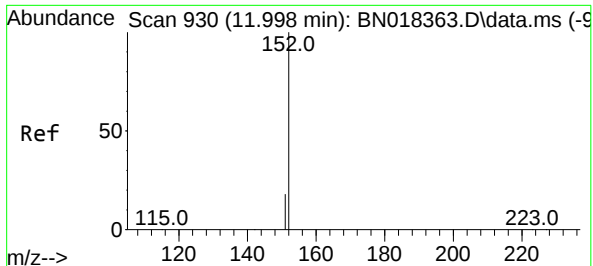

#11

2-Methylnaphthalene-d10

Concen: 0.370 ng

RT: 11.998 min Scan# 911

Delta R.T. 0.000 min

Lab File: BN018363.D

Acq: 07 Jan 2022 11:02

Instrument :

BNA_N

ClientSampleId :





SSTDICCC0.4

Tgt Ion:152 Resp: 84669

Ion Ratio Lower Upper

152 100

151 20.4 16.2 24.2



#12

2-Methylnaphthalene

Concen: 0.398 ng

RT: 12.069 min Scan# 946

Delta R.T. 0.000 min

Lab File: BN018363.D

Acq: 07 Jan 2022 11:02




Tgt Ion:142 Resp: 86002


Ion Ratio Lower Upper

142 100

141 88.3 70.0 105.0

115 36.8 27.8 41.8









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.256 min Scan# 1182
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:164 Resp: 66262
Ion Ratio Lower Upper
164 100
162 98.9 80.2 120.2
160 44.8 36.9 55.3



#14
2,4,6-Tribromophenol
Concen: 0.332 ng
RT: 15.753 min Scan# 1300
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:330 Resp: 7382
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 34.7 21.3 31.9#









#15
2-Fluorobiphenyl
Concen: 0.385 ng
RT: 12.886 min Scan# 1074
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:172 Resp: 96668
Ion Ratio Lower Upper
172 100
171 33.7 27.4 41.0
170 21.9 18.4 27.6



#16
Acenaphthylene
Concen: 0.423 ng
RT: 13.964 min Scan# 1159
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:152 Resp: 98581
Ion Ratio Lower Upper
152 100
151 19.7 15.8 23.6
153 13.0 10.5 15.7







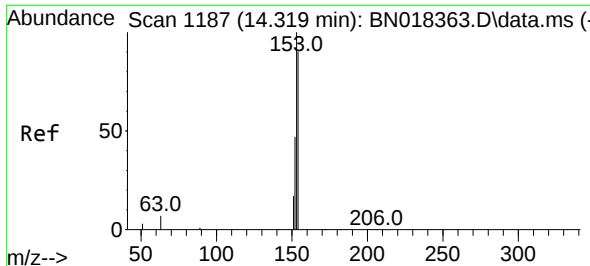

#17
Acenaphthene
Concen: 0.428 ng
RT: 14.319 min Scan# 1187
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:154 Resp: 73298
Ion Ratio Lower Upper
154 100
153 113.8 90.9 136.3
152 55.6 45.0 67.4

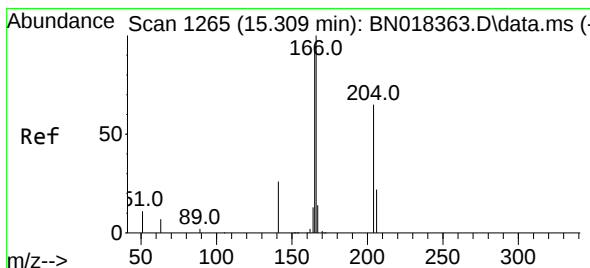

#18
Fluorene
Concen: 0.405 ng
RT: 15.309 min Scan# 1265
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:166 Resp: 81736
Ion Ratio Lower Upper
166 100
165 98.1 77.8 116.6
167 13.5 10.9 16.3









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.993 min Scan# 1401
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:188 Resp: 109610
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.4 7.0 10.4#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.564 ng
RT: 15.423 min Scan# 1274
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:198 Resp: 1169
Ion Ratio Lower Upper
198 100
182 23.5 15.5 23.3#
77 0.0 0.0 0.0







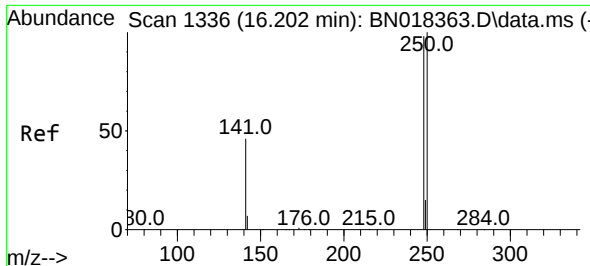

#21
4-Bromophenyl-phenylether
Concen: 0.349 ng
RT: 16.202 min Scan# 1336
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:248 Resp: 23204
Ion Ratio Lower Upper
248 100
250 102.2 74.4 111.6
141 47.8 43.7 65.5

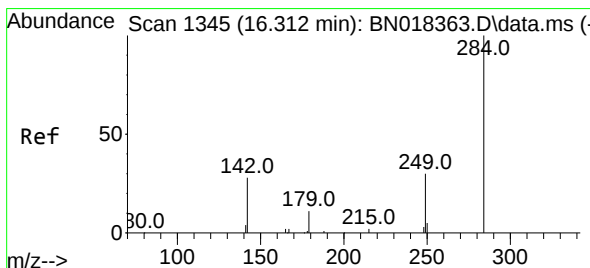

#22
Hexachlorobenzene
Concen: 0.378 ng
RT: 16.312 min Scan# 1345
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:284 Resp: 32046
Ion Ratio Lower Upper
284 100
142 36.3 21.6 32.4#
249 28.8 23.5 35.3









#23
Atrazine
Concen: 0.317 ng
RT: 16.470 min Scan# 1358
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:200 Resp: 12690
Ion Ratio Lower Upper
200 100
173 30.4 20.3 30.5
215 45.0 40.4 60.6



#24
Pentachlorophenol
Concen: 0.320 ng
RT: 16.665 min Scan# 1374
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:266 Resp: 3780
Ion Ratio Lower Upper
266 100
264 62.1 49.5 74.3
268 63.8 50.6 76.0









#25
Phenanthrene
Concen: 0.425 ng
RT: 17.030 min Scan# 1404
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:178 Resp: 122909
Ion Ratio Lower Upper
178 100
176 19.1 15.3 22.9
179 15.2 12.3 18.5



#26
Anthracene
Concen: 0.419 ng
RT: 17.127 min Scan# 1412
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:178 Resp: 95479
Ion Ratio Lower Upper
178 100
176 18.4 14.8 22.2
179 15.2 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.350 ng
RT: 19.033 min Scan# 1690
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:212 Resp: 121975
Ion Ratio Lower Upper
212 100
106 16.7 8.4 12.6#
104 9.1 4.5 6.7#



#28
Fluoranthene
Concen: 0.393 ng
RT: 19.063 min Scan# 1696
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:202 Resp: 133054
Ion Ratio Lower Upper
202 100
101 13.4 7.2 10.8#
203 17.0 13.7 20.5







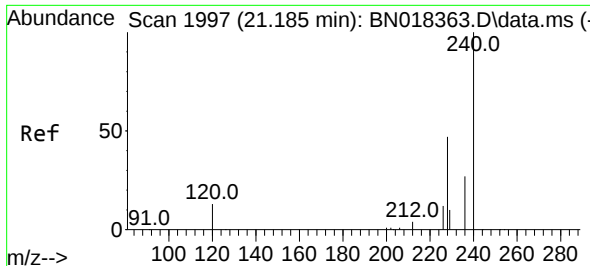

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.185 min Scan# 1997
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:240 Resp: 91291
Ion Ratio Lower Upper
240 100
120 12.9 6.0 9.0#
236 26.6 21.4 32.2

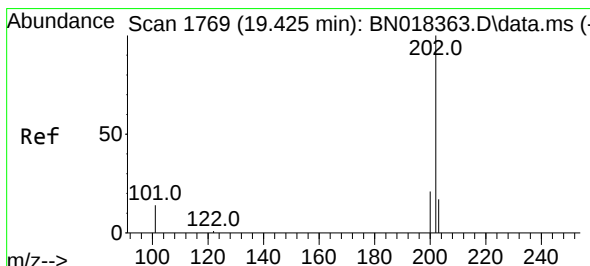

#30
Pyrene
Concen: 0.364 ng
RT: 19.425 min Scan# 1769
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:202 Resp: 130376
Ion Ratio Lower Upper
202 100
200 21.0 16.6 25.0
203 17.3 14.1 21.1









#31
 Terphenyl-d14
 Concen: 0.342 ng
 RT: 19.639 min Scan# 1812
 Delta R.T. 0.000 min
 Lab File: BN018363.D
 Acq: 07 Jan 2022 11:02




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:244 Resp: 79389
 Ion Ratio Lower Upper
 244 100
 212 8.0 6.2 9.2
 122 16.4 7.9 11.9#



#32
 Benzo(a)anthracene
 Concen: 0.395 ng
 RT: 21.174 min Scan# 1996
 Delta R.T. 0.000 min
 Lab File: BN018363.D
 Acq: 07 Jan 2022 11:02

Tgt Ion:228 Resp: 96697
 Ion Ratio Lower Upper
 228 100
 226 26.2 21.3 31.9
 229 19.7 15.9 23.9







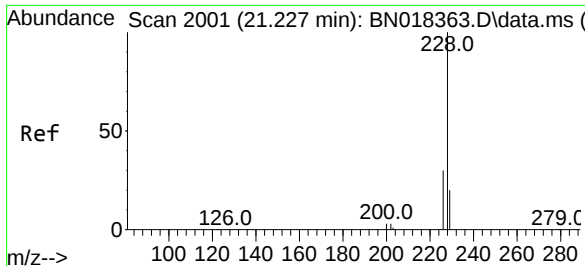

#33
Chrysene
Concen: 0.428 ng
RT: 21.227 min Scan# 2001
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:228 Resp: 125761
Ion Ratio Lower Upper
228 100
226 29.2 24.2 36.4
229 19.8 15.5 23.3



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.388 ng
RT: 21.121 min Scan# 1991
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:149 Resp: 44175
Ion Ratio Lower Upper
149 100
167 26.0 23.7 35.5
279 3.1 3.6 5.4#



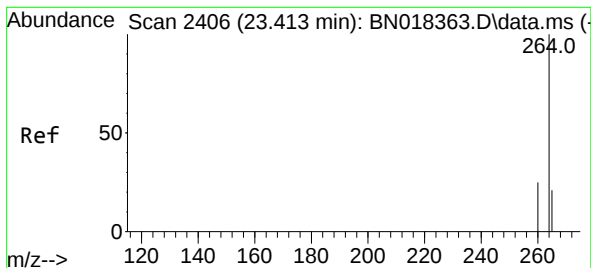

#35

Perylene-d12

Concen: 0.400 ng

RT: 23.413 min Scan# 2406

Delta R.T. 0.000 min

Lab File: BN018363.D

Acq: 07 Jan 2022 11:02

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:264 Resp: 82835

Ion Ratio Lower Upper

264 100

260 25.2 20.2 30.4

265 23.3 18.2 27.2

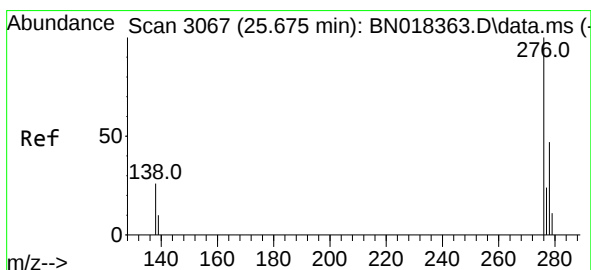

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.479 ng

RT: 25.675 min Scan# 3067

Delta R.T. 0.000 min

Lab File: BN018363.D

Acq: 07 Jan 2022 11:02




Tgt Ion:276 Resp: 94730


Ion Ratio Lower Upper

276 100

138 27.9 14.9 22.3#

277 24.9 19.9 29.9









#37
Benzo(b)fluoranthene
Concen: 0.419 ng
RT: 22.742 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:252 Resp: 110257
Ion Ratio Lower Upper
252 100
253 22.0 17.8 26.6
125 12.1 6.0 9.0#



#38
Benzo(k)fluoranthene
Concen: 0.424 ng
RT: 22.786 min Scan# 2223
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:252 Resp: 105610
Ion Ratio Lower Upper
252 100
253 21.9 17.7 26.5
125 12.2 6.2 9.2#









#39
Benzo(a)pyrene
Concen: 0.421 ng
RT: 23.317 min Scan# 2378
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:252 Resp: 96361
Ion Ratio Lower Upper
252 100
253 22.4 17.8 26.6
125 13.8 7.0 10.4#

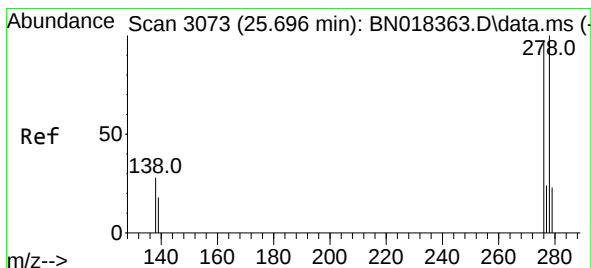

#40
Dibenzo(a,h)anthracene
Concen: 0.481 ng
RT: 25.696 min Scan# 3073
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Tgt Ion:278 Resp: 67848
Ion Ratio Lower Upper
278 100
139 18.9 10.8 16.2#
279 23.9 19.0 28.4



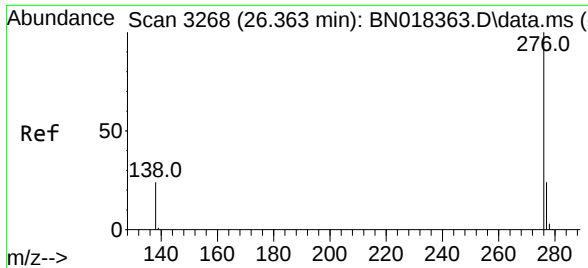

#41
Benzo(g,h,i)perylene
Concen: 0.469 ng
RT: 26.363 min Scan# 31
Delta R.T. 0.000 min
Lab File: BN018363.D
Acq: 07 Jan 2022 11:02

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:276 Resp: 92601
Ion Ratio Lower Upper
276 100
277 24.2 19.0 28.6
138 24.7 12.6 19.0#

