

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010722\
 Data File : BN018365.D
 Acq On : 07 Jan 2022 12:14
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Jan 07 13:19:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 07 13:11:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.633	152	34144	0.400	ng	0.00
7) Naphthalene-d8	10.407	136	151929	0.400	ng	# 0.00
13) Acenaphthene-d10	14.256	164	75529	0.400	ng	0.00
19) Phenanthrene-d10	16.993	188	126093	0.400	ng	# 0.00
29) Chrysene-d12	21.185	240	115738	0.400	ng	# 0.00
35) Perylene-d12	23.409	264	111242	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.227	112	146882	2.147	ng	0.00
5) Phenol-d6	6.813	99	153513	2.320	ng	0.00
8) Nitrobenzene-d5	8.772	82	169165	1.873	ng	0.00
11) 2-Methylnaphthalene-d10	11.994	152	402793	1.576	ng	0.00
14) 2,4,6-Tribromophenol	15.753	330	54559	2.152	ng	0.00
15) 2-Fluorobiphenyl	12.886	172	465080	1.627	ng	0.00
27) Fluoranthene-d10	19.028	212	634850	1.582	ng	0.00
31) Terphenyl-d14	19.639	244	415242	1.412	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.170	88	30443	1.563	ng	# 57
3) n-Nitrosodimethylamine	3.493	42	55866	1.992	ng	95
6) bis(2-Chloroethyl)ether	7.062	93	159739	1.966	ng	100
9) Naphthalene	10.445	128	638689	1.700	ng	100
10) Hexachlorobutadiene	10.749	225	118221	1.130	ng	# 99
12) 2-Methylnaphthalene	12.070	142	397328	1.650	ng	99
16) Acenaphthylene	13.964	152	550179	2.071	ng	100
17) Acenaphthene	14.320	154	354643	1.818	ng	99
18) Fluorene	15.296	166	408282	1.777	ng	100
20) 4,6-Dinitro-2-methylph...	15.398	198	16555	6.945	ng	# 80
21) 4-Bromophenyl-phenylether	16.190	248	125593	1.640	ng	# 80
22) Hexachlorobenzene	16.312	284	153892	1.577	ng	# 91
23) Atrazine	16.470	200	91356	1.985	ng	95
24) Pentachlorophenol	16.665	266	41292	3.041	ng	99
25) Phenanthrene	17.030	178	609435	1.833	ng	100
26) Anthracene	17.127	178	543556	2.074	ng	100
28) Fluoranthene	19.058	202	657911	1.690	ng	# 95
30) Pyrene	19.420	202	666493	1.469	ng	100
32) Benzo(a)anthracene	21.174	228	622448	2.007	ng	99
33) Chrysene	21.217	228	631347	1.694	ng	99
34) Bis(2-ethylhexyl)phtha...	21.121	149	367249	2.542	ng	# 95
36) Indeno(1,2,3-cd)pyrene	25.668	276	642403	2.418	ng	# 91
37) Benzo(b)fluoranthene	22.738	252	626672	1.773	ng	# 96
38) Benzo(k)fluoranthene	22.786	252	617014	1.844	ng	# 97
39) Benzo(a)pyrene	23.313	252	573376	1.864	ng	# 96
40) Dibenzo(a,h)anthracene	25.685	278	495265	2.615	ng	# 95
41) Benzo(g,h,i)perylene	26.353	276	560376	2.114	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010722\
Data File : BN018365.D
Acq On : 07 Jan 2022 12:14
Operator : CG/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Quant Time: Jan 07 13:19:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 07 13:11:58 2022
Response via : Initial Calibration




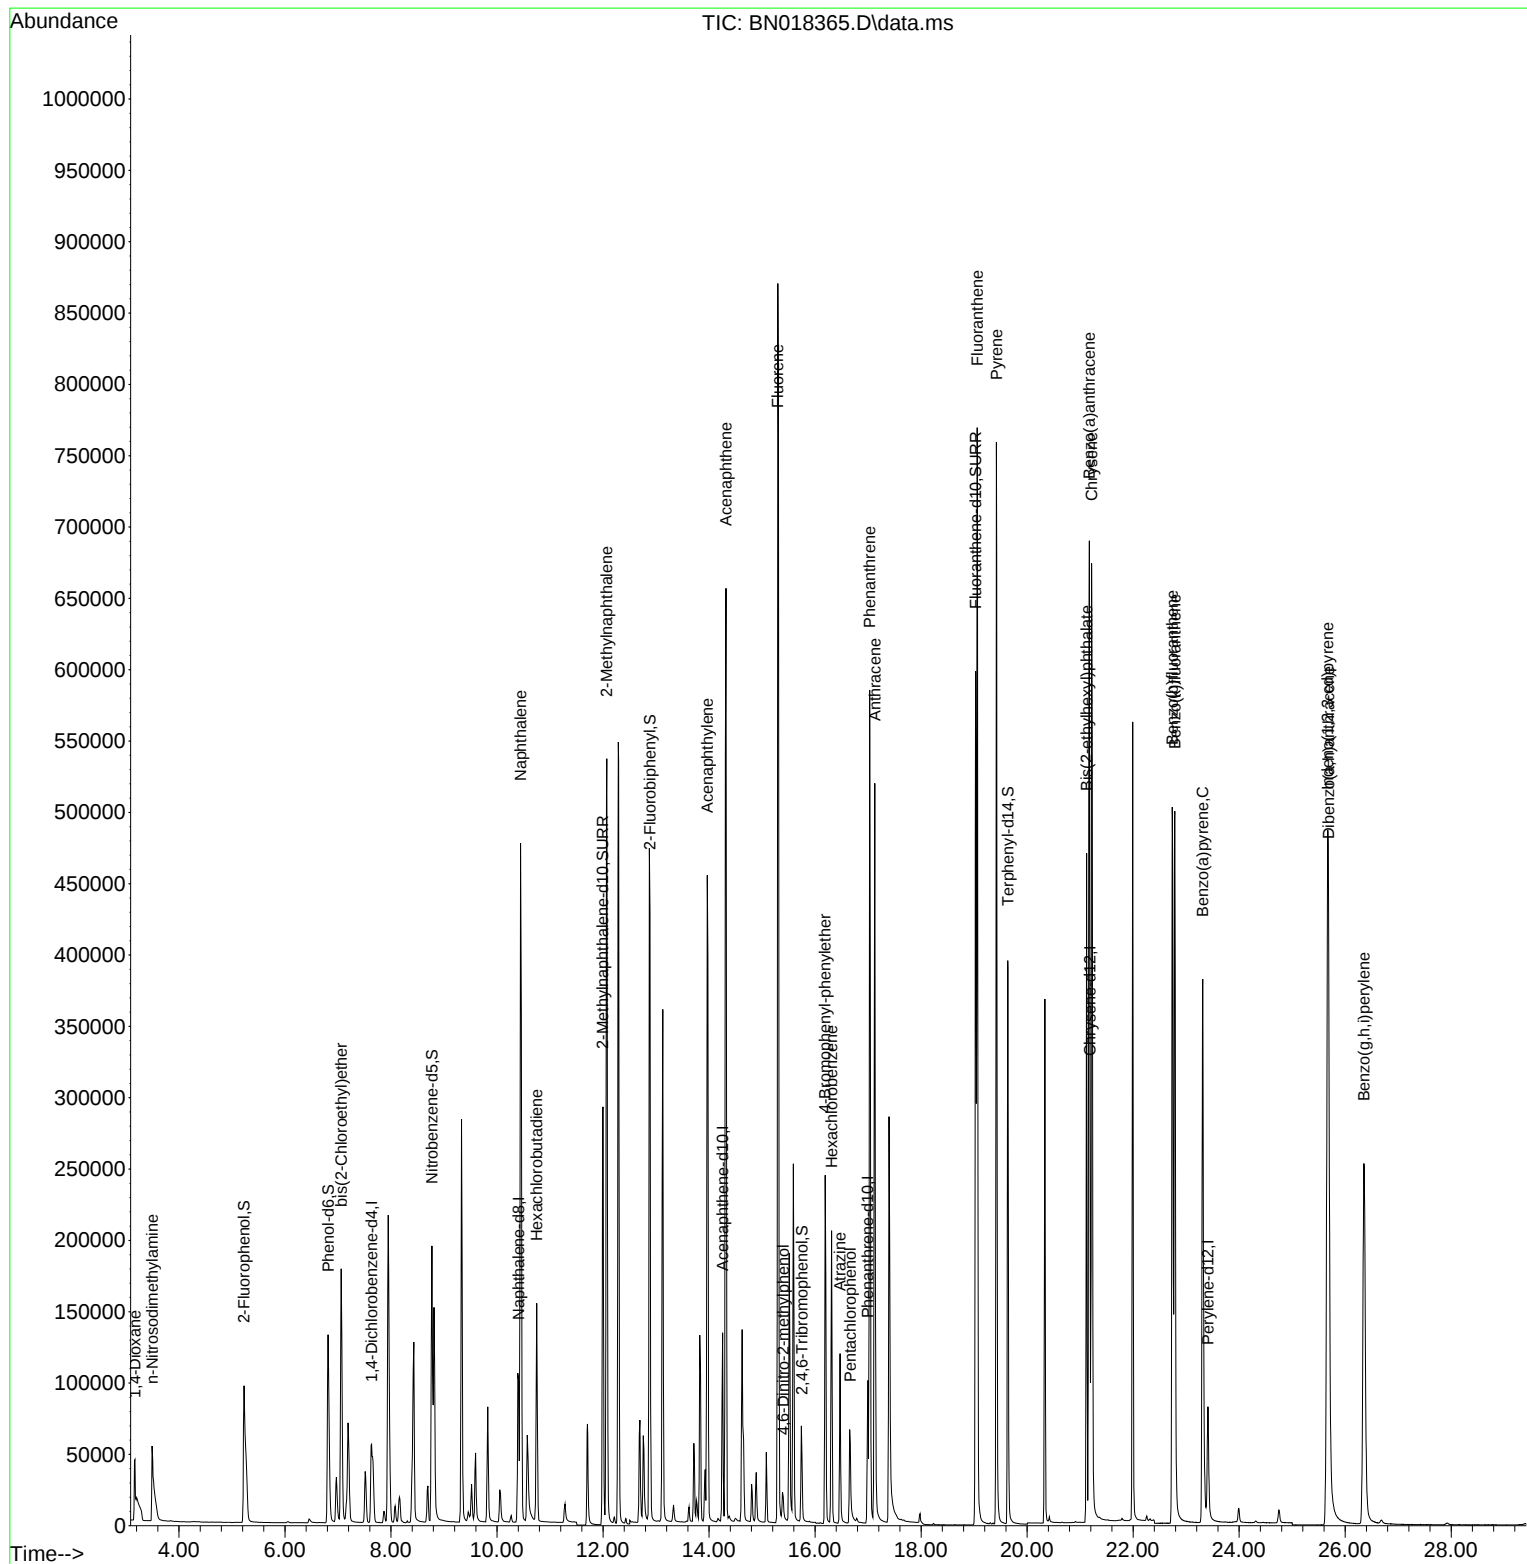


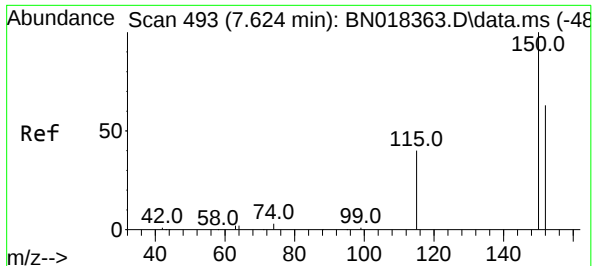

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.633 min Scan# 493
Delta R.T. 0.009 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 34144
Ion Ratio Lower Upper
152 100
150 156.0 121.7 182.5
115 60.3 43.8 65.8

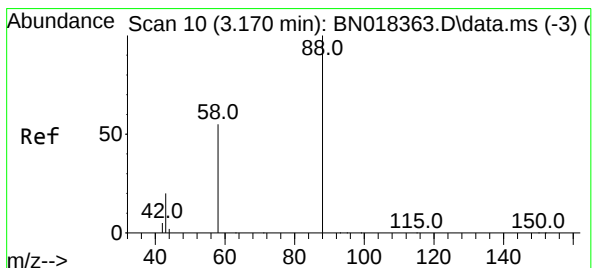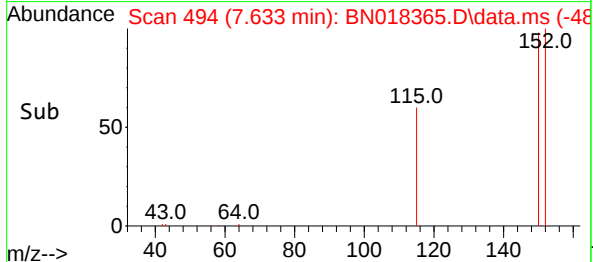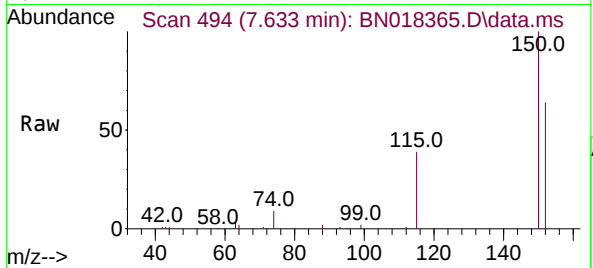

#2
1,4-Dioxane
Concen: 1.563 ng
RT: 3.170 min Scan# 10
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Tgt Ion: 88 Resp: 30443
Ion Ratio Lower Upper
88 100
43 31.3 69.7 104.5#
58 75.3 83.8 125.8#


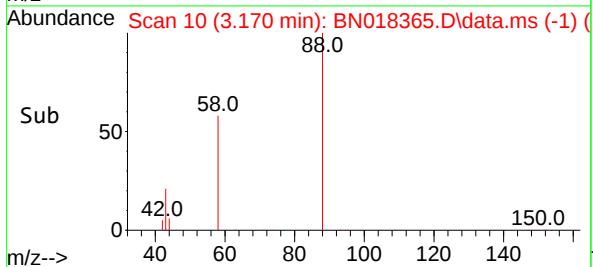

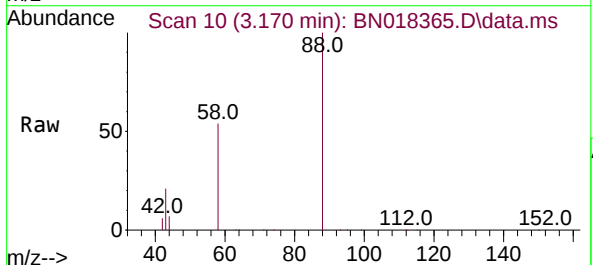


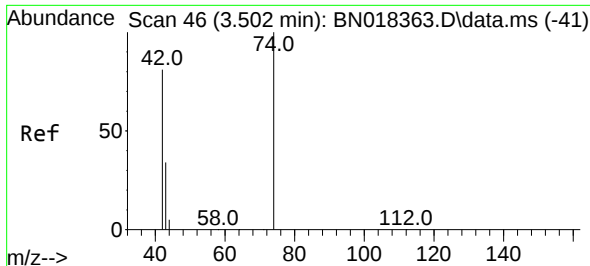

#3
n-Nitrosodimethylamine
Concen: 1.992 ng
RT: 3.493 min Scan# 41
Delta R.T. -0.009 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 55866
Ion Ratio Lower Upper
42 100
74 129.1 108.6 163.0
44 6.4 5.8 8.8

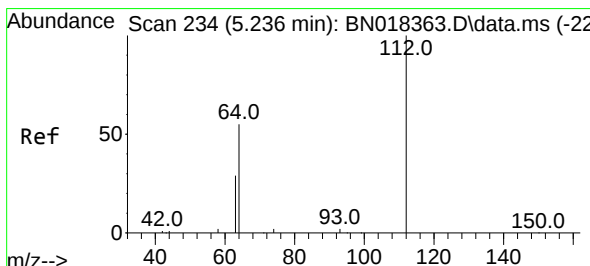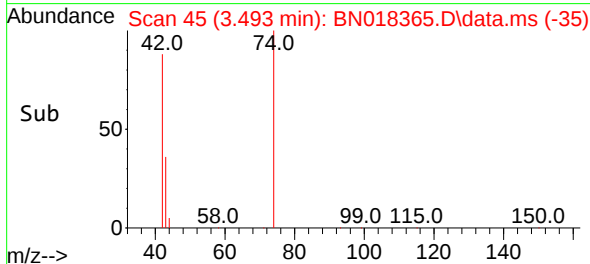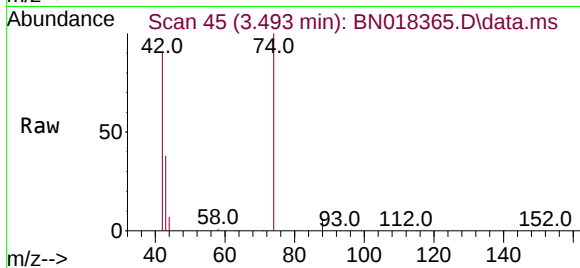

#4
2-Fluorophenol
Concen: 2.147 ng
RT: 5.227 min Scan# 233
Delta R.T. -0.009 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Tgt Ion: 112 Resp: 146882
Ion Ratio Lower Upper
112 100
64 59.9 48.0 72.0
63 31.6 25.3 37.9


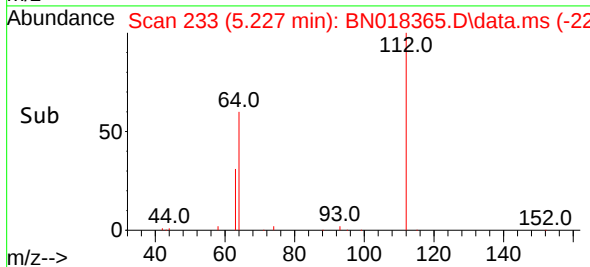

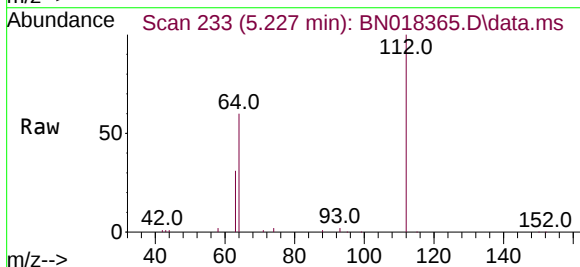




#5
Phenol-d6
Concen: 2.320 ng
RT: 6.813 min Scan# 405
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 153513
Ion Ratio Lower Upper
99 100
42 20.7 16.3 24.5
71 34.3 26.8 40.2

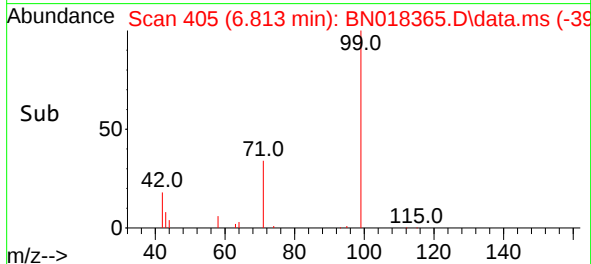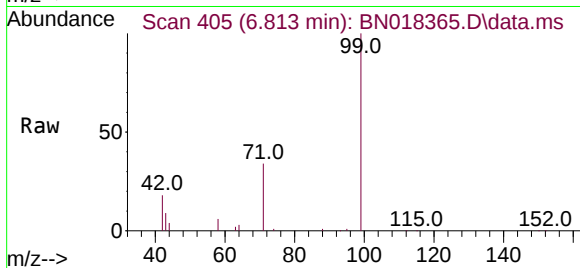

#6
bis(2-Chloroethyl)ether
Concen: 1.966 ng
RT: 7.062 min Scan# 432
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Tgt Ion: 93 Resp: 159739
Ion Ratio Lower Upper
93 100
63 76.9 61.7 92.5
95 32.5 26.2 39.4


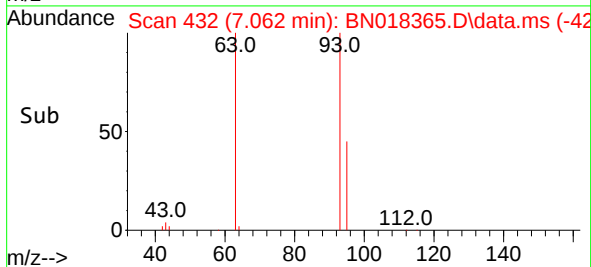

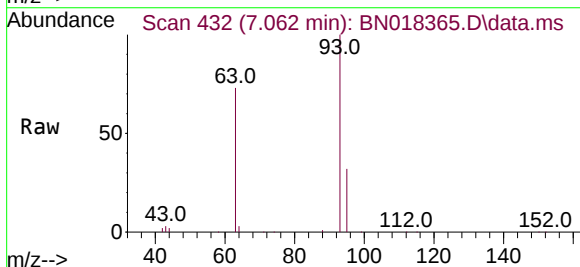




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.407 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:136 Resp: 151929
Ion Ratio Lower Upper
136 100
137 10.8 8.8 13.2
54 4.8 5.0 7.6#
68 4.2 4.4 6.6#

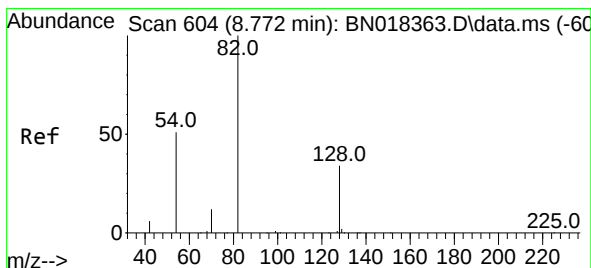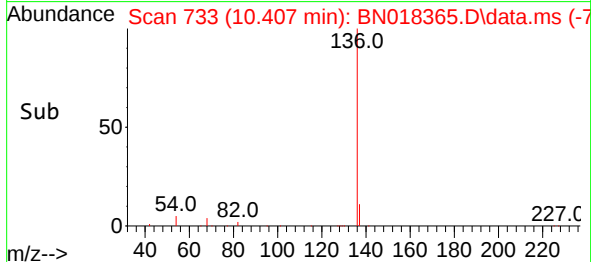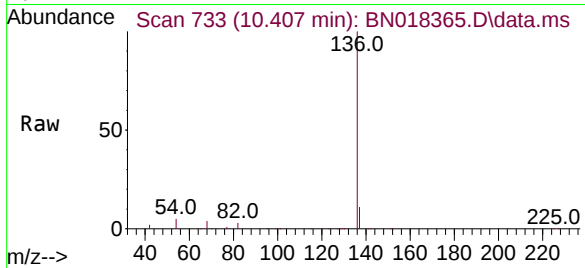

#8
Nitrobenzene-d5
Concen: 1.873 ng
RT: 8.772 min Scan# 604
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Tgt Ion: 82 Resp: 169165
Ion Ratio Lower Upper
82 100
128 38.7 33.7 50.5
54 47.0 36.6 55.0


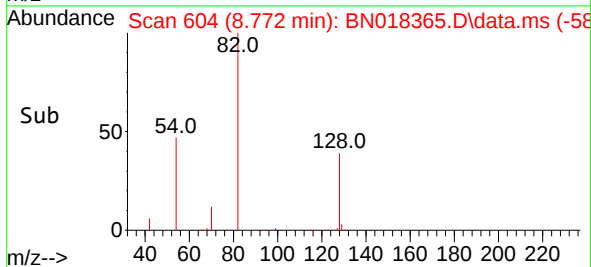

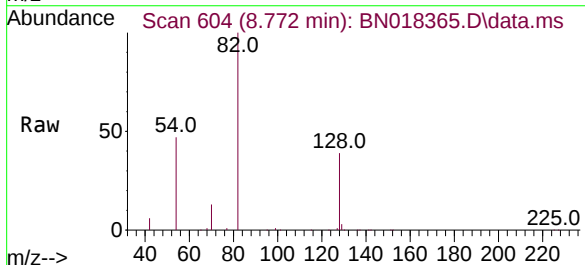




#9
Naphthalene
Concen: 1.700 ng
RT: 10.445 min Scan# 736
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:128 Resp: 638689
Ion Ratio Lower Upper
128 100
129 10.9 8.7 13.1
127 13.3 10.4 15.6

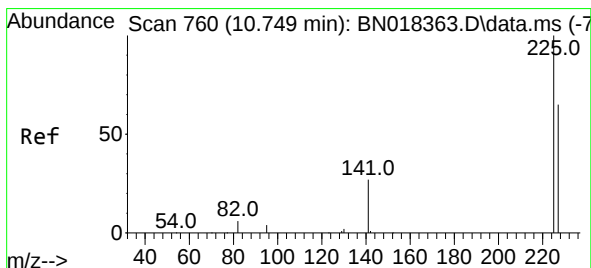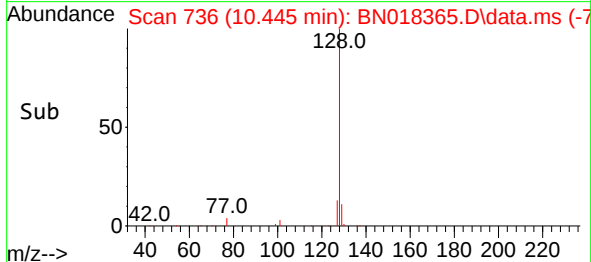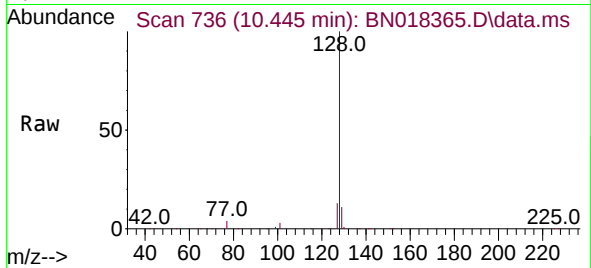

#10
Hexachlorobutadiene
Concen: 1.130 ng
RT: 10.749 min Scan# 760
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Tgt Ion:225 Resp: 118221
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.3 51.0 76.6

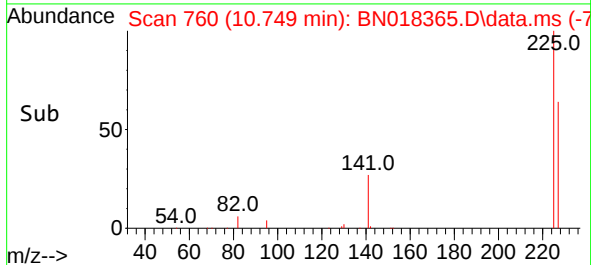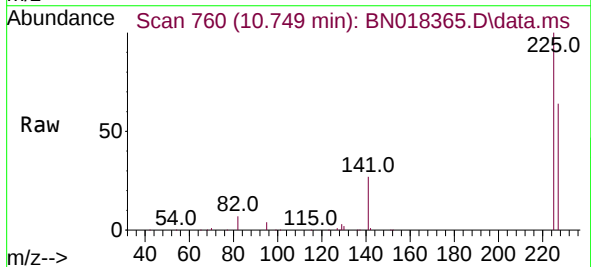

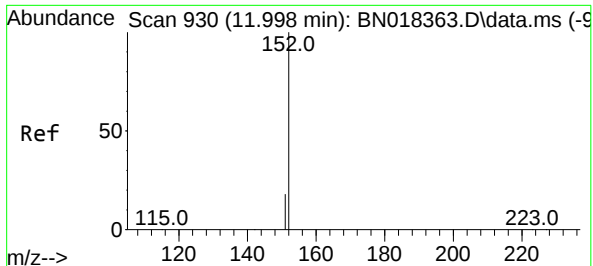

#11

2-Methylnaphthalene-d10

Concen: 1.576 ng

RT: 11.994 min Scan# 91

Delta R.T. -0.004 min

Lab File: BN018365.D

Acq: 07 Jan 2022 12:14

Instrument :

BNA_N

ClientSampleId :





SSTDICC1.6

Tgt Ion:152 Resp: 402793

Ion Ratio Lower Upper

152 100

151 20.4 16.2 24.2

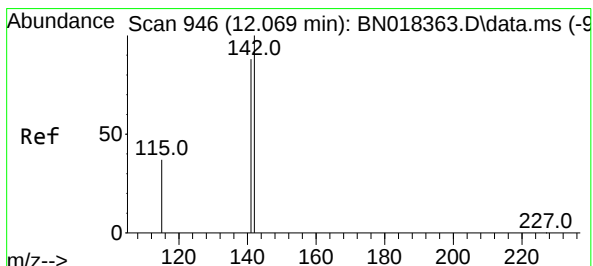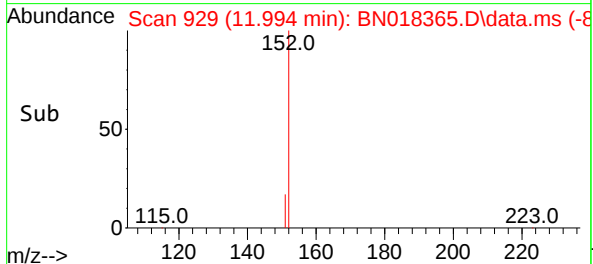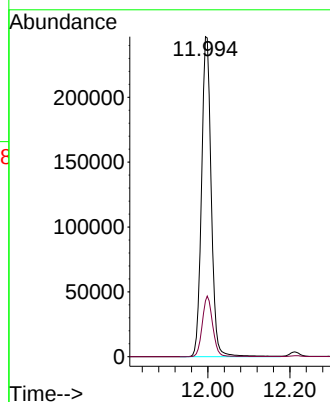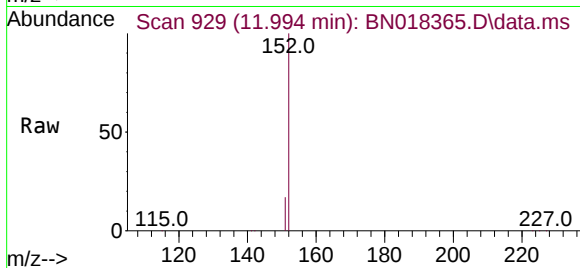

#12

2-Methylnaphthalene

Concen: 1.650 ng

RT: 12.070 min Scan# 946

Delta R.T. 0.000 min

Lab File: BN018365.D

Acq: 07 Jan 2022 12:14




Tgt Ion:142 Resp: 397328


Ion Ratio Lower Upper

142 100

141 87.5 70.0 105.0

115 35.9 27.8 41.8


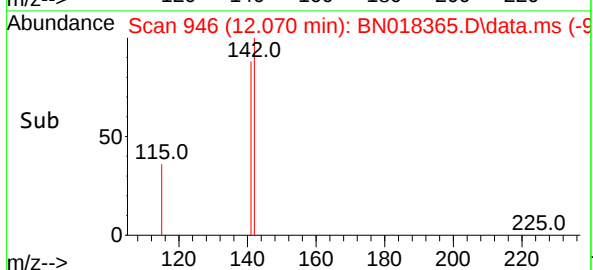
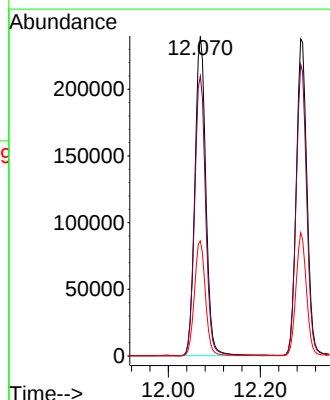
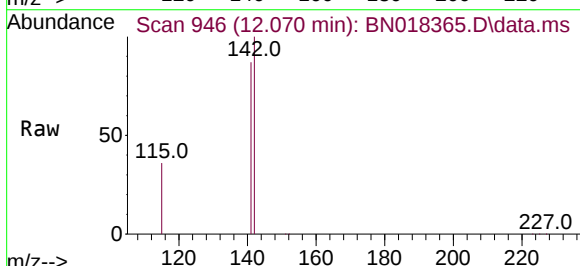


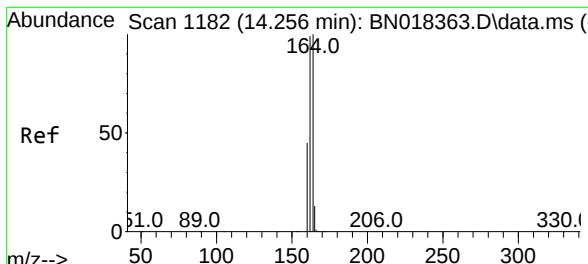

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.256 min Scan# 1182
 Delta R.T. 0.000 min
 Lab File: BN018365.D
 Acq: 07 Jan 2022 12:14




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	164	Resp:	75529
Ion Ratio	Lower	Upper	
164	100		
162	100.2	80.2	120.2
160	45.3	36.9	55.3

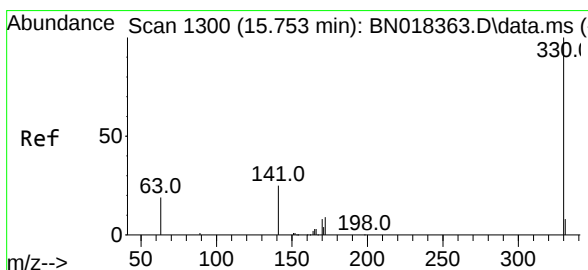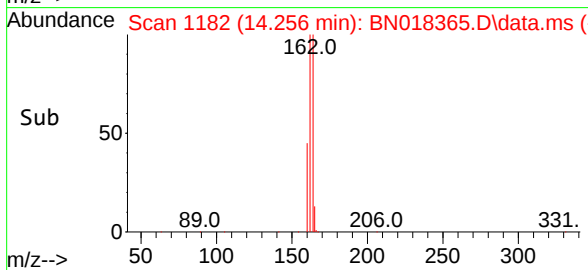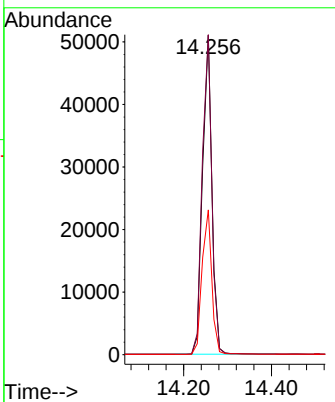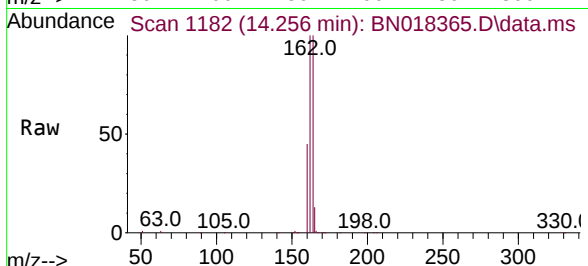

#14
 2,4,6-Tribromophenol
 Concen: 2.152 ng
 RT: 15.753 min Scan# 1300
 Delta R.T. 0.000 min
 Lab File: BN018365.D
 Acq: 07 Jan 2022 12:14

Tgt Ion:	330	Resp:	54559
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	35.3	21.3	31.9#


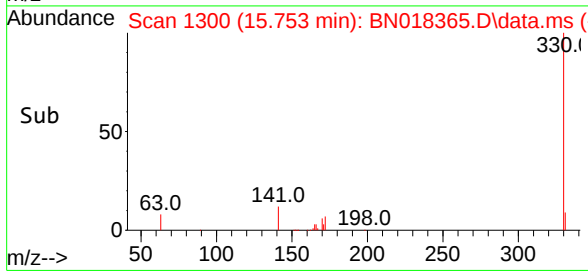
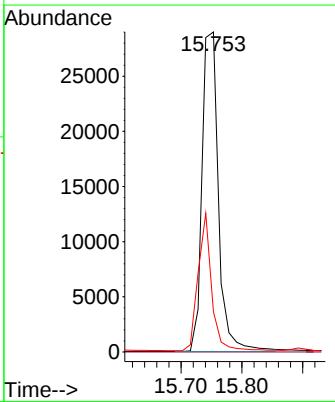
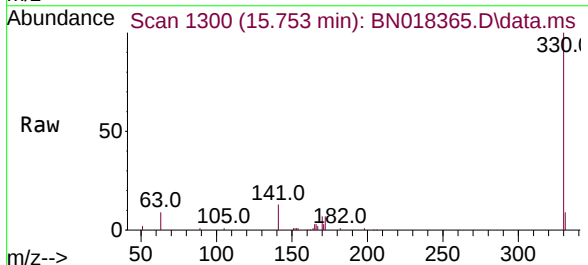


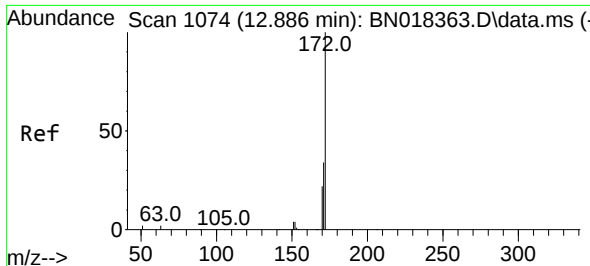

#15
2-Fluorobiphenyl
Concen: 1.627 ng
RT: 12.886 min Scan# 1074
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:172 Resp: 465080
Ion Ratio Lower Upper
172 100
171 33.1 27.4 41.0
170 21.3 18.4 27.6

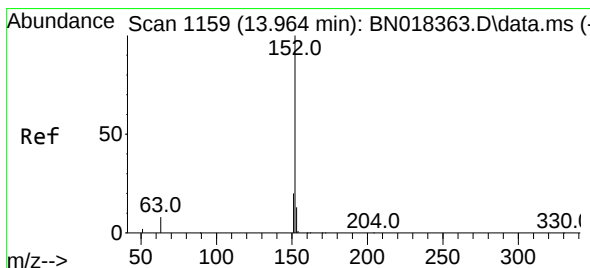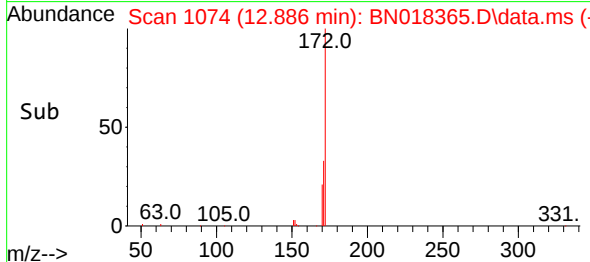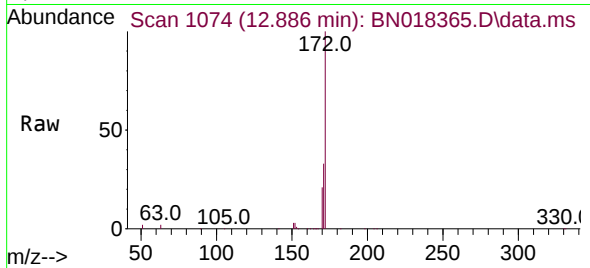

#16
Acenaphthylene
Concen: 2.071 ng
RT: 13.964 min Scan# 1159
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Tgt Ion:152 Resp: 550179
Ion Ratio Lower Upper
152 100
151 19.7 15.8 23.6
153 13.0 10.5 15.7


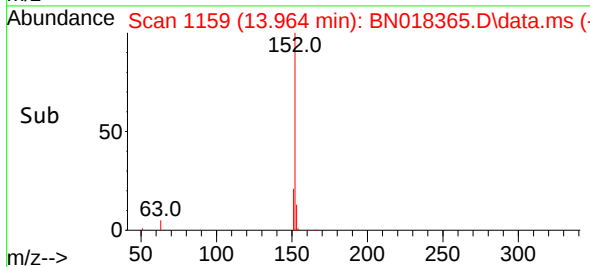

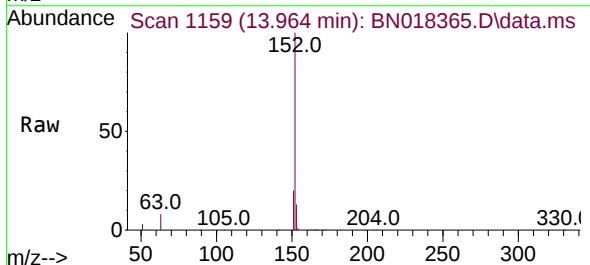


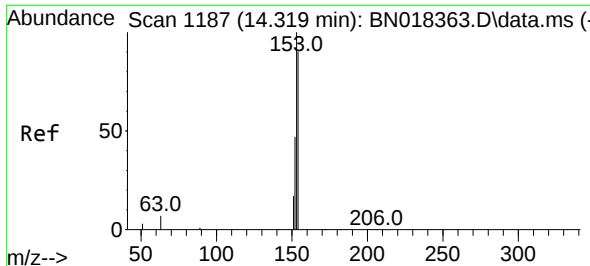

#17
Acenaphthene
Concen: 1.818 ng
RT: 14.320 min Scan# 1187
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 354643
Ion Ratio Lower Upper
154 100
153 113.0 90.9 136.3
152 54.8 45.0 67.4

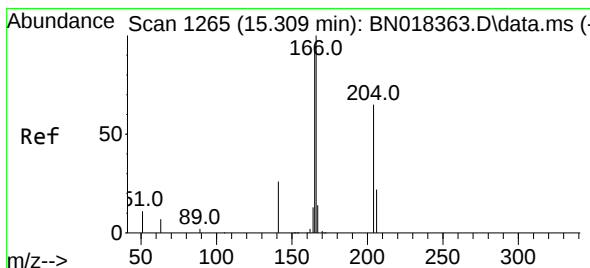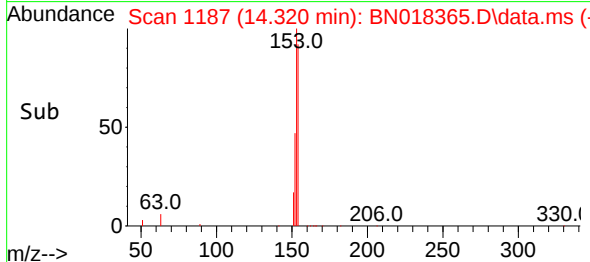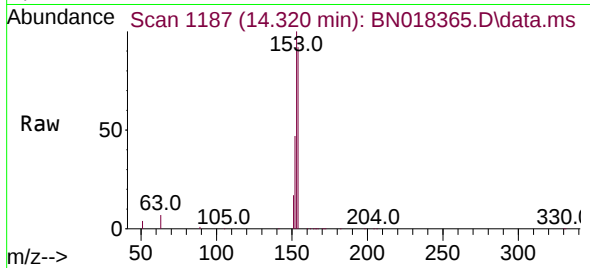

#18
Fluorene
Concen: 1.777 ng
RT: 15.296 min Scan# 1264
Delta R.T. -0.013 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Tgt Ion:166 Resp: 408282
Ion Ratio Lower Upper
166 100
165 97.4 77.8 116.6
167 13.5 10.9 16.3


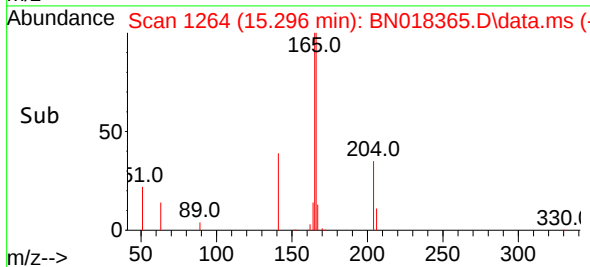

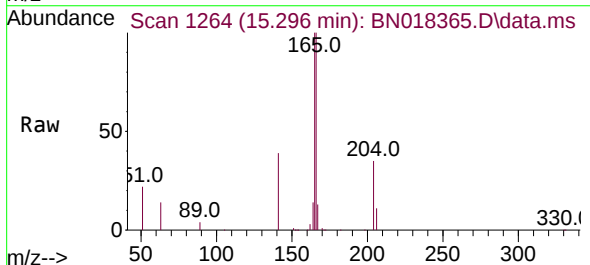




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.993 min Scan# 1401
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:188 Resp: 126093
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.0 7.0 10.4#

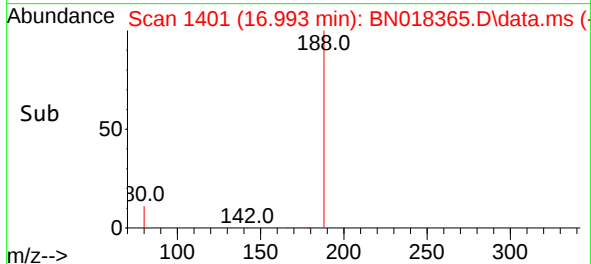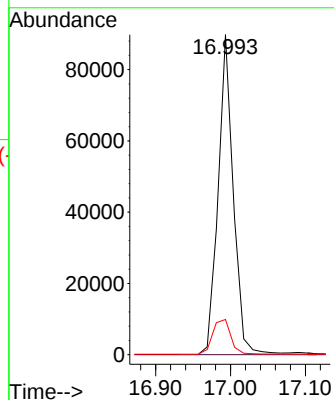

#20
4,6-Dinitro-2-methylphenol
Concen: 6.945 ng
RT: 15.398 min Scan# 1272
Delta R.T. -0.025 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Tgt Ion:198 Resp: 16555
Ion Ratio Lower Upper
198 100
182 10.4 15.5 23.3#
77 0.0 0.0 0.0


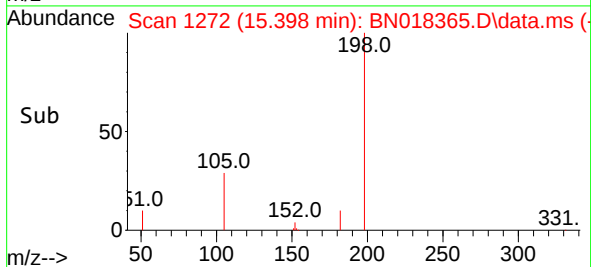
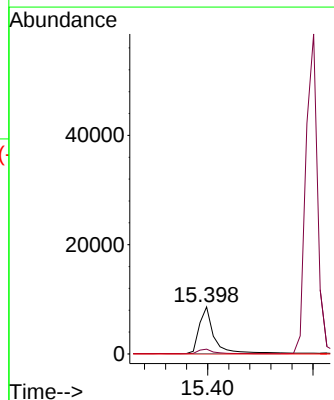
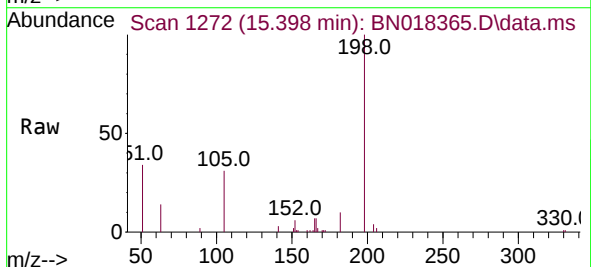


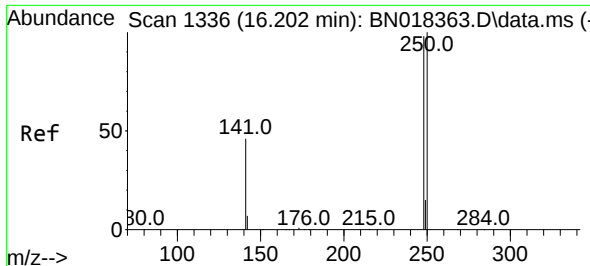

#21
4-Bromophenyl-phenylether
Concen: 1.640 ng
RT: 16.190 min Scan# 1335
Delta R.T. -0.012 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 125593
Ion Ratio Lower Upper
248 100
250 90.0 74.4 111.6
141 88.7 43.7 65.5#

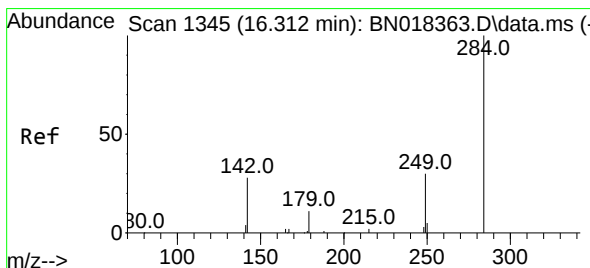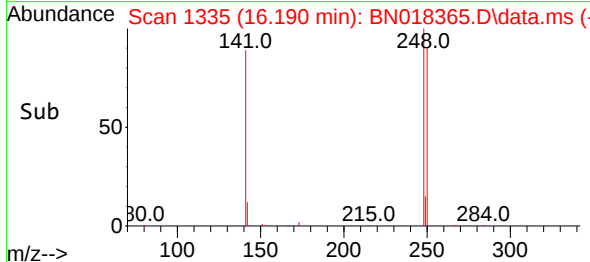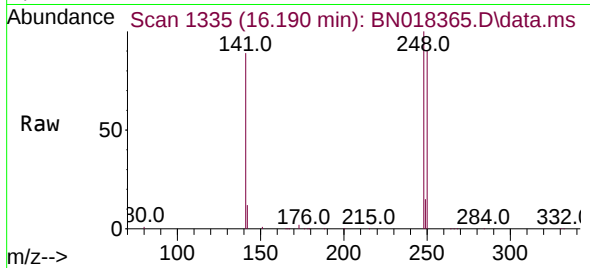

#22
Hexachlorobenzene
Concen: 1.577 ng
RT: 16.312 min Scan# 1345
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Tgt Ion:284 Resp: 153892
Ion Ratio Lower Upper
284 100
142 36.7 21.6 32.4#
249 29.0 23.5 35.3

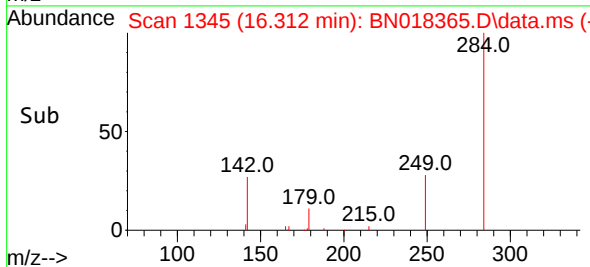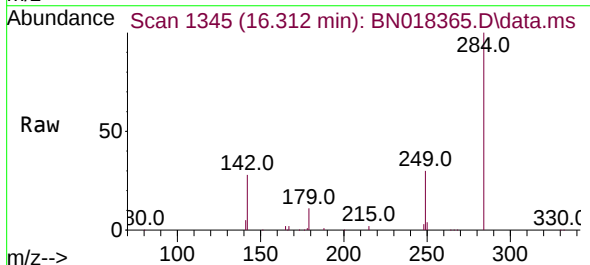

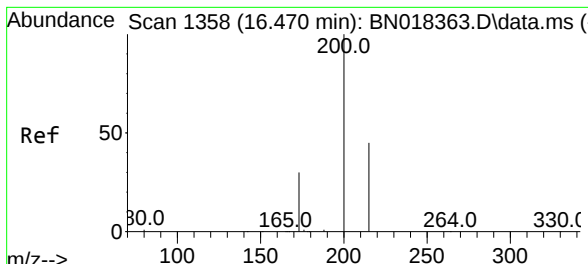

#23

Atrazine

Concen: 1.985 ng

RT: 16.470 min Scan# 1358

Delta R.T. 0.000 min

Lab File: BN018365.D

Acq: 07 Jan 2022 12:14

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:200 Resp: 91356

Ion Ratio Lower Upper

200 100

173 26.7 20.3 30.5

215 46.5 40.4 60.6

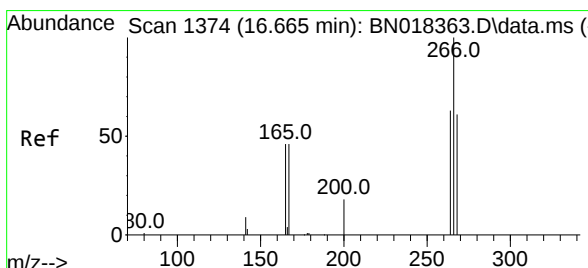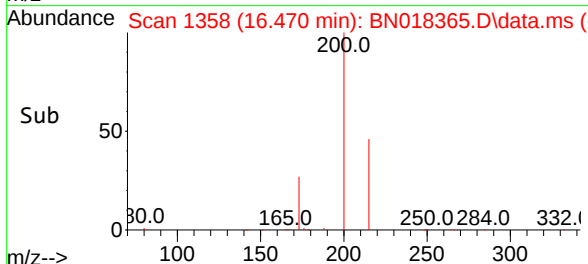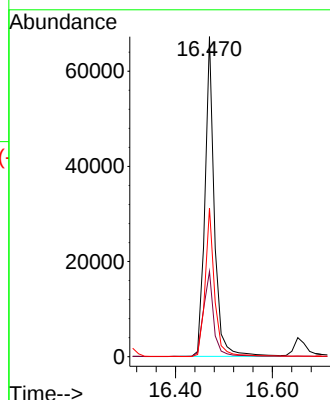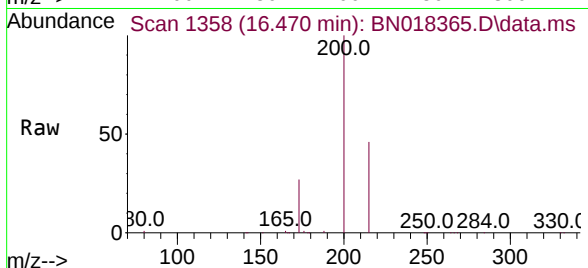

#24

Pentachlorophenol

Concen: 3.041 ng

RT: 16.665 min Scan# 1374

Delta R.T. 0.000 min

Lab File: BN018365.D

Acq: 07 Jan 2022 12:14




Tgt Ion:266 Resp: 41292


Ion Ratio Lower Upper

266 100

264 62.4 49.5 74.3

268 63.8 50.6 76.0

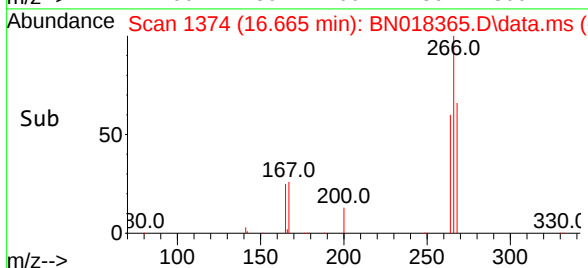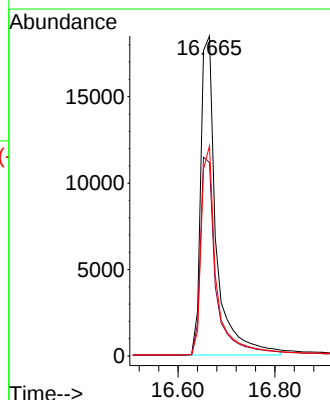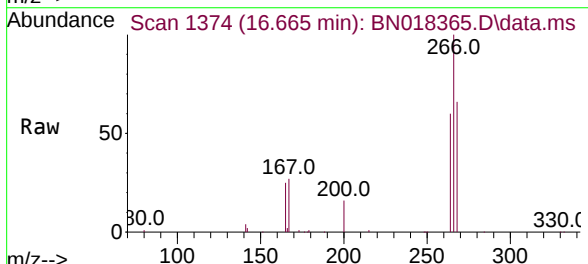




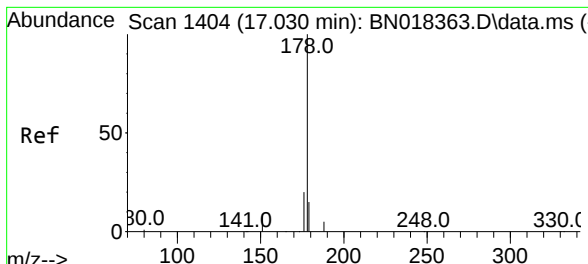


#25
 Phenanthrene
 Concen: 1.833 ng
 RT: 17.030 min Scan# 1404
 Delta R.T. 0.000 min
 Lab File: BN018365.D
 Acq: 07 Jan 2022 12:14

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:178 Resp: 609435




Ion	Ratio	Lower	Upper
178	100		
176	19.1	15.3	22.9
179	15.2	12.3	18.5

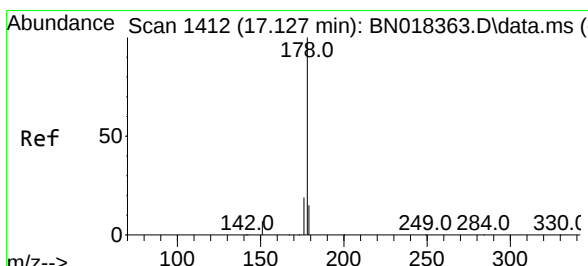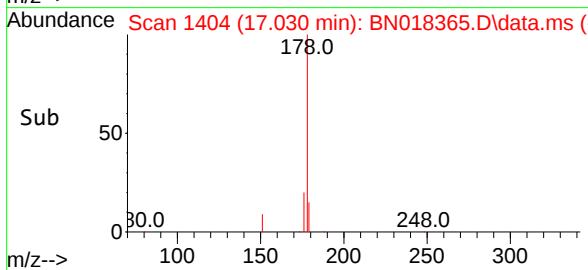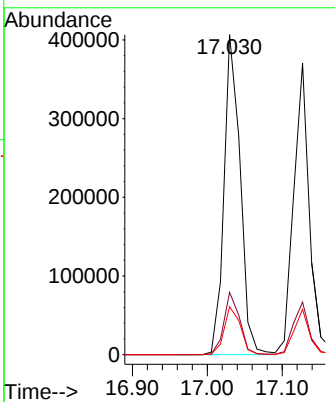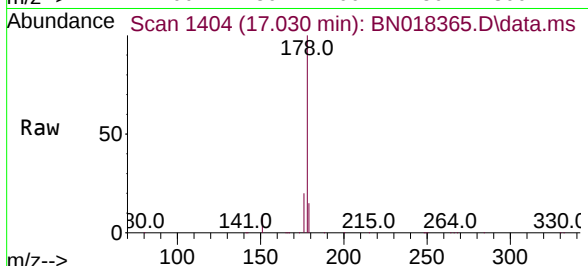


#26
 Anthracene
 Concen: 2.074 ng
 RT: 17.127 min Scan# 1412
 Delta R.T. 0.000 min
 Lab File: BN018365.D
 Acq: 07 Jan 2022 12:14

Tgt Ion:178 Resp: 543556

Ion	Ratio	Lower	Upper
178	100		
176	18.4	14.8	22.2
179	15.3	12.2	18.4


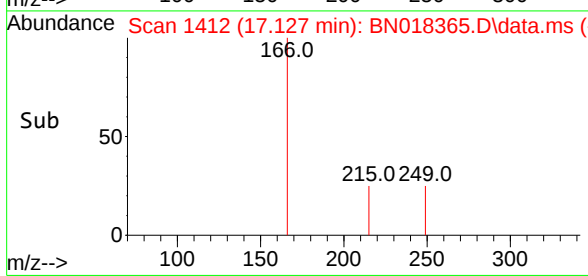
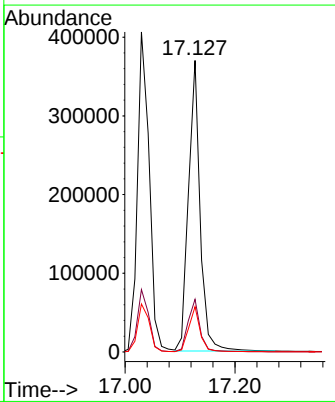
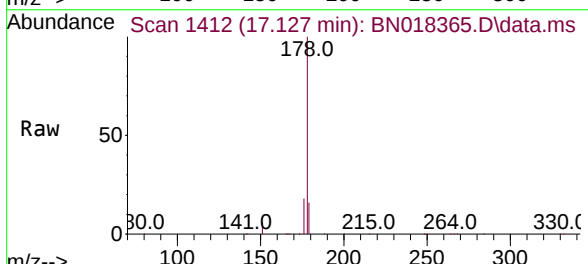


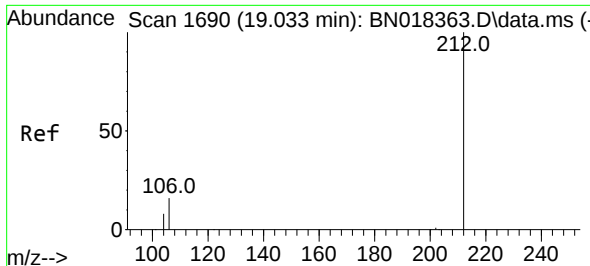

#27
Fluoranthene-d10
Concen: 1.582 ng
RT: 19.028 min Scan# 1689
Delta R.T. -0.005 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 634850
Ion Ratio Lower Upper
212 100
106 16.7 8.4 12.6#
104 9.1 4.5 6.7#

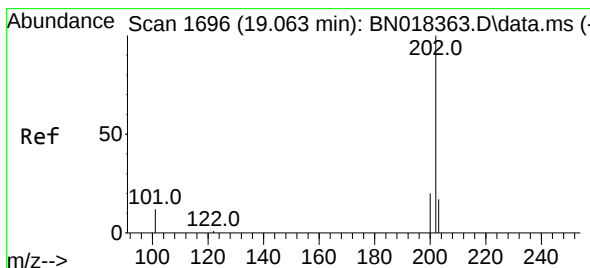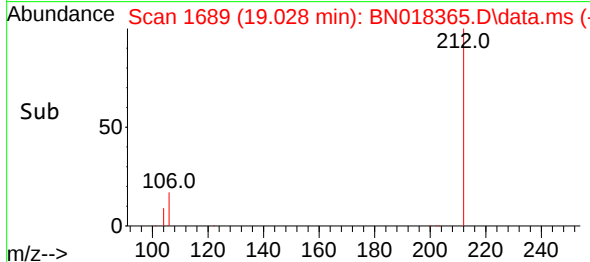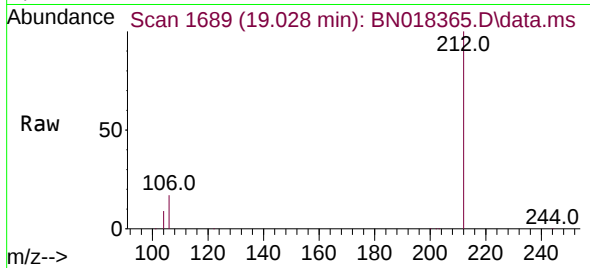

#28
Fluoranthene
Concen: 1.690 ng
RT: 19.058 min Scan# 1695
Delta R.T. -0.005 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Tgt Ion:202 Resp: 657911
Ion Ratio Lower Upper
202 100
101 13.6 7.2 10.8#
203 17.4 13.7 20.5


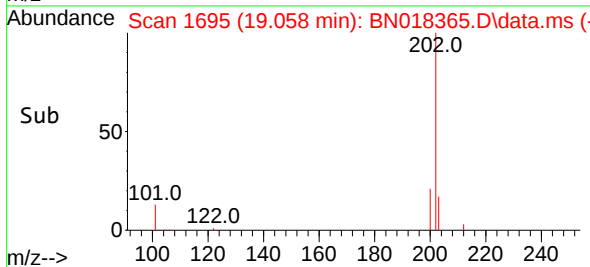

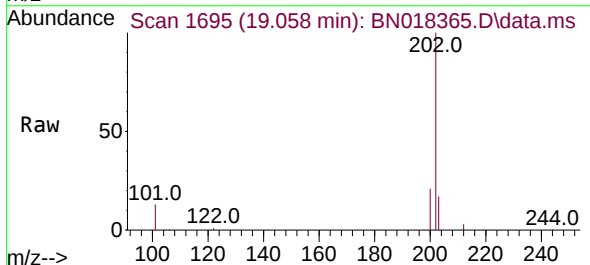


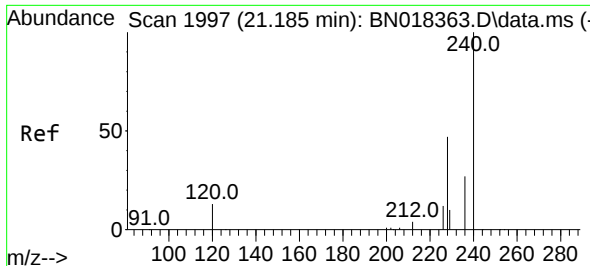

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.185 min Scan# 1997
Delta R.T. 0.000 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:240 Resp: 115738
Ion Ratio Lower Upper
240 100
120 10.6 6.0 9.0#
236 26.6 21.4 32.2

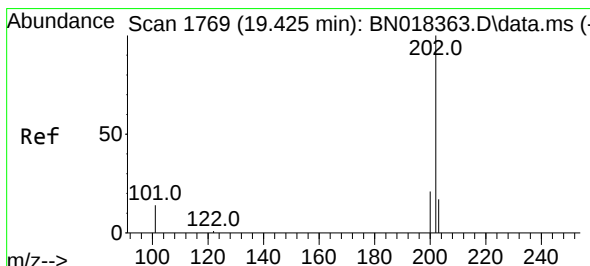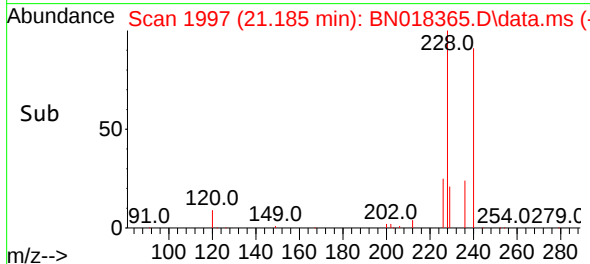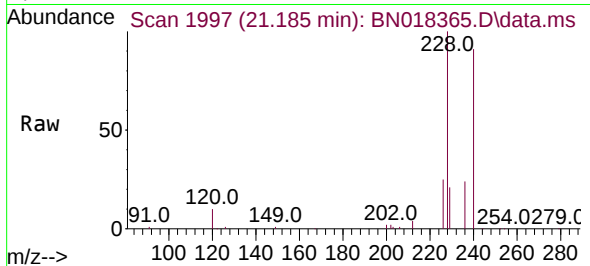

#30
Pyrene
Concen: 1.469 ng
RT: 19.420 min Scan# 1768
Delta R.T. -0.005 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Tgt Ion:202 Resp: 666493
Ion Ratio Lower Upper
202 100
200 21.0 16.6 25.0
203 17.5 14.1 21.1


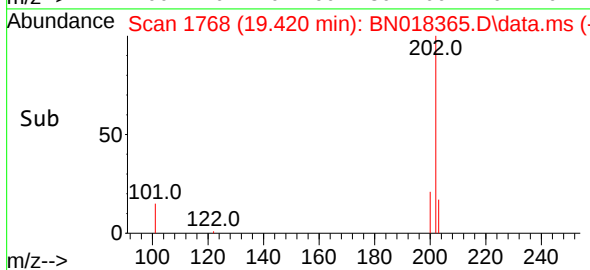

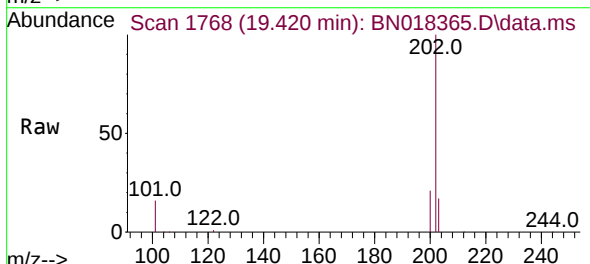




#31
 Terphenyl-d14
 Concen: 1.412 ng
 RT: 19.639 min Scan# 1812
 Delta R.T. 0.000 min
 Lab File: BN018365.D
 Acq: 07 Jan 2022 12:14




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:244 Resp: 415242
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.2 9.2
 122 14.0 7.9 11.9#

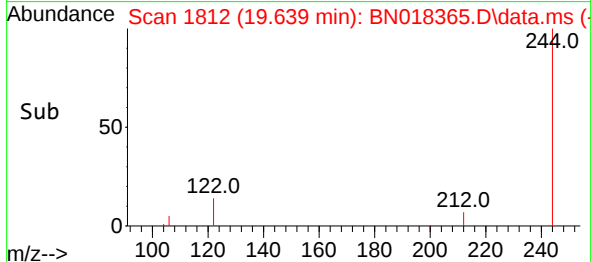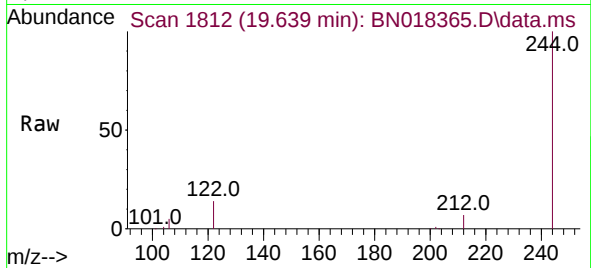

#32
 Benzo(a)anthracene
 Concen: 2.007 ng
 RT: 21.174 min Scan# 1996
 Delta R.T. 0.000 min
 Lab File: BN018365.D
 Acq: 07 Jan 2022 12:14

Tgt Ion:228 Resp: 622448
 Ion Ratio Lower Upper
 228 100
 226 25.9 21.3 31.9
 229 20.2 15.9 23.9

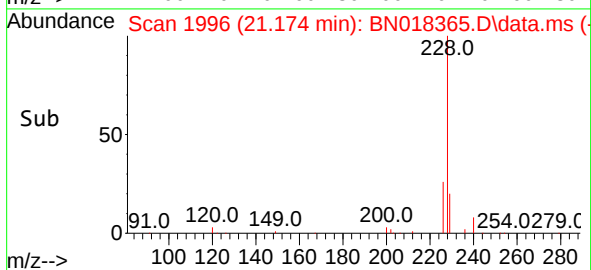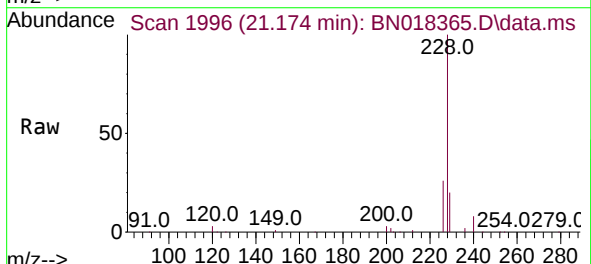

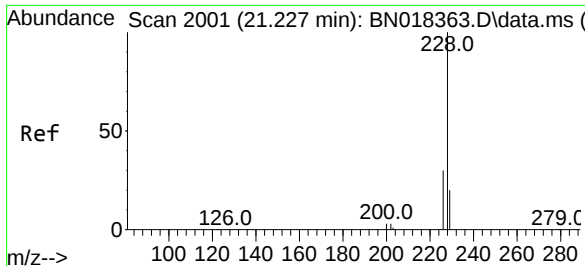

#33

Chrysene

Concen: 1.694 ng

RT: 21.217 min Scan# 2000

Delta R.T. -0.011 min

Lab File: BN018365.D

Acq: 07 Jan 2022 12:14

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:228 Resp: 631347

Ion Ratio Lower Upper

228 100

226 30.9 24.2 36.4

229 19.0 15.5 23.3

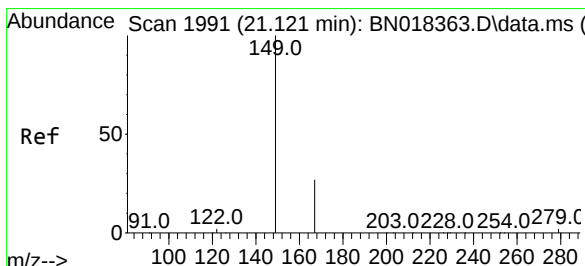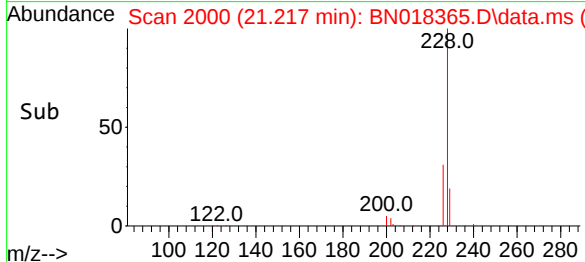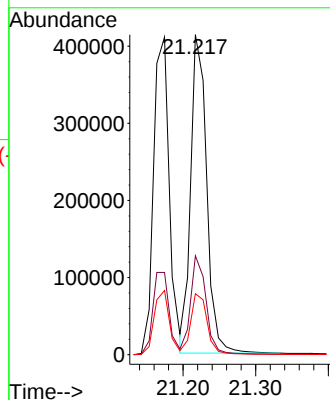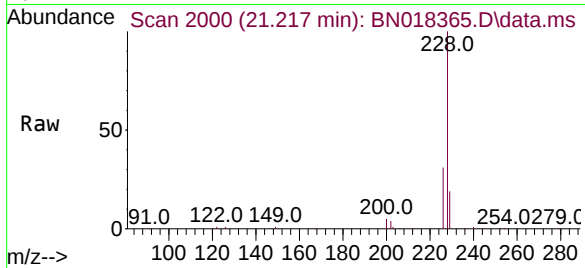

#34

Bis(2-ethylhexyl)phthalate

Concen: 2.542 ng

RT: 21.121 min Scan# 1991

Delta R.T. 0.000 min

Lab File: BN018365.D

Acq: 07 Jan 2022 12:14




Tgt Ion:149 Resp: 367249


Ion Ratio Lower Upper

149 100

167 26.9 23.7 35.5

279 3.2 3.6 5.4#

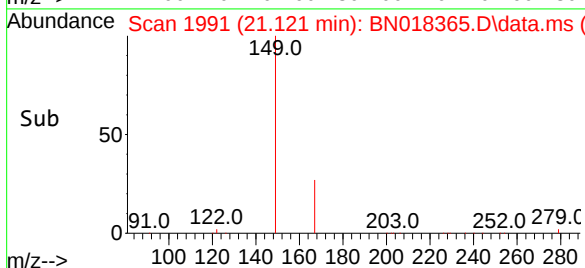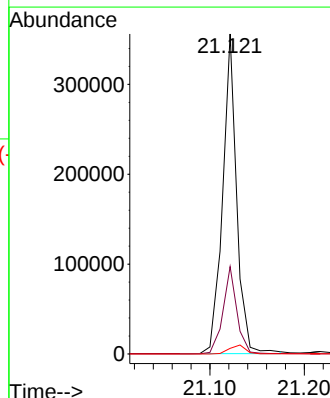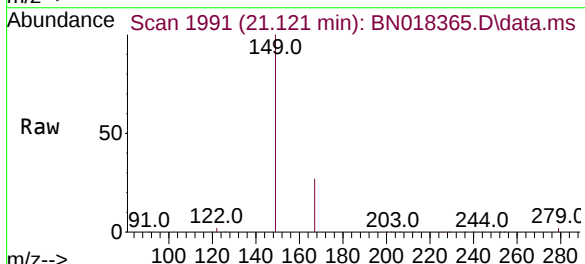

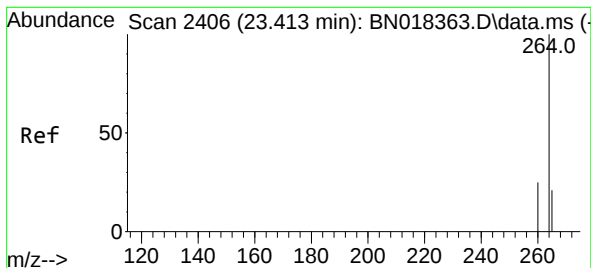

#35

Perylene-d12

Concen: 0.400 ng

RT: 23.409 min Scan# 2405

Delta R.T. -0.003 min

Lab File: BN018365.D

Acq: 07 Jan 2022 12:14

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:264 Resp: 111242

Ion Ratio Lower Upper

264 100

260 25.2 20.2 30.4

265 22.5 18.2 27.2

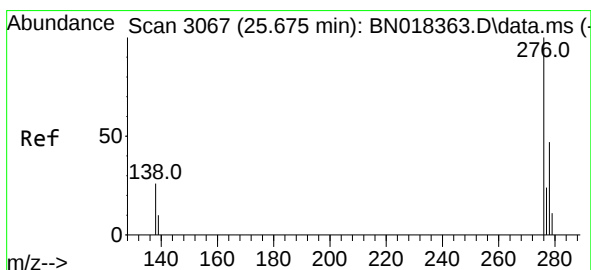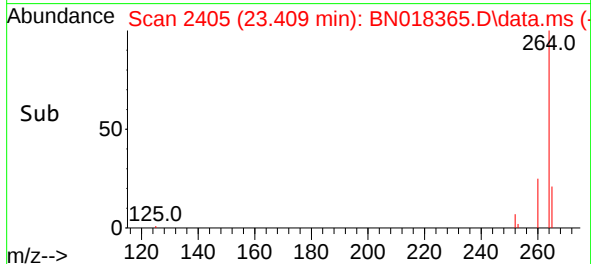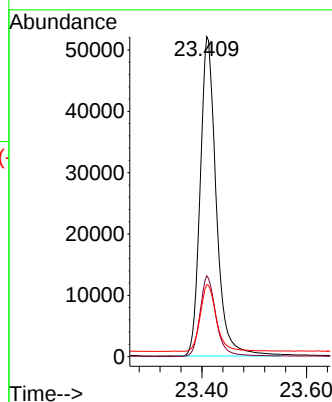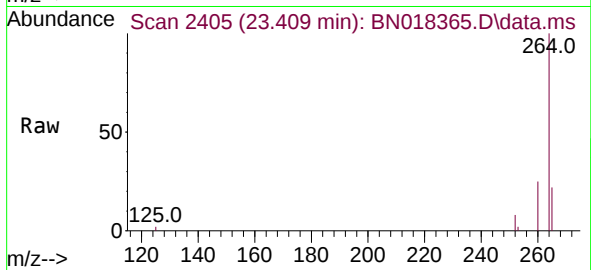

#36

Indeno(1,2,3-cd)pyrene

Concen: 2.418 ng

RT: 25.668 min Scan# 3065

Delta R.T. -0.007 min

Lab File: BN018365.D

Acq: 07 Jan 2022 12:14




Tgt Ion:276 Resp: 642403


Ion Ratio Lower Upper

276 100

138 28.4 14.9 22.3#

277 25.0 19.9 29.9

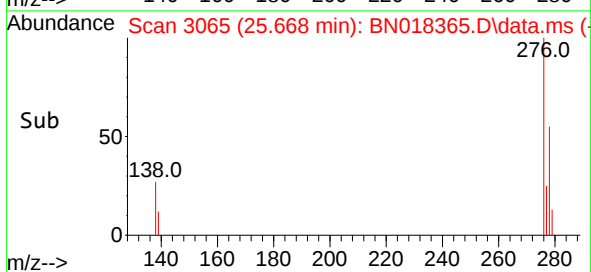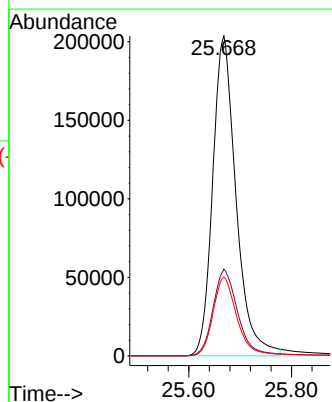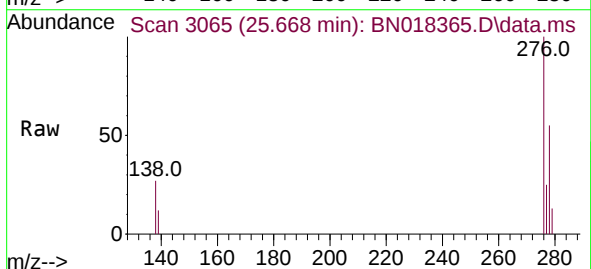



#37

Benzo(b)fluoranthene

Concen: 1.773 ng

RT: 22.738 min Scan# 2209

Delta R.T. -0.003 min

Lab File: BN018365.D

Acq: 07 Jan 2022 12:14

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:252 Resp: 626672

Ion Ratio Lower Upper

252 100

253 21.8 17.8 26.6

125 11.7 6.0 9.0#

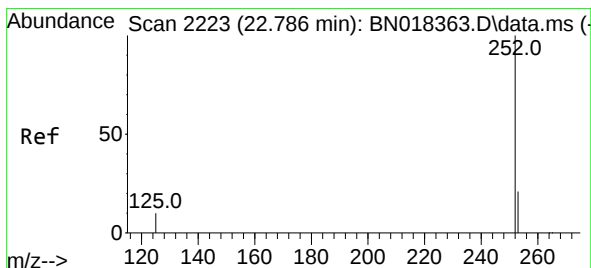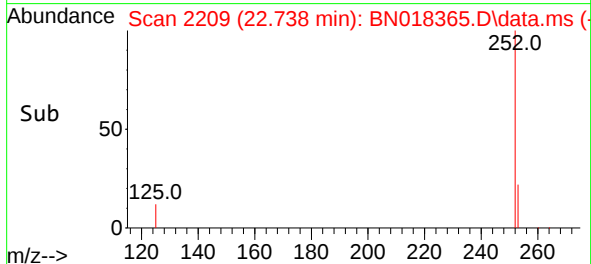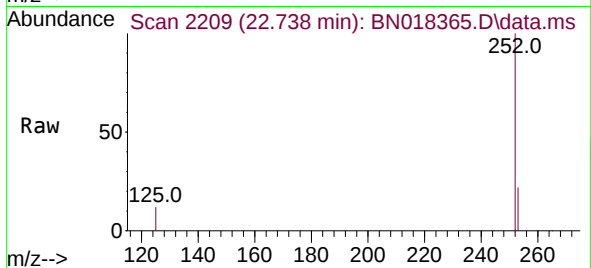

#38

Benzo(k)fluoranthene

Concen: 1.844 ng

RT: 22.786 min Scan# 2223

Delta R.T. 0.000 min

Lab File: BN018365.D

Acq: 07 Jan 2022 12:14




Tgt Ion:252 Resp: 617014


Ion Ratio Lower Upper

252 100

253 21.9 17.7 26.5

125 11.7 6.2 9.2#


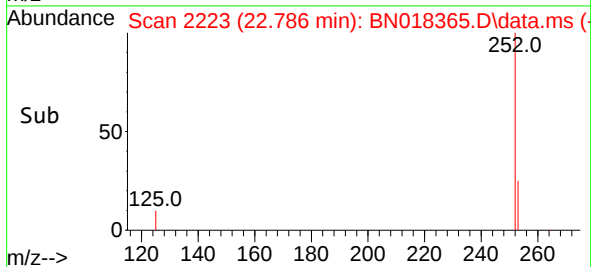

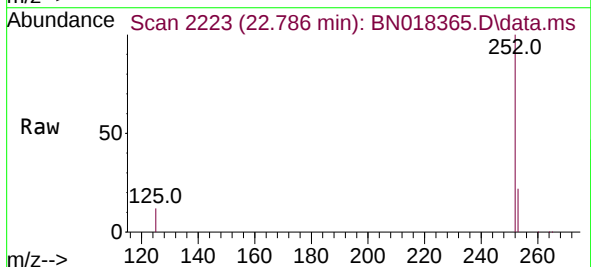




#39
Benzo(a)pyrene
Concen: 1.864 ng
RT: 23.313 min Scan# 21
Delta R.T. -0.003 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 573376
Ion Ratio Lower Upper
252 100
253 21.8 17.8 26.6
125 12.8 7.0 10.4#

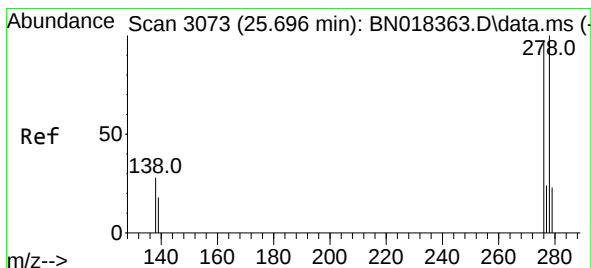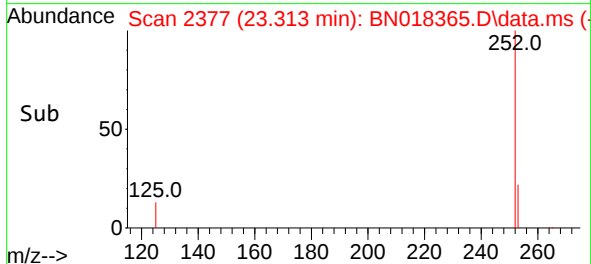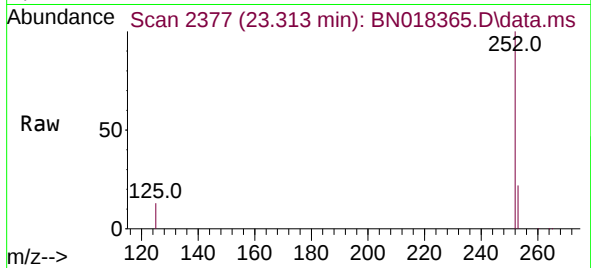

#40
Dibenzo(a,h)anthracene
Concen: 2.615 ng
RT: 25.685 min Scan# 3070
Delta R.T. -0.010 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14


Tgt Ion:278 Resp: 495265
Ion Ratio Lower Upper
278 100
139 18.8 10.8 16.2#
279 23.7 19.0 28.4

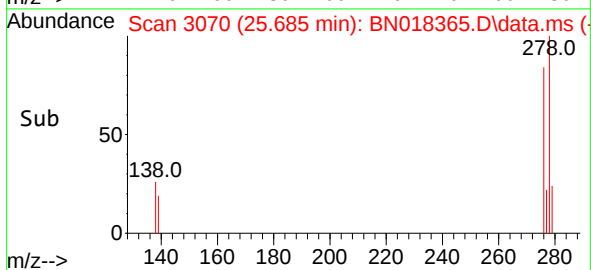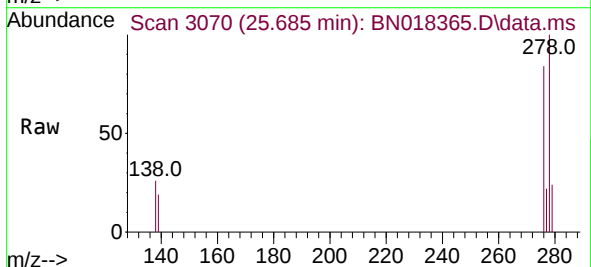

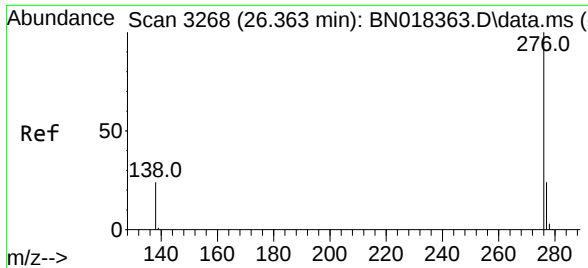

#41
Benzo(g,h,i)perylene
Concen: 2.114 ng
RT: 26.353 min Scan# 31
Delta R.T. -0.010 min
Lab File: BN018365.D
Acq: 07 Jan 2022 12:14

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

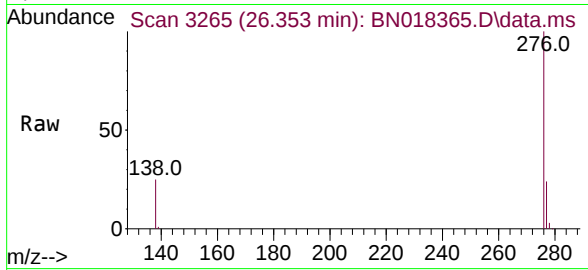

Tgt Ion:276 Resp: 560376
Ion Ratio Lower Upper
276 100
277 23.8 19.0 28.6
138 24.8 12.6 19.0#

