
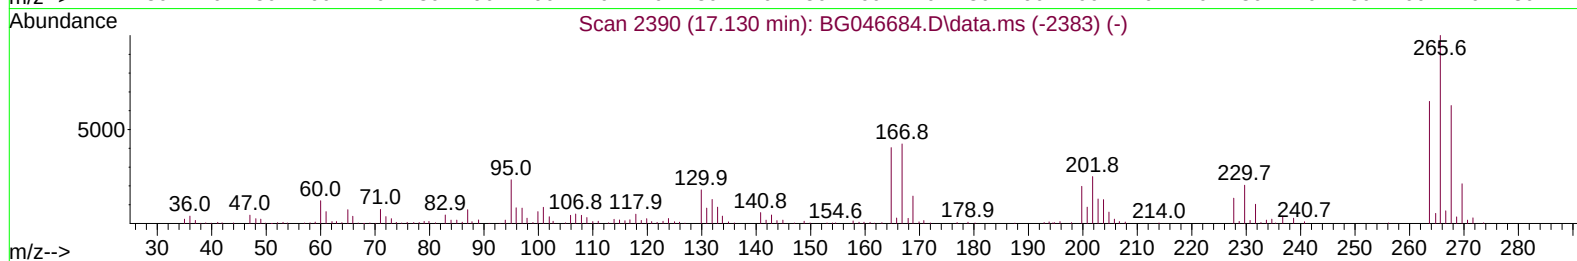
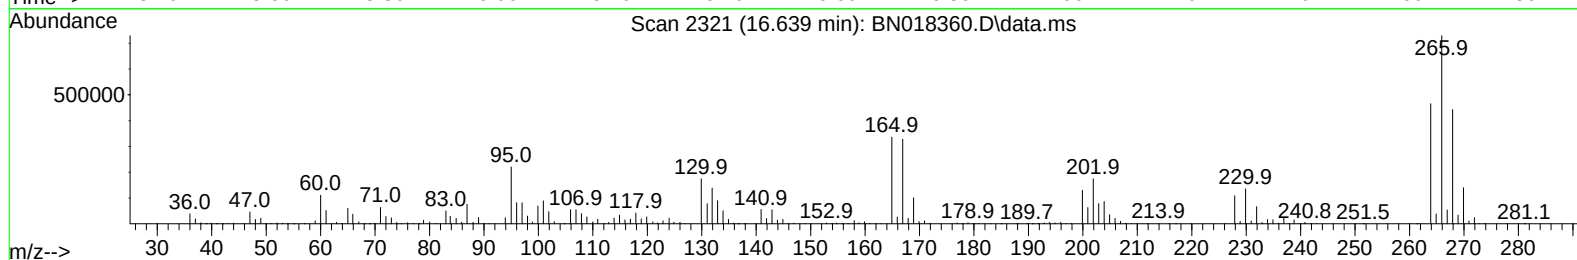


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010722\
 Data File : BN018360.D
 Acq On : 07 Jan 2022 09:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 14:34:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 07 14:34:24 2022
 Response via : Initial Calibration

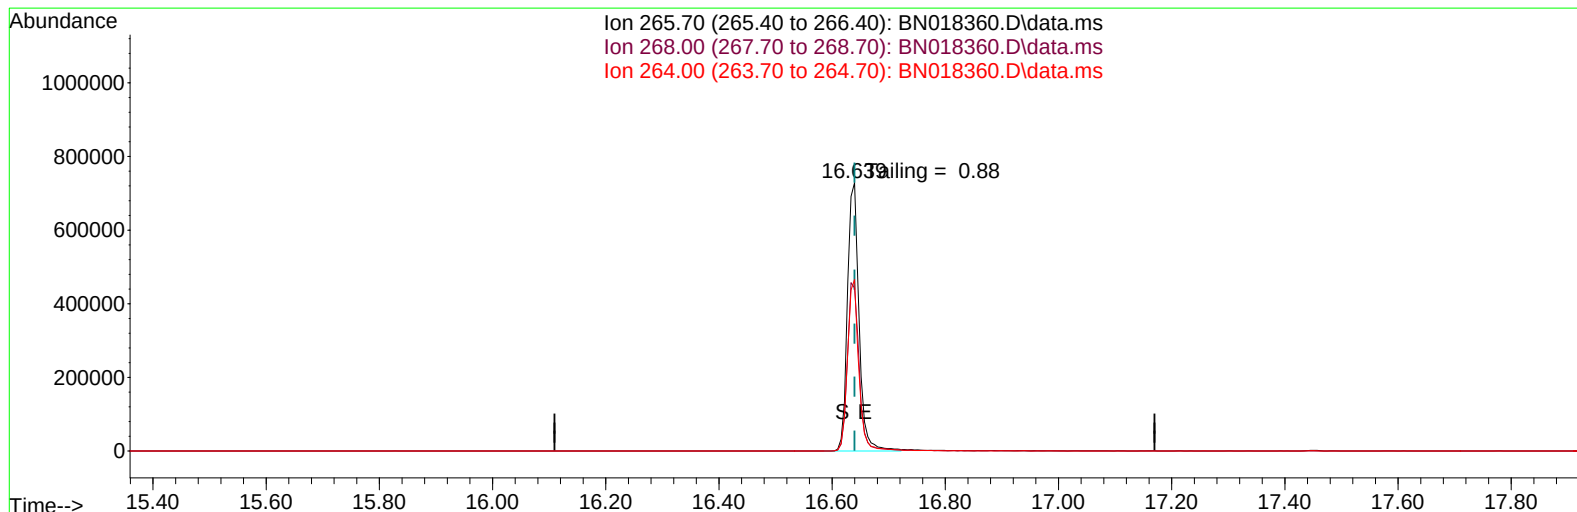

TIC: BN018360.D\data.ms

(70) Pentachlorophenol (C)




16.639min (0.000) 23583.89 ng

response 1045149

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.76
264.00	61.60	63.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010722\
Data File : BN018360.D
Acq On : 07 Jan 2022 09:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 14:34:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 07 14:34:24 2022
Response via : Initial Calibration

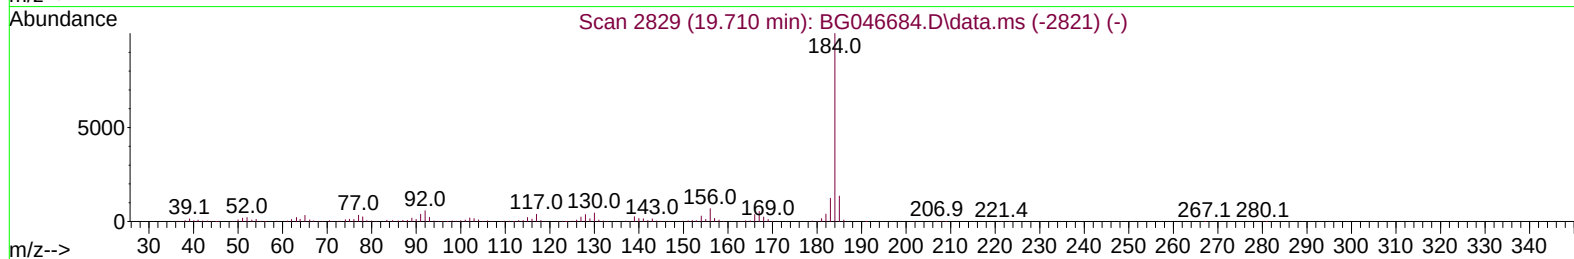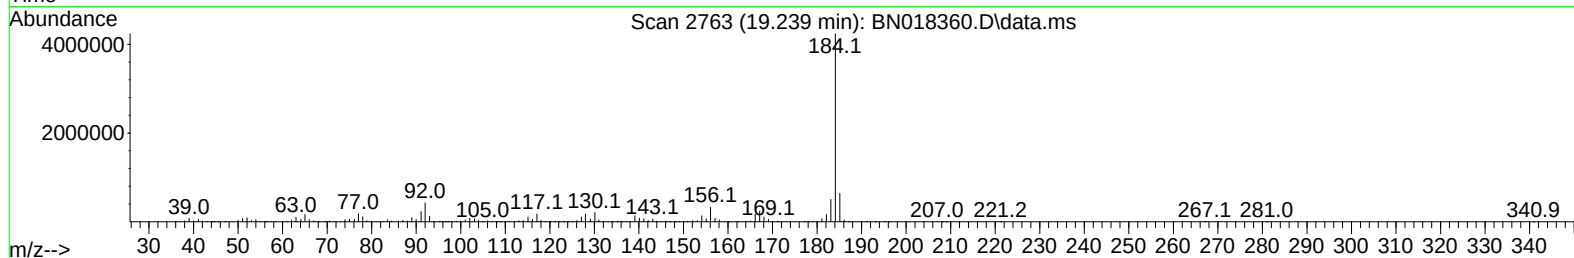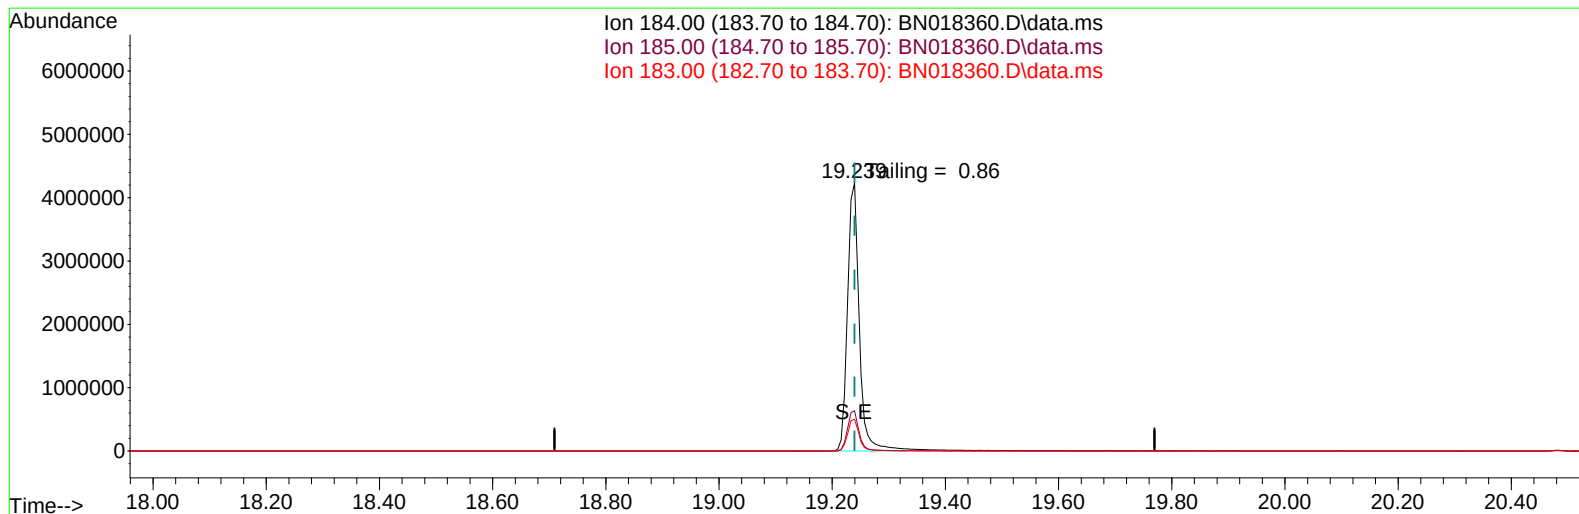

TIC: BN018360.D\data.ms

(77) Benzidine**19.239min (0.000) 11163.66 ng****response 6235873**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.03
183.00	13.20	11.82
0.00	0.00	0.00