
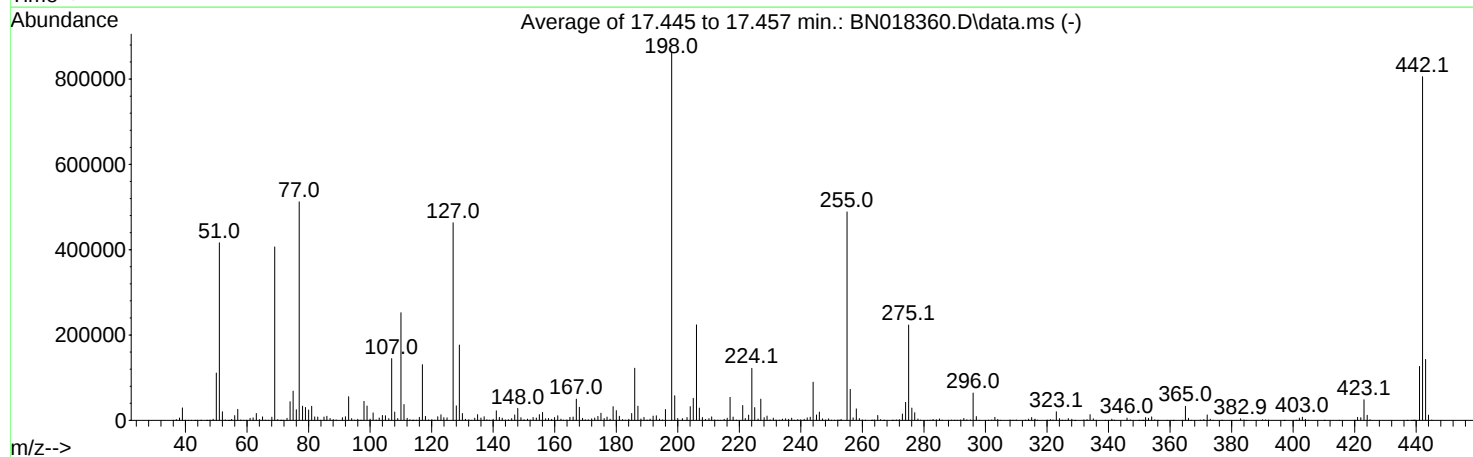


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010722\
 Data File : BN018360.D
 Acq On : 07 Jan 2022 09:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 07 14:23:23 2022

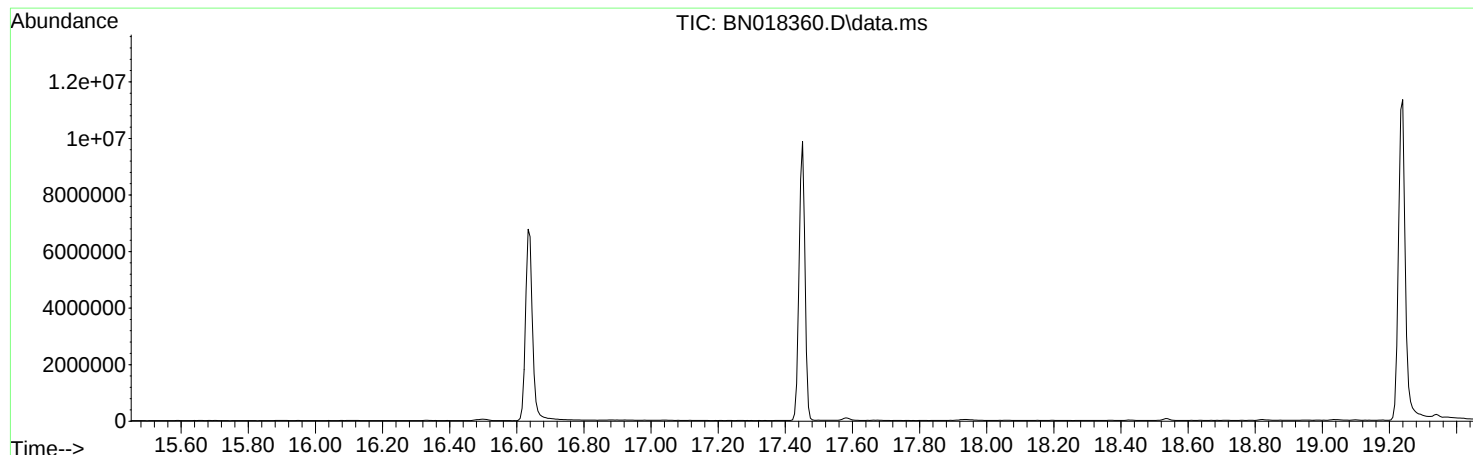

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	416497	PASS
68	69	0.00	2	1.9	7561	PASS
69	198	0.00	100	47.1	406496	PASS
70	69	0.00	2	0.5	2057	PASS
127	198	10	80	53.7	463317	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	862293	PASS
199	198	5	9	6.7	57621	PASS
275	198	10	60	25.9	223573	PASS
365	198	1	100	3.8	33101	PASS
441	198	0.01	100	14.6	126248	PASS
442	442	50	100	100.0	805653	PASS
443	442	15	24	17.8	143093	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/7/2022	BNA_N	<u>BN018360.D</u>
Compound Name	Response	Retention Time
DDT	2776987	20.48
DDD	21409	20.03
DDE	2065	19.53
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23474	2800461	0.84

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010722\
 Data File : BN018360.D
 Acq On : 07 Jan 2022 09:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jan 07 14:34:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 07 14:34:24 2022
 Response via : Initial Calibration

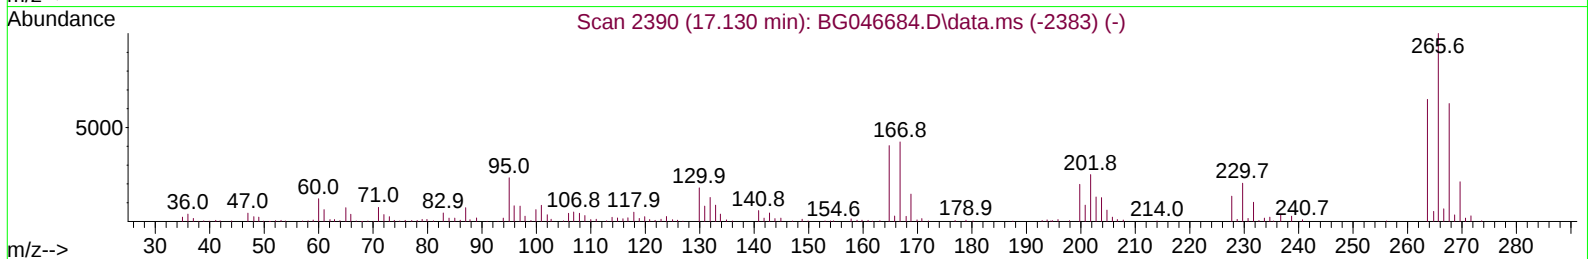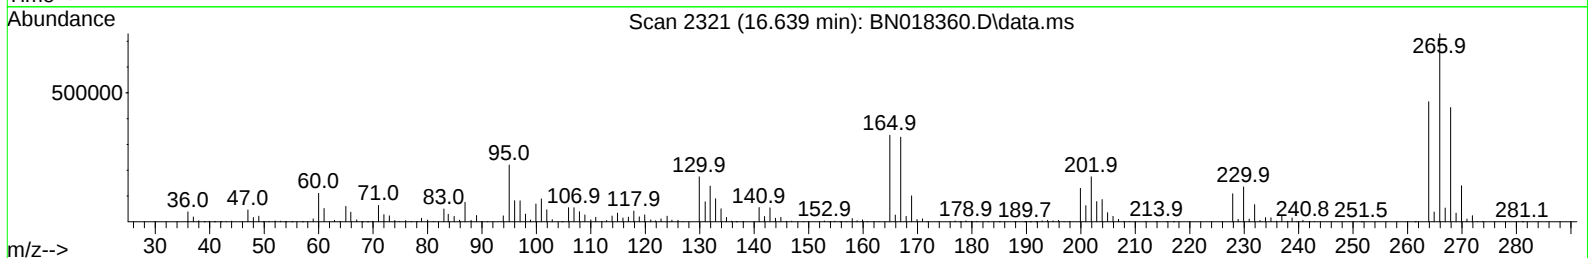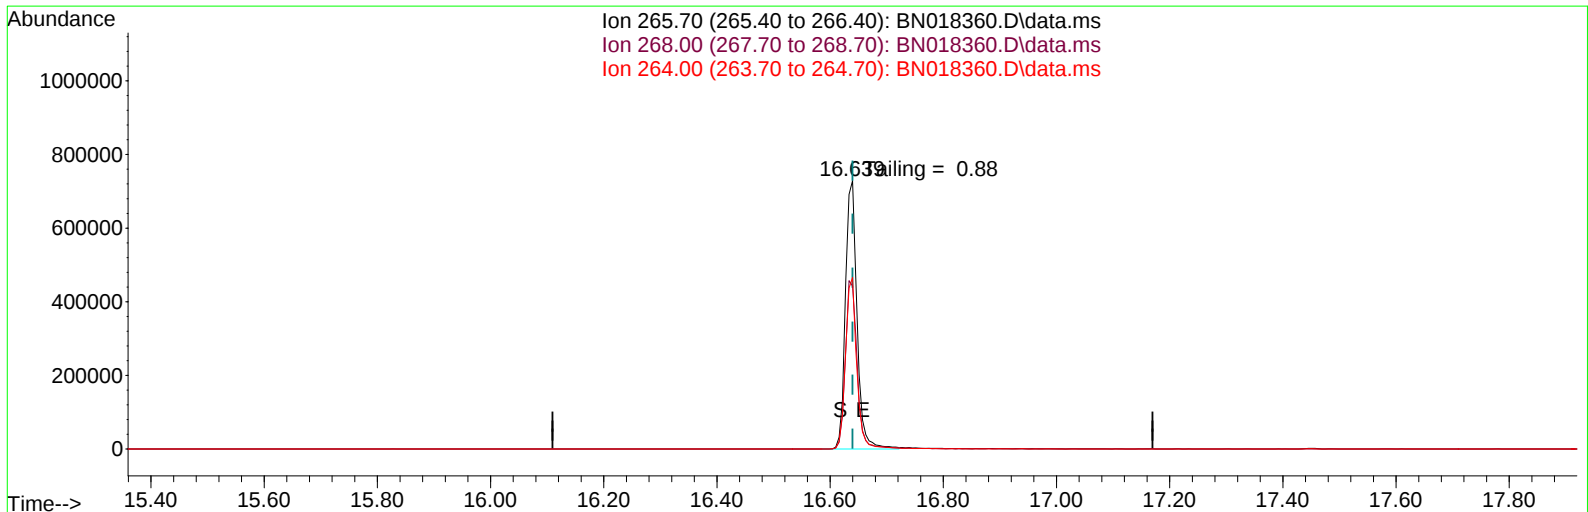

TIC: BN018360.D\data.ms

(70) Pentachlorophenol (C)

16.639min (0.000) 23583.89 ng




response 1045149

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.76
264.00	61.60	63.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010722\
Data File : BN018360.D
Acq On : 07 Jan 2022 09:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 07 14:34:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 07 14:34:24 2022
Response via : Initial Calibration

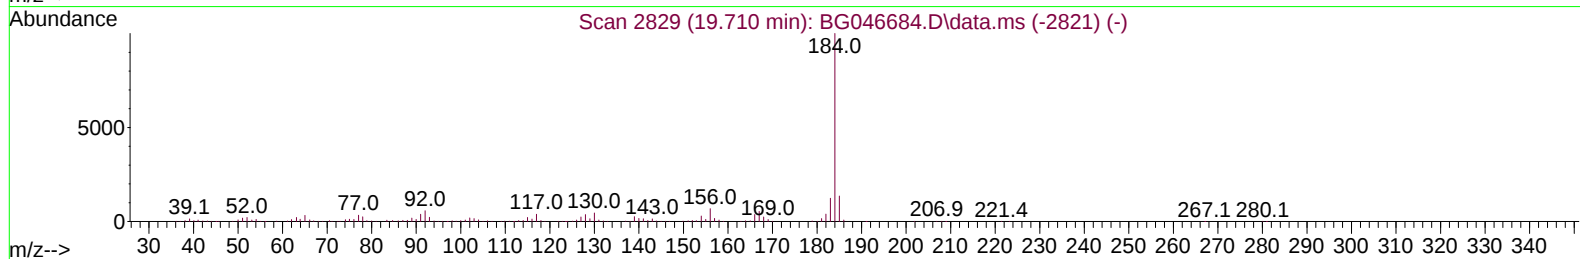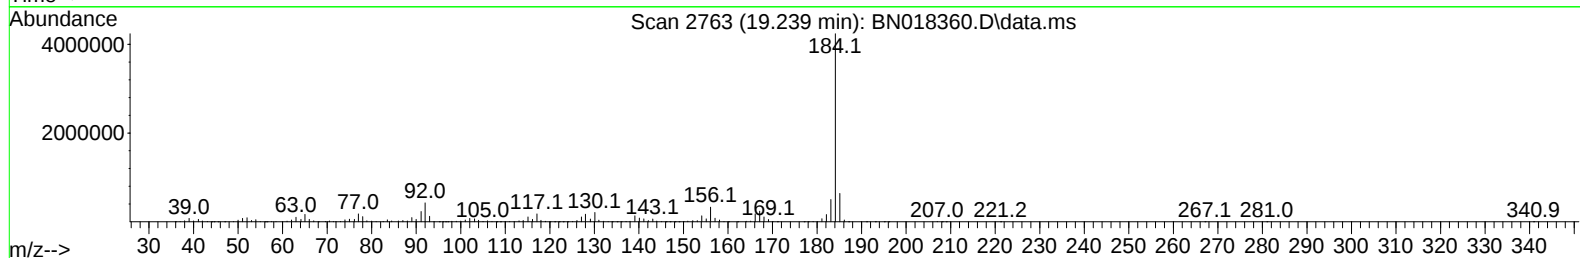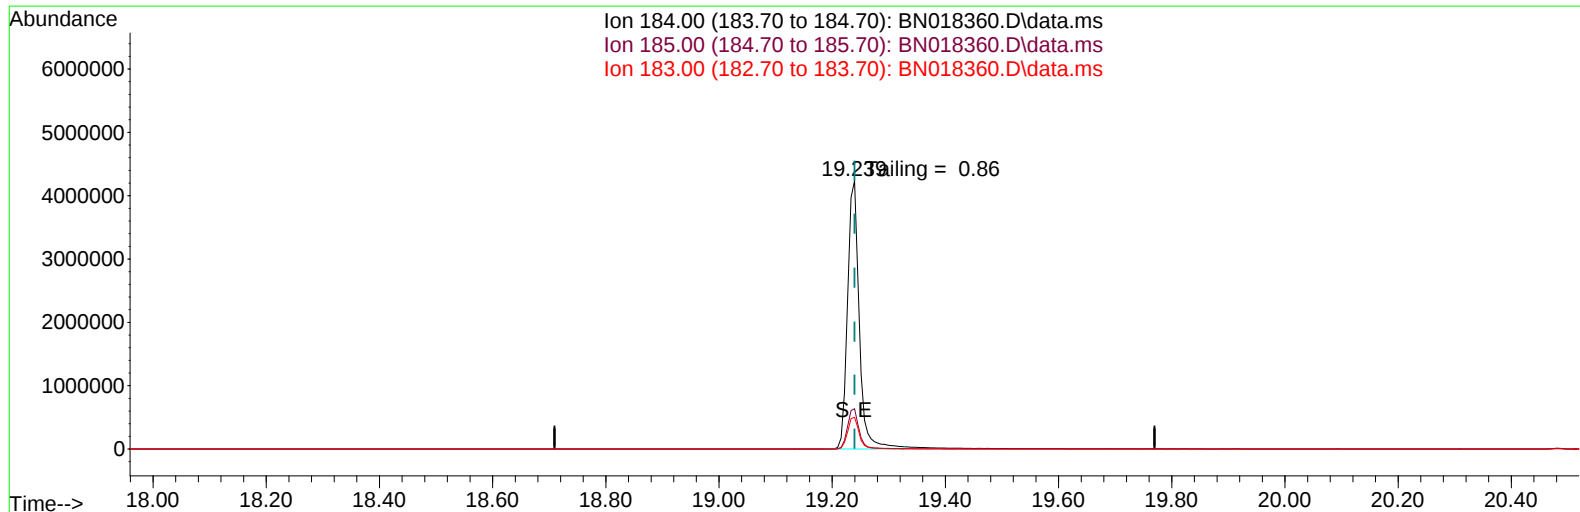

TIC: BN018360.D\data.ms

(77) Benzidine

19.239min (0.000) 11163.66 ng

response 6235873

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.03
183.00	13.20	11.82
0.00	0.00	0.00