
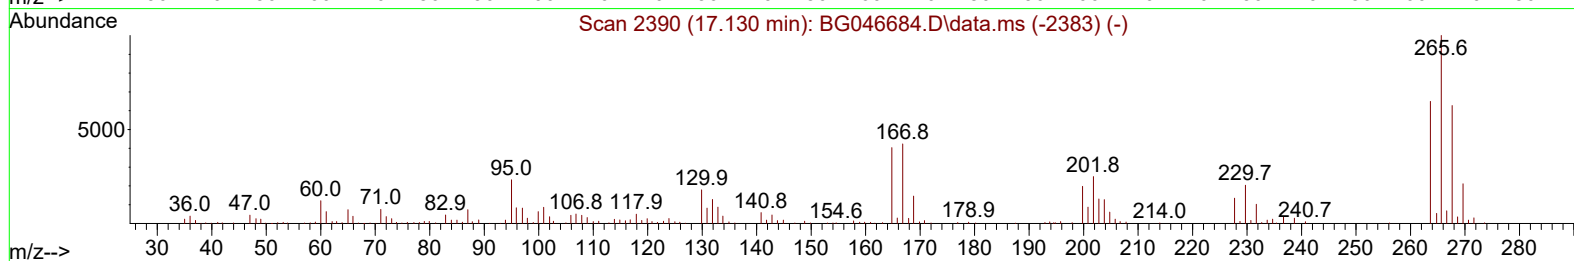
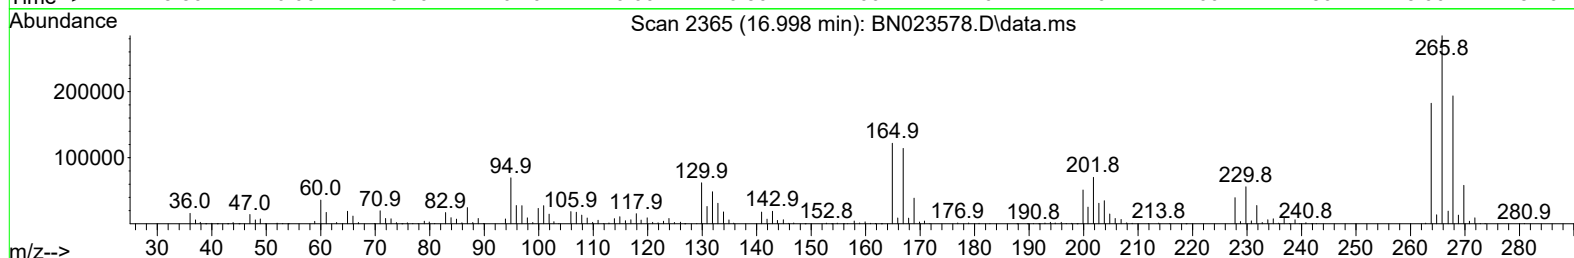


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010723\
 Data File : BN023578.D
 Acq On : 06 Jan 2023 16:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 05:32:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 07 05:32:52 2023
 Response via : Initial Calibration

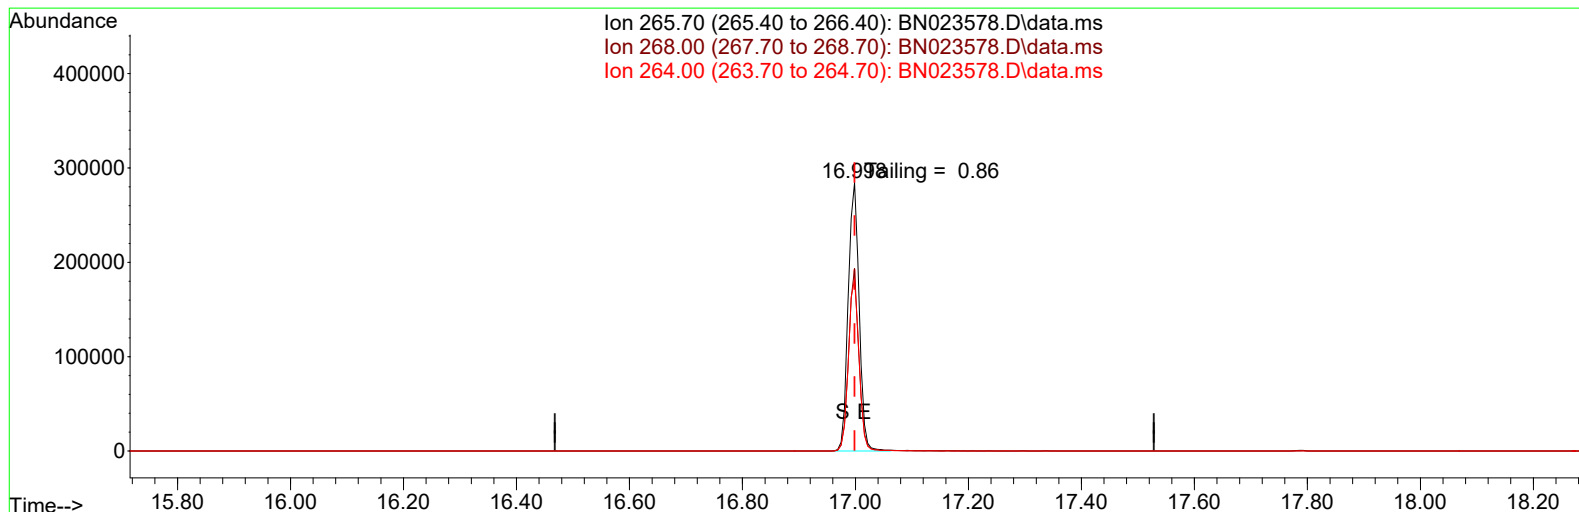

TIC: BN023578.D\data.ms

(70) Pentachlorophenol (C)




16.998min (0.000) 22660.24 ng

response 383939

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.99
264.00	61.60	64.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010723\
Data File : BN023578.D
Acq On : 06 Jan 2023 16:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 05:32:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 07 05:32:52 2023
Response via : Initial Calibration

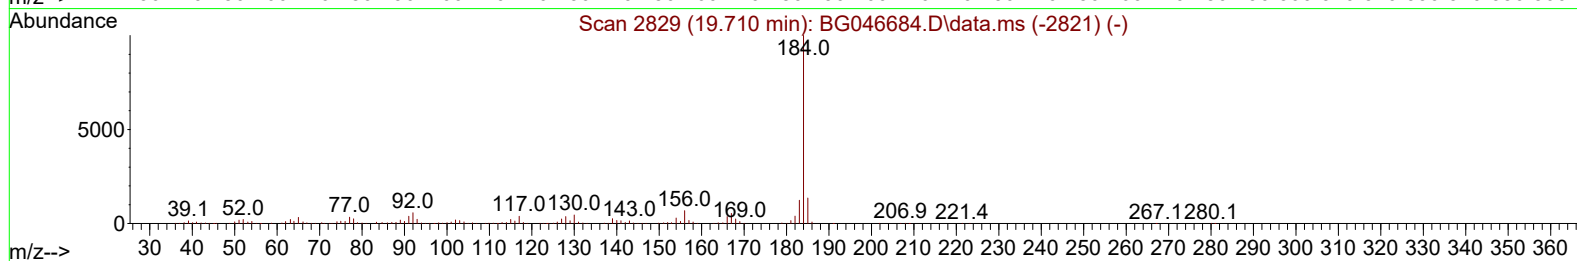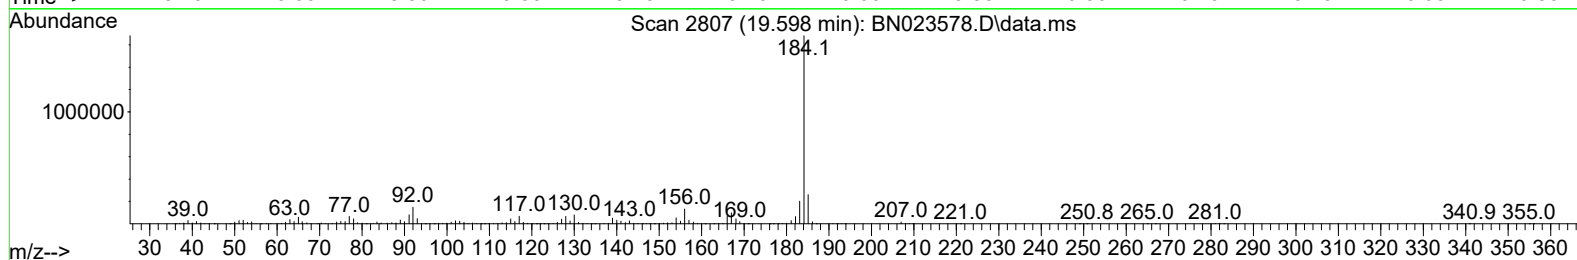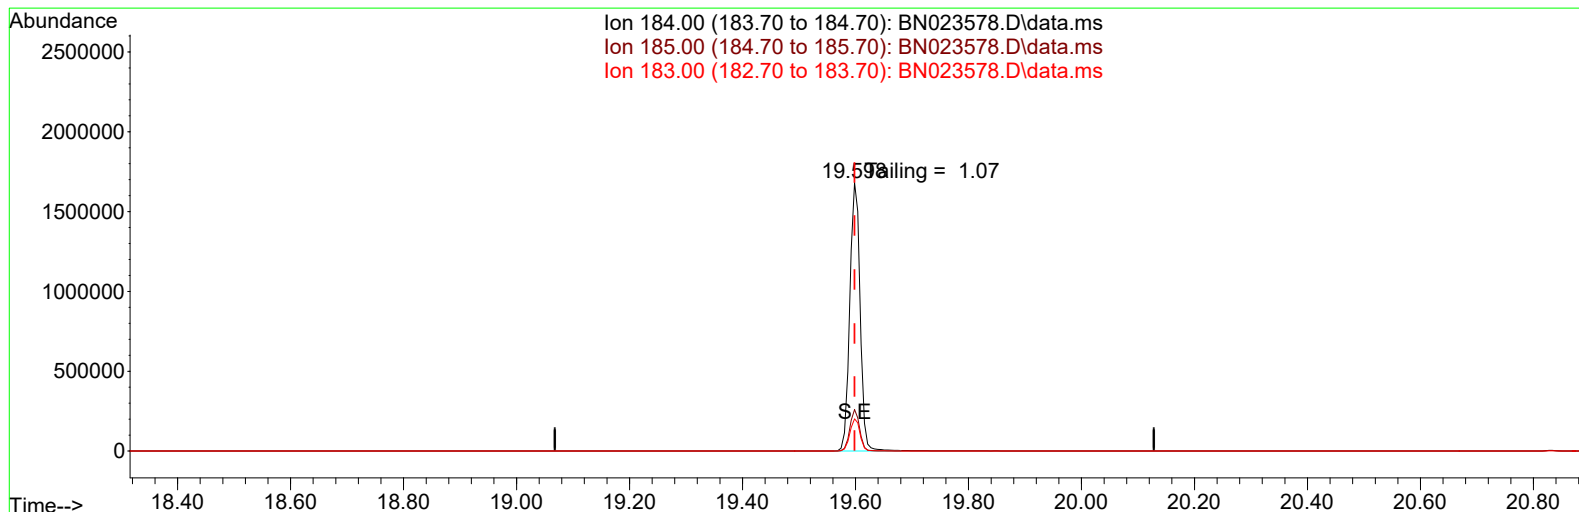

TIC: BN023578.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response 2146579

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.47
183.00	13.20	11.98
0.00	0.00	0.00