
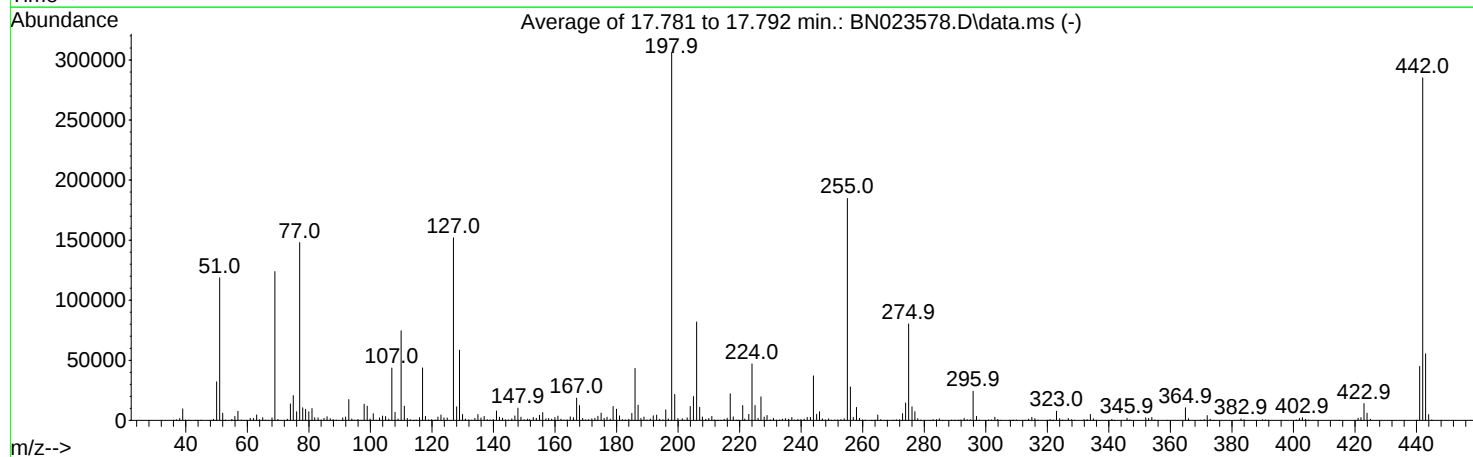


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010723\
 Data File : BN023578.D
 Acq On : 06 Jan 2023 16:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 07 02:04:12 2023

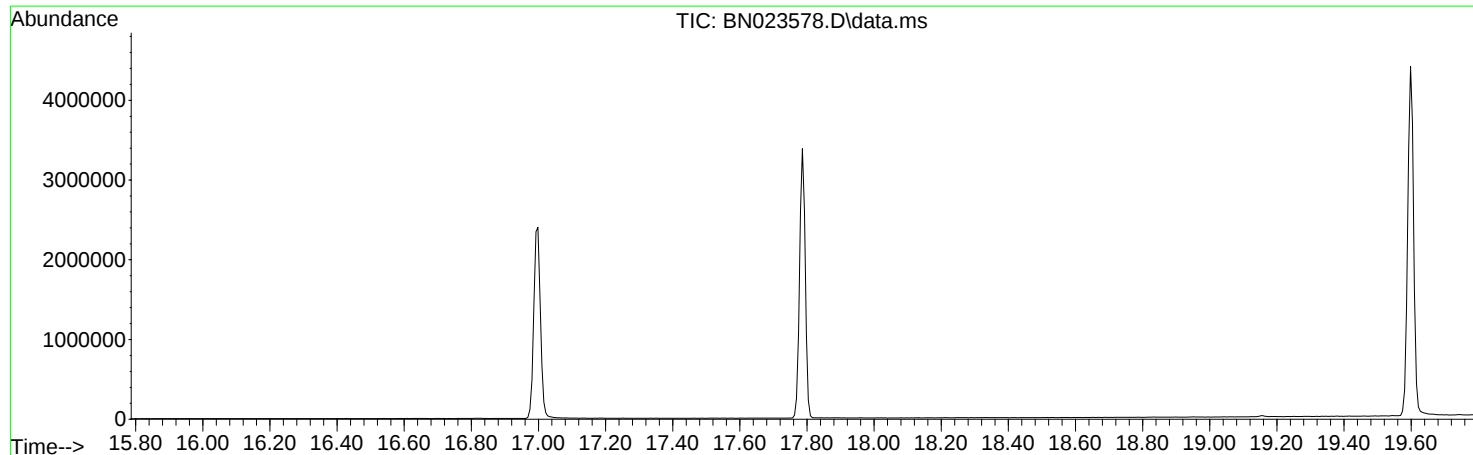




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	118635	PASS
68	69	0.00	2	1.7	2120	PASS
69	198	0.00	100	40.5	123923	PASS
70	69	0.00	2	0.6	792	PASS
127	198	10	80	49.6	151933	PASS
197	198	0.00	2	0.4	1171	PASS
198	198	100	100	100.0	306219	PASS
199	198	5	9	7.1	21589	PASS
275	198	10	60	26.2	80347	PASS
365	198	1	100	3.4	10476	PASS
441	198	0.01	100	14.6	44848	PASS
442	442	50	100	100.0	285120	PASS
443	442	15	24	19.5	55472	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010723\
 Data File : BN023578.D
 Acq On : 06 Jan 2023 16:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jan 07 05:32:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 07 05:32:52 2023
 Response via : Initial Calibration

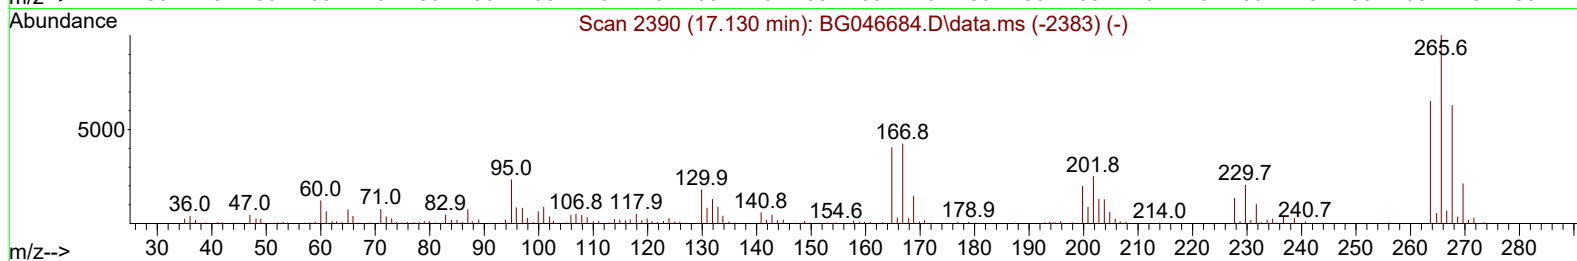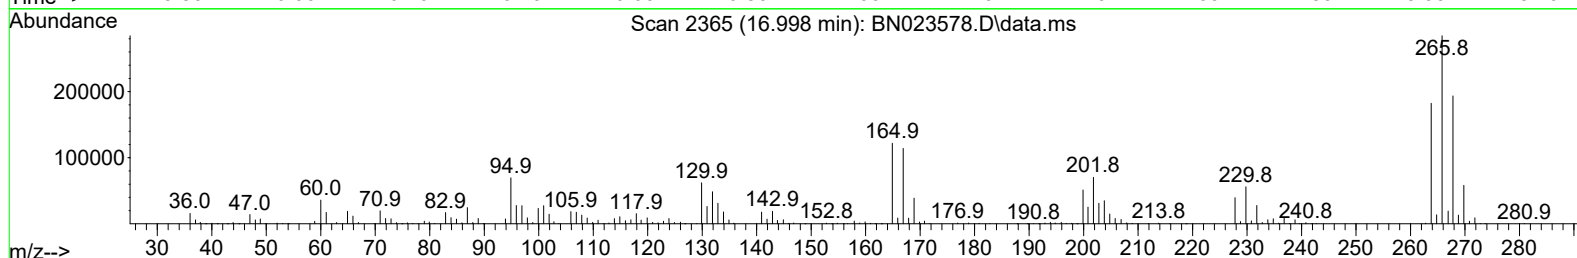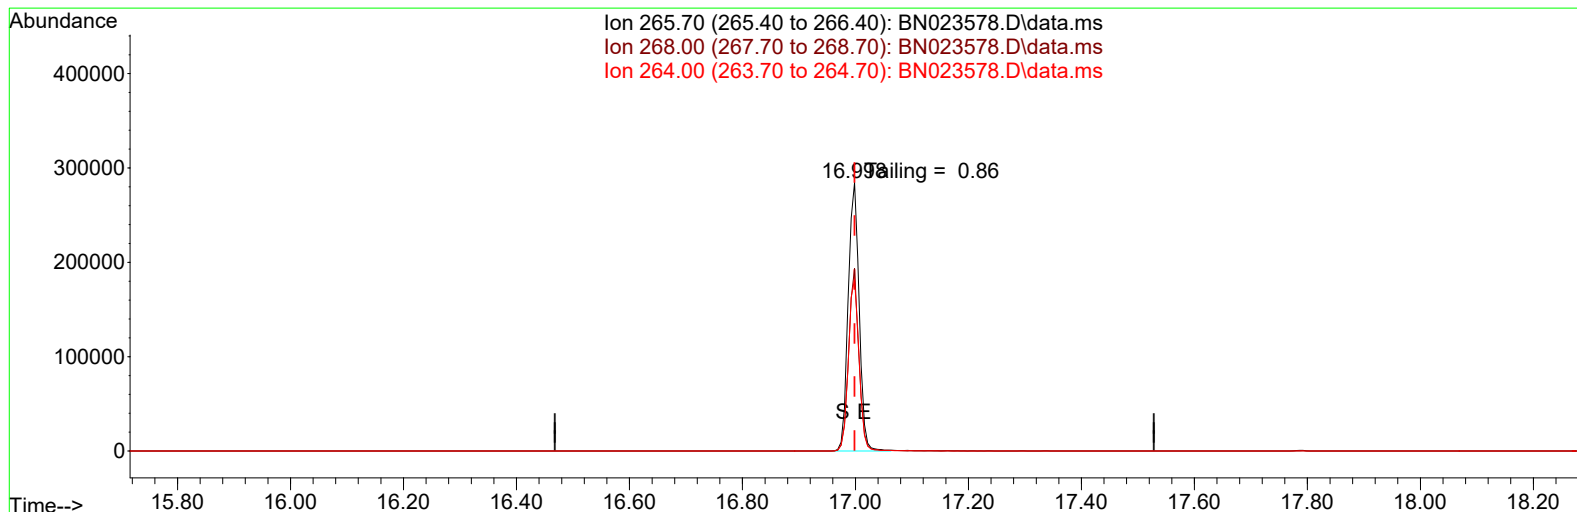

TIC: BN023578.D\data.ms

(70) Pentachlorophenol (C)

16.998min (0.000) 22660.24 ng




response 383939

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.99
264.00	61.60	64.07
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010723\  
Data File : BN023578.D  
Acq On    : 06 Jan 2023  16:50  
Operator   : CG/JU  
Sample     : DFTPP  
Misc       :  
ALS Vial   : 1    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 07 05:32:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 07 05:32:52 2023
Response via : Initial Calibration

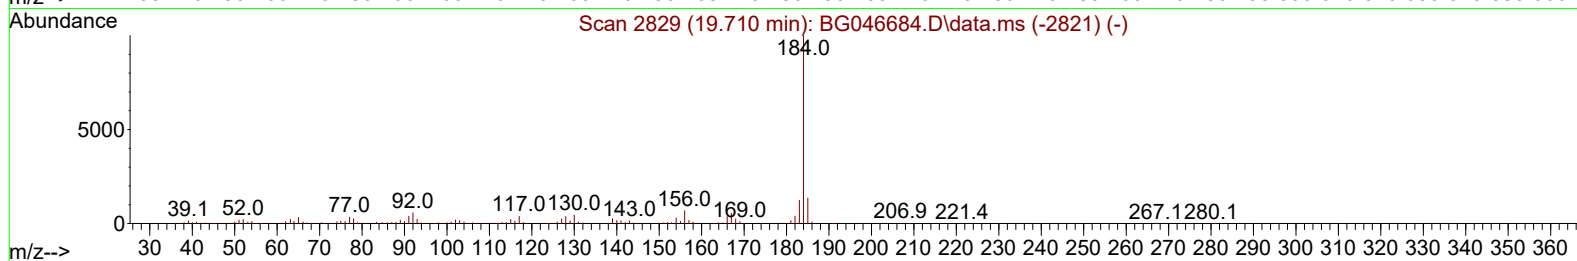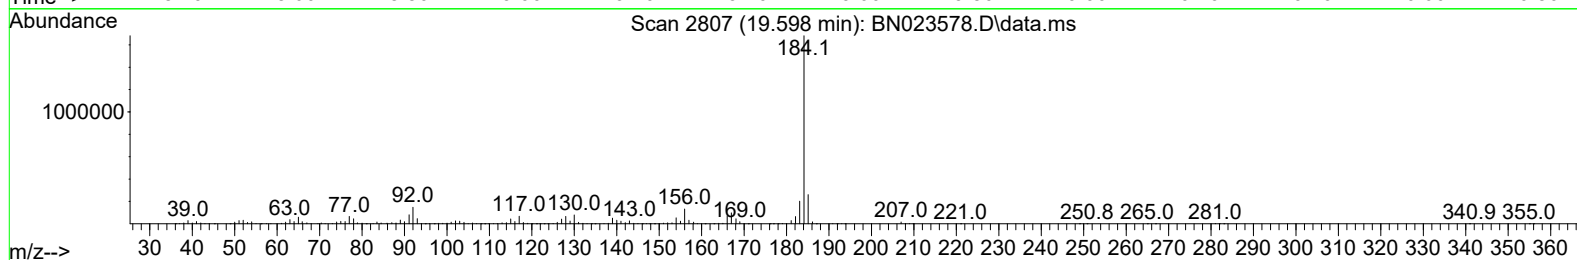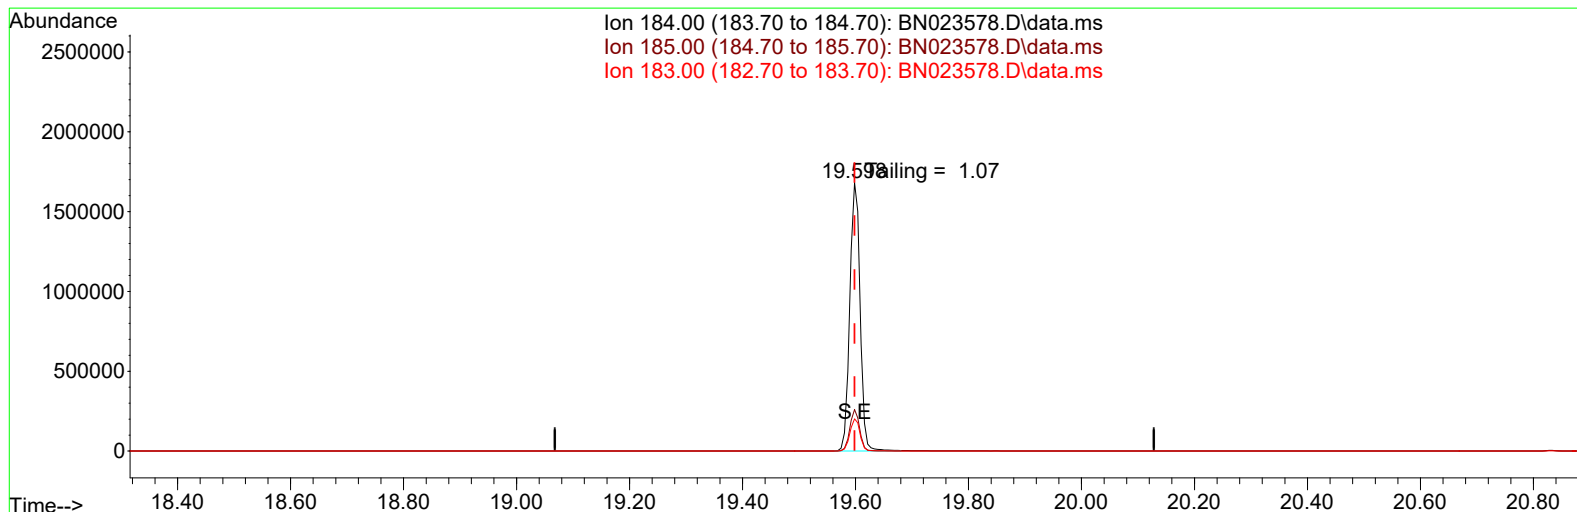

TIC: BN023578.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response **2146579**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.47
183.00	13.20	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/6/2023	BNA_N	<u>BN023578.D</u>
Compound Name	Response	Retention Time
DDT	1014659	20.833
DDD	29639	20.392
DDE	1441	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31080	1045739	2.97

Instrument :
BNA_N
ClientSampleId :
DFTPP