


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010924\
Data File : BN029223.D
Acq On : 09 Jan 2024 10:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 28 01:20:47 2023

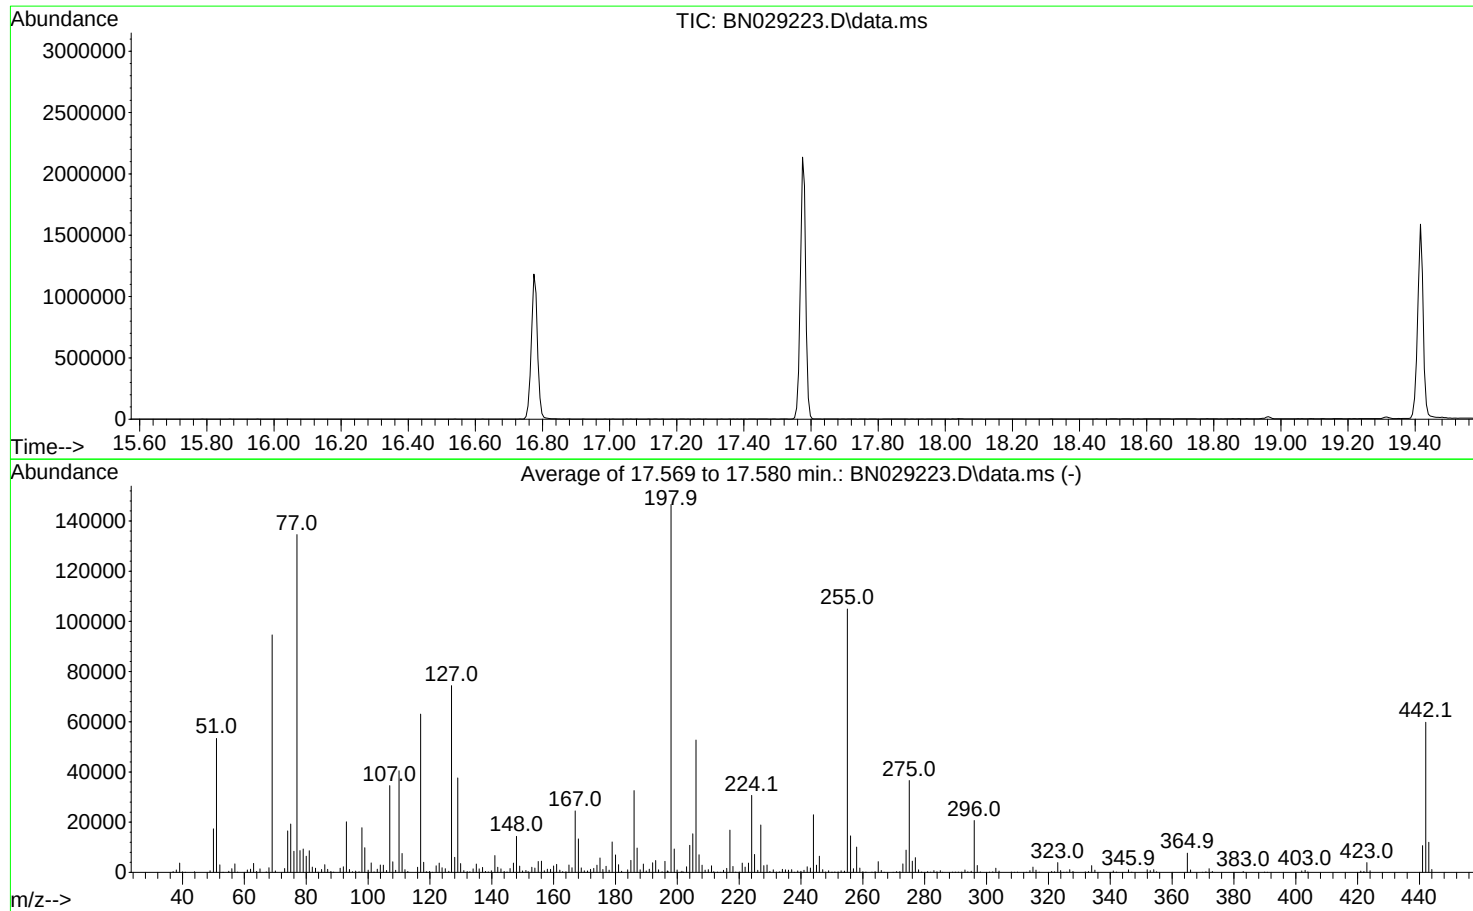




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	53389	PASS
68	69	0.00	2	2.0	1867	PASS
69	198	0.00	100	64.6	94616	PASS
70	69	0.00	2	0.6	545	PASS
127	198	10	80	50.8	74395	PASS
197	198	0.00	2	0.4	579	PASS
198	198	100	100	100.0	146571	PASS
199	198	5	9	6.3	9298	PASS
275	198	10	60	25.0	36592	PASS
365	198	1	100	5.2	7636	PASS
441	198	0.01	100	7.3	10679	PASS
442	442	50	100	100.0	59827	PASS
443	442	15	24	20.1	12014	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010924\
Data File : BN029223.D
Acq On : 09 Jan 2024 10:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 10 01:36:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

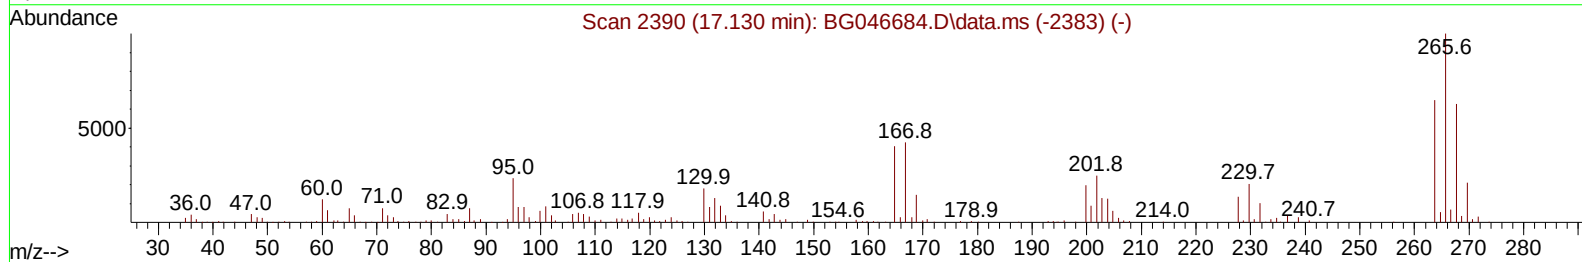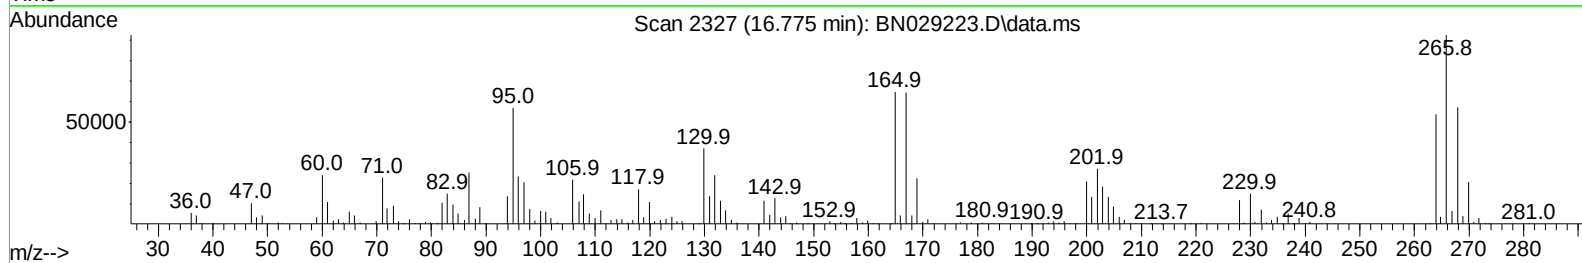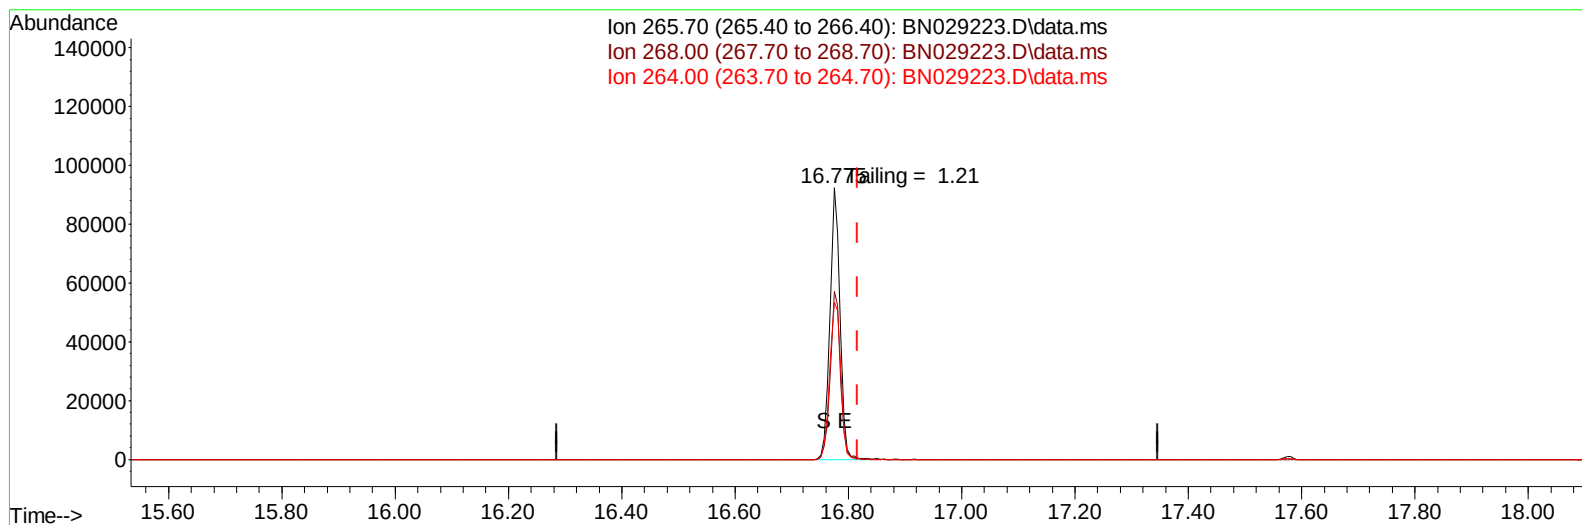

TIC: BN029223.D\data.ms

(70) Pentachlorophenol (C)

16.775min (-0.041) 12045.50 ng




response 113247

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.80
264.00	61.60	57.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010924\
Data File : BN029223.D
Acq On : 09 Jan 2024 10:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 10 01:36:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

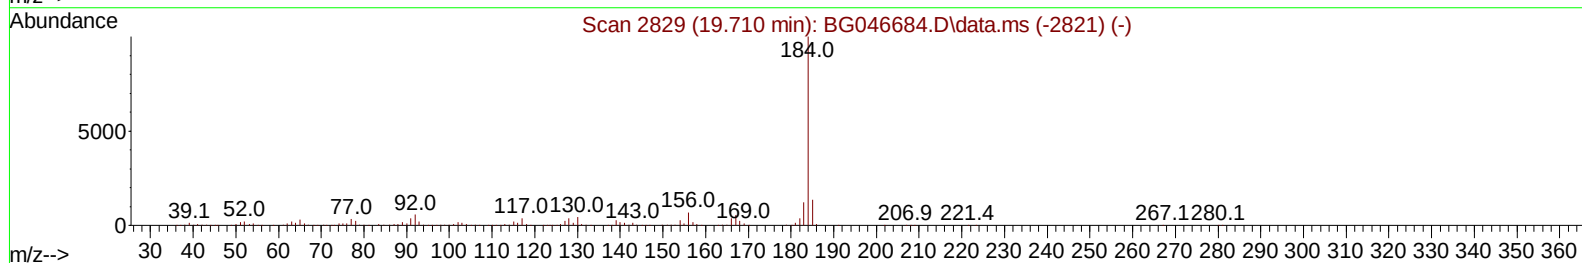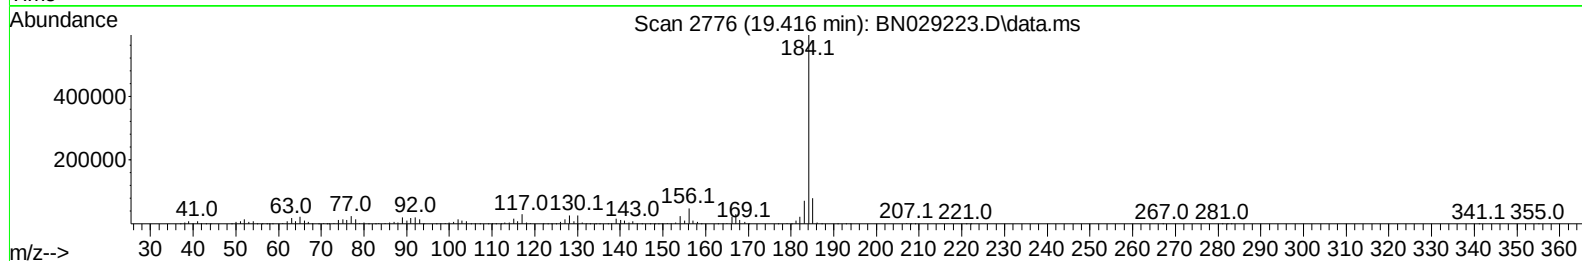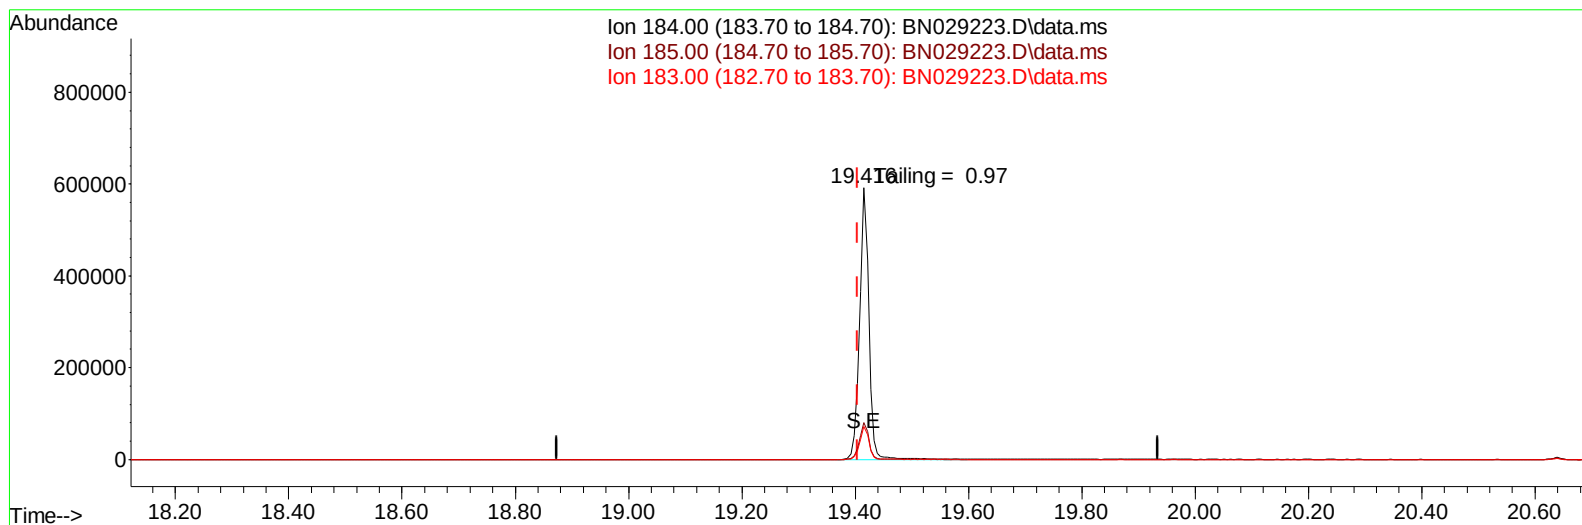

TIC: BN029223.D\data.ms

(77) Benzidine

19.416min (+ 0.012) 0.00 ng

response 661572

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.64
183.00	13.20	12.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/9/2024	BNA_N	<u>BN029223.D</u>
Compound Name	Response	Retention Time
DDT	372727	20.639
DDD	8726	20.192
DDE	755	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9481	382208	2.48

Instrument :
BNA_N
ClientSampleId :
DFTPP