


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN011020\
Data File : BN009340.D
Acq On : 10 Jan 2020 18:28
Operator : JU
Sample : PB125830BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 10 23:12:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 16:45:39 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK30

Manual Integrations
APPROVED

mohammad
1/13/2020 2:22:09 PM

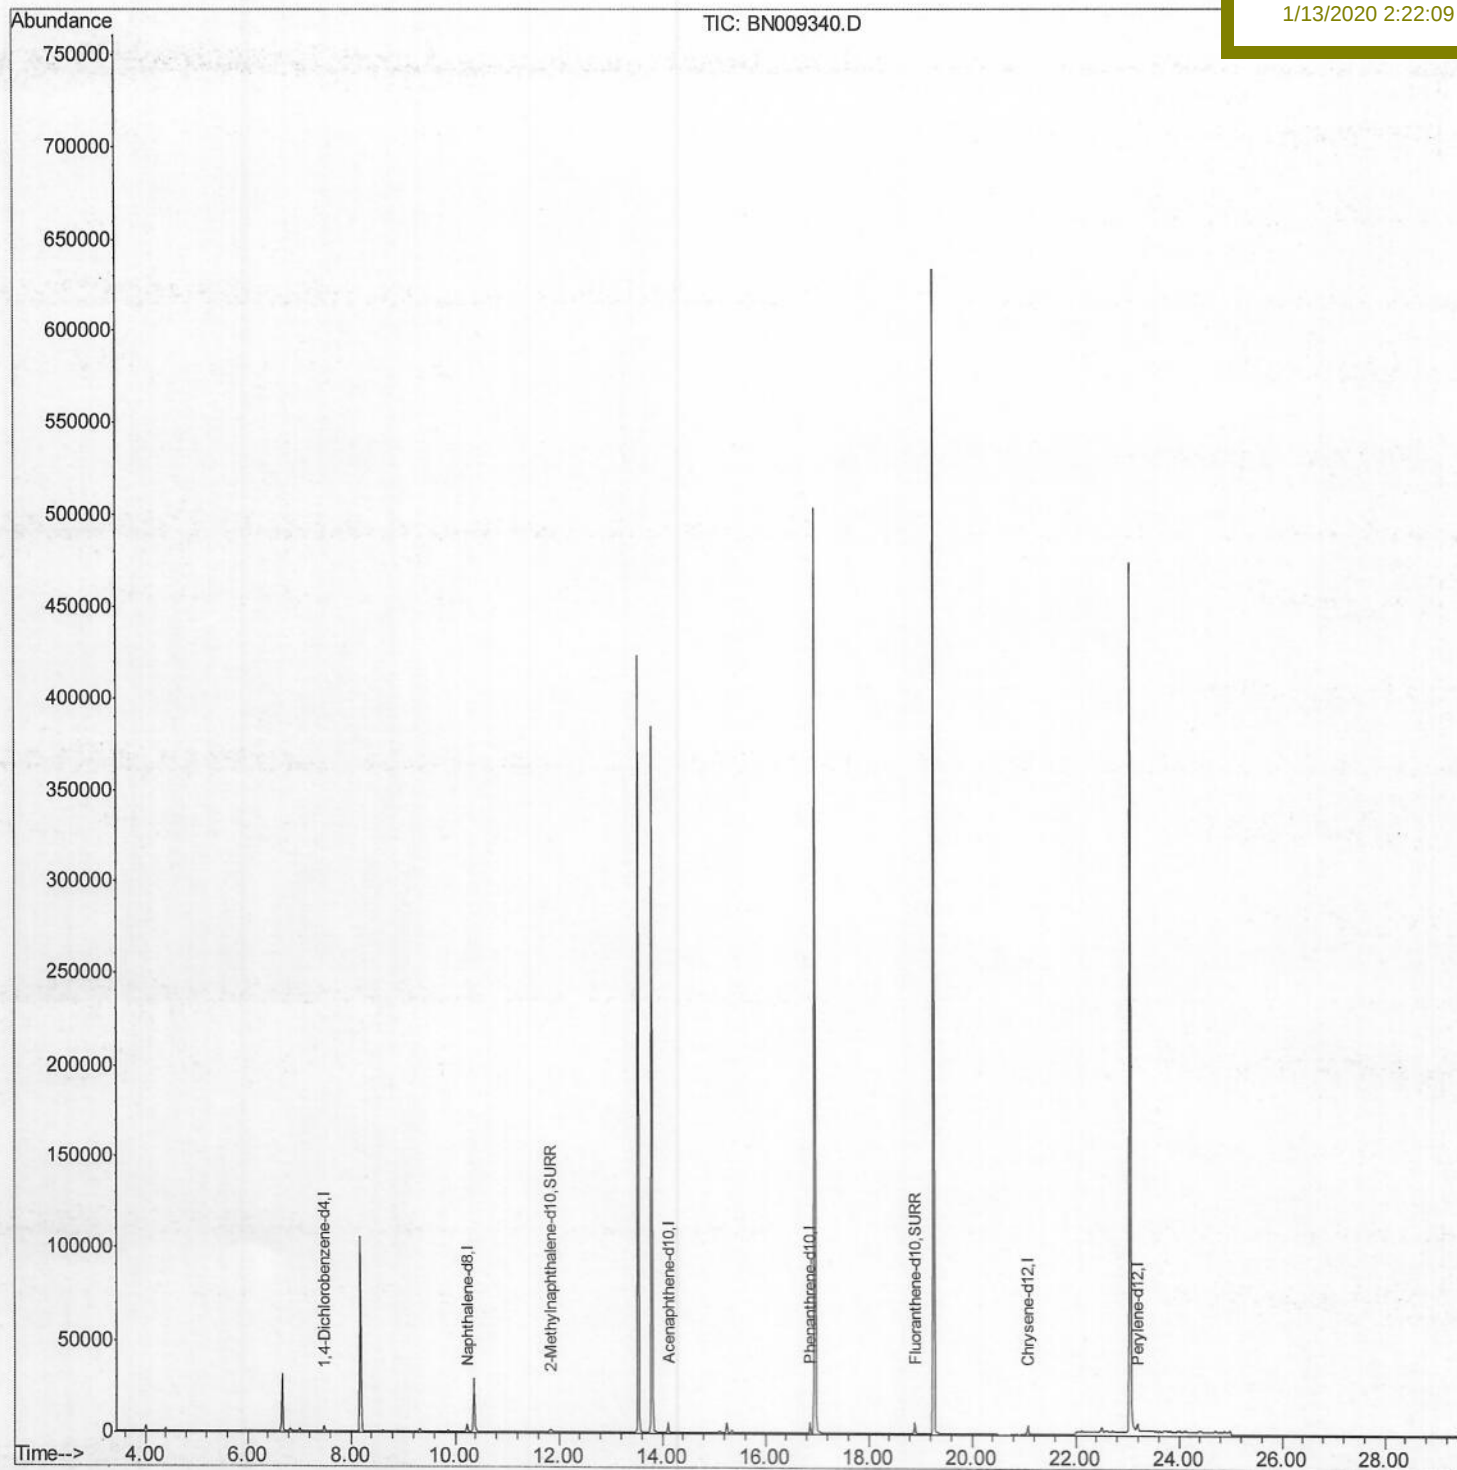

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN011020\

Data File : BN009340.D

Acq On : 10 Jan 2020 18:28

Operator : JU

Sample : PB125830BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 10 23:08:11 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Jan 10 16:45:39 2020

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




SBLK30

Manual Integrations

APPROVED

mohammad

1/13/2020 2:22:09 PM

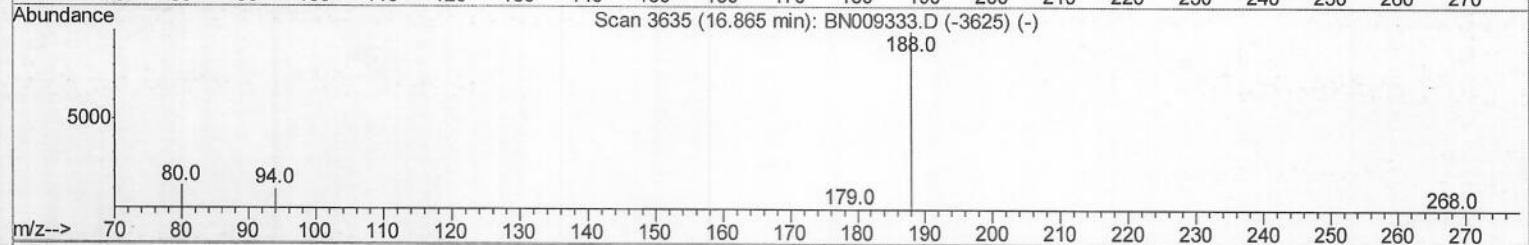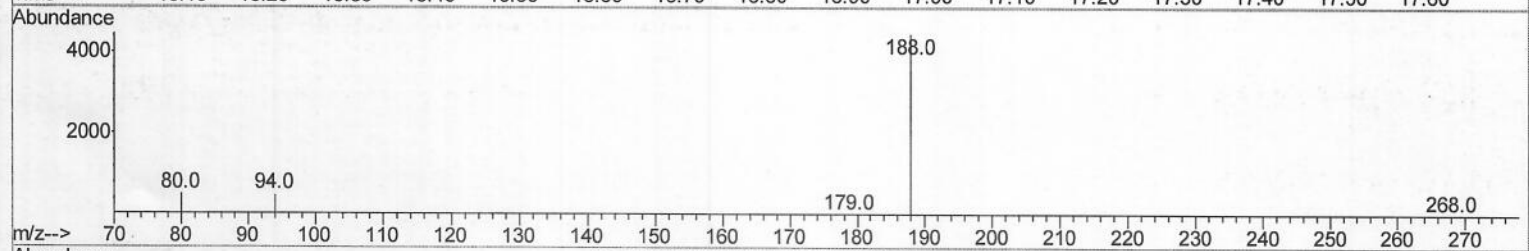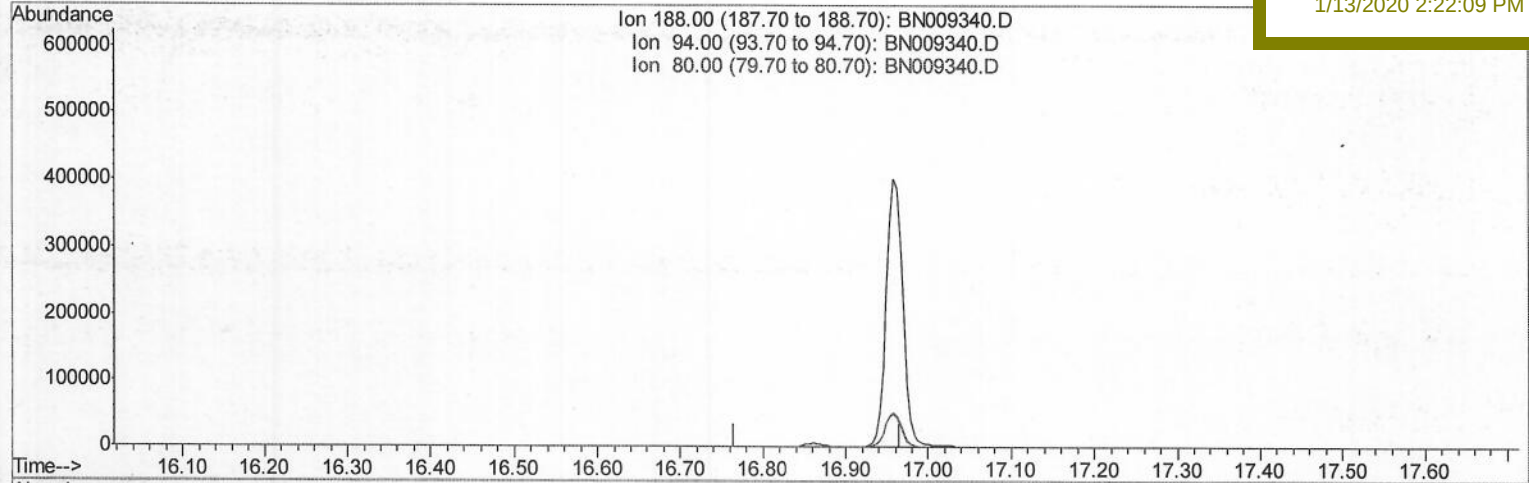

TIC: BN009340.D

(10) Phenanthrene-d10 (I)

16.865min (-16.865) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.70	0.00#
80.00	13.40	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN011020\

Data File : BN009340.D

Acq On : 10 Jan 2020 18:28

Operator : JU

Sample : PB125830BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 10 23:08:11 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Jan 10 16:45:39 2020

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




SBLK30

Manual Integrations

APPROVED

mohammad

1/13/2020 2:22:09 PM

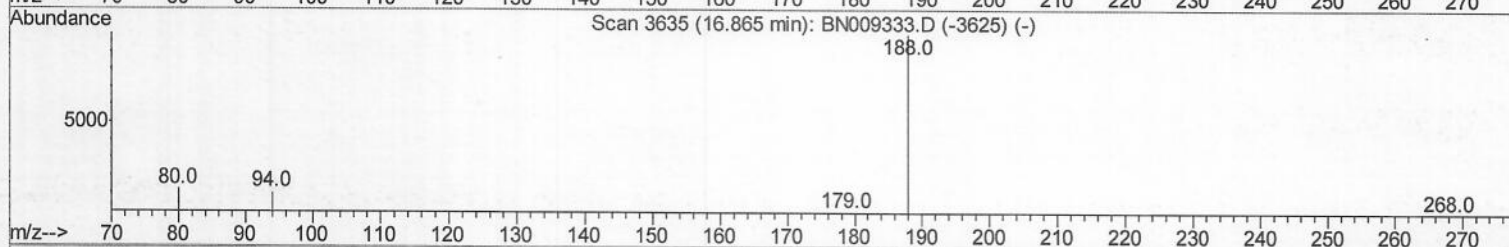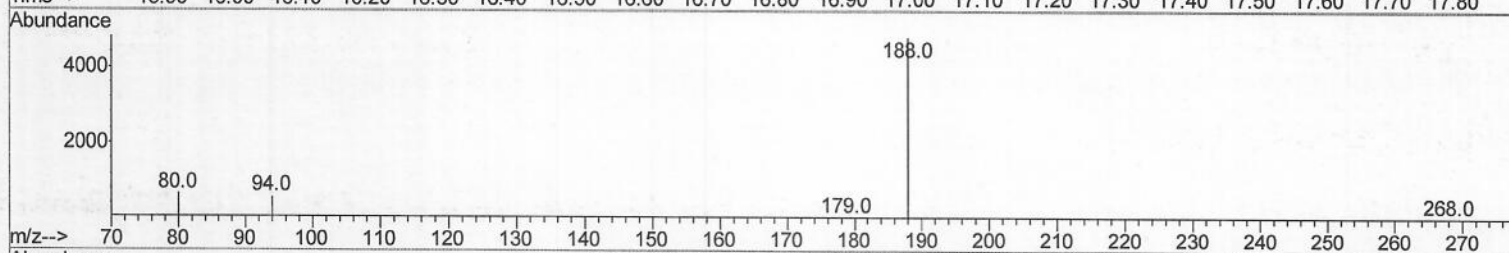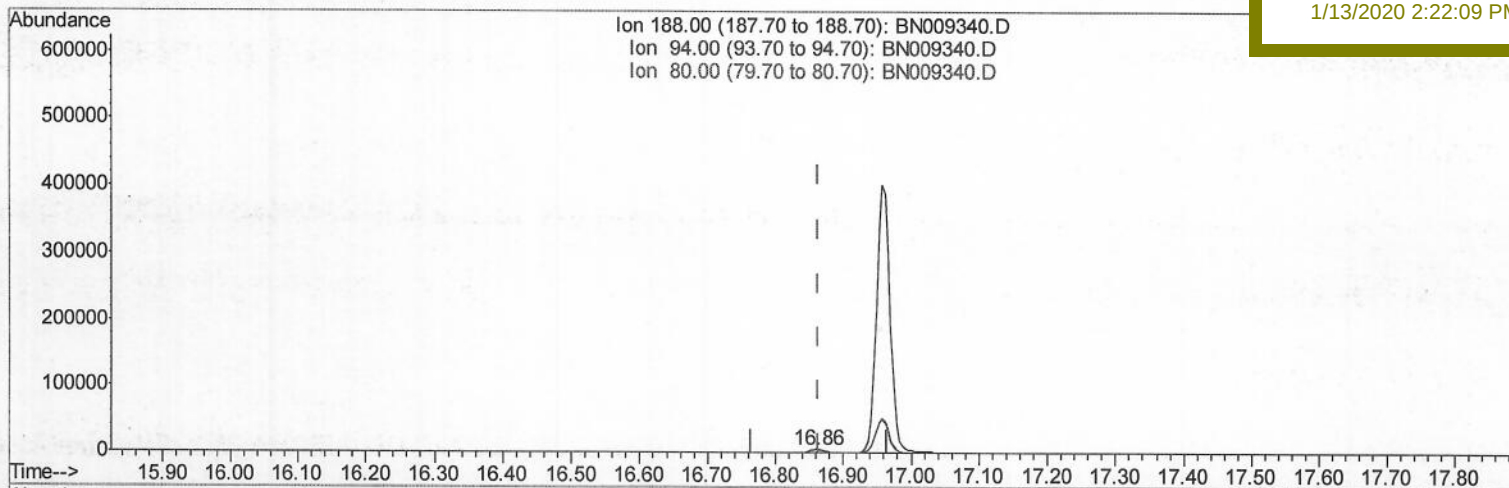

TIC: BN009340.D

(10) Phenanthrene-d10 (I)

16.861min (-0.004) 0.40ng/ul m

JU01/13/20

response 6539

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	11.80
80.00	13.40	13.80
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN011020\
Data File : BN009340.D
Acq On : 10 Jan 2020 18:28
Operator : JU
Sample : PB125830BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 10 23:12:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 16:45:39 2020
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
SBLK30

Manual Integrations
APPROVED

mohammad
1/13/2020 2:22:09 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	1424	0.40	ng/ul	0.00
2) Naphthalene-d8	10.23	136	5102	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.11	164	3088	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.86	188	6539m	0.40	ng/ul	0.00
16) Chrysene-d12	21.08	240	5040	0.40	ng/ul	0.00
20) Perylene-d12	23.19	264	5770	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.84	152	2840	0.34	ng/ul	0.00
14) Fluoranthene-d10	18.90	212	6763	0.34	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 01/13/20