

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN011020\

Data File : BN009341.D

Acq On : 10 Jan 2020 19:03

Operator : JU

Sample : PB125832BL

Misc :

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jan 10 23:14:30 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Jan 10 16:45:39 2020

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :


SBLK32

Manual Integrations

APPROVED

mohammad

1/13/2020 2:22:12 PM

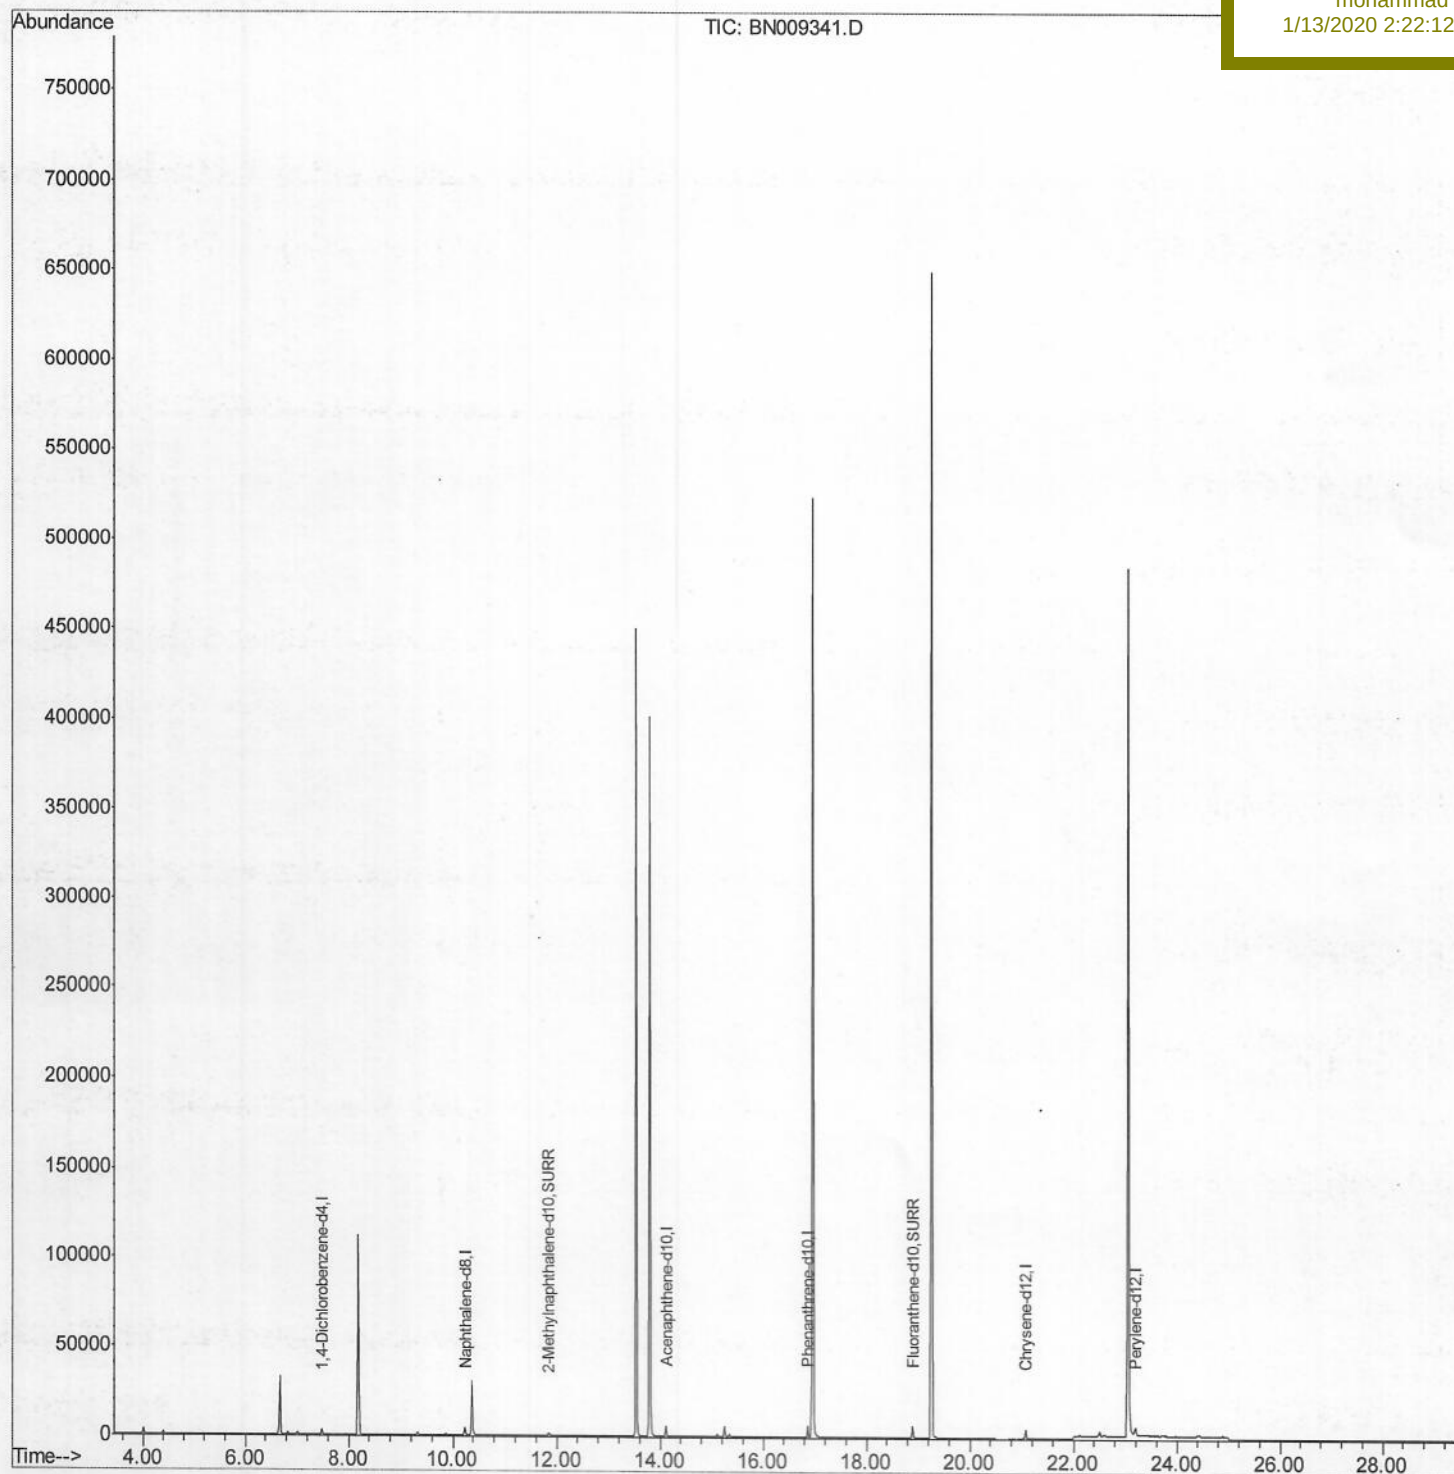

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN011020\

Data File : BN009341.D

Acq On : 10 Jan 2020 19:03

Operator : JU

Sample : PB125832BL

Misc :

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jan 10 23:08:17 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Jan 10 16:45:39 2020

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




SBLK32

Manual Integrations

APPROVED

mohammad

1/13/2020 2:22:12 PM

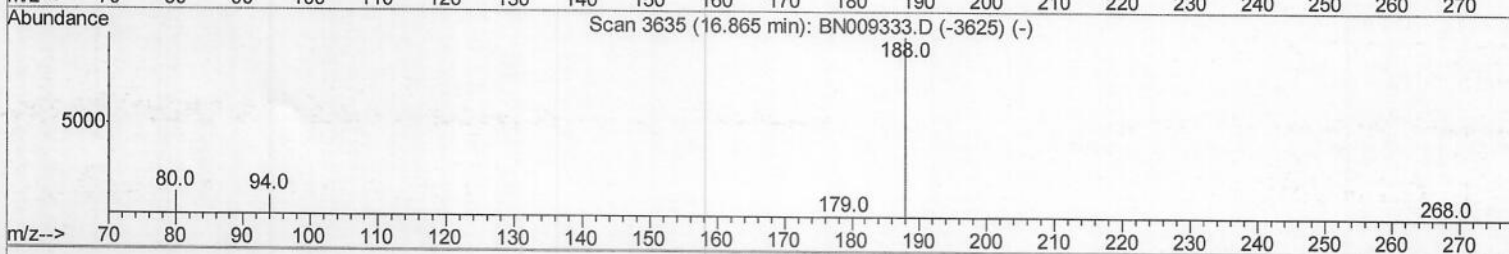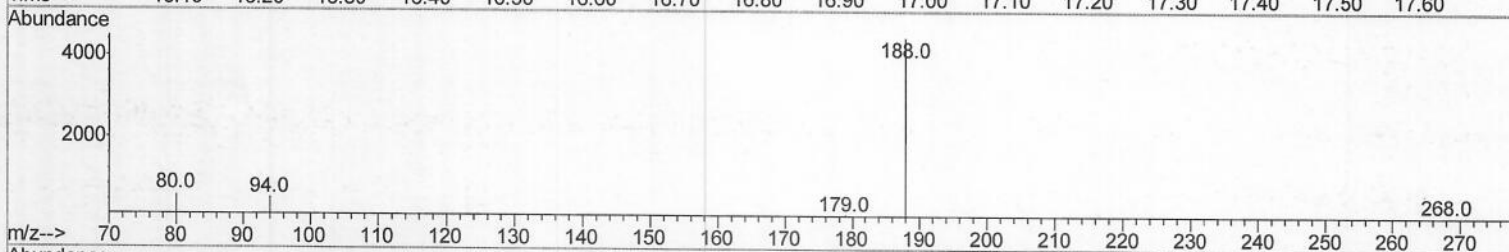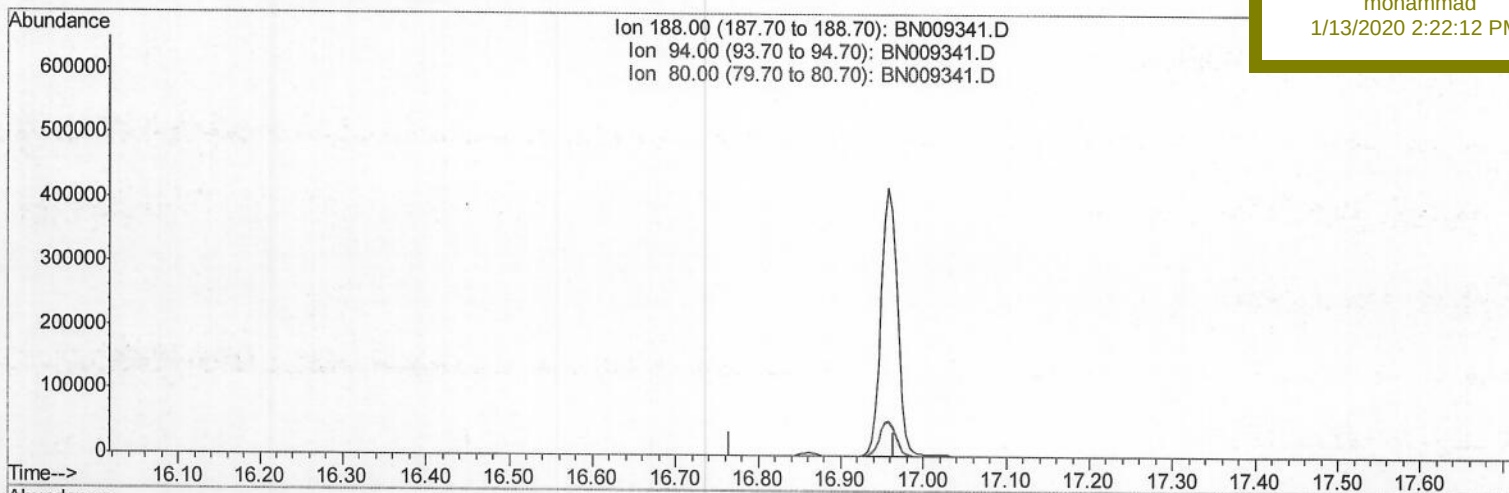

TIC: BN009341.D

(10) Phenanthrene-d10 (I)

16.865min (-16.865) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.70	0.00#
80.00	13.40	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN011020\
Data File : BN009341.D
Acq On : 10 Jan 2020 19:03
Operator : JU
Sample : PB125832BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jan 10 23:14:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 16:45:39 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK32

Manual Integrations
APPROVED

mohammad
1/13/2020 2:22:12 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	1468	0.40	ng/ul	0.00
2) Naphthalene-d8	10.23	136	5386	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.11	164	3208	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.86	188	6698m	0.40	ng/ul	0.00
16) Chrysene-d12	21.07	240	5230	0.40	ng/ul	0.00
20) Perylene-d12	23.19	264	5875	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.84	152	3020	0.34	ng/ul	0.00
14) Fluoranthene-d10	18.90	212	7011	0.34	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 01/13/20

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN011020\

Data File : BN009341.D

Acq On : 10 Jan 2020 19:03

Operator : JU

Sample : PB125832BL

Misc :

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jan 10 23:08:17 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Jan 10 16:45:39 2020

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




SBLK32

Manual Integrations

APPROVED

mohammad

1/13/2020 2:22:12 PM

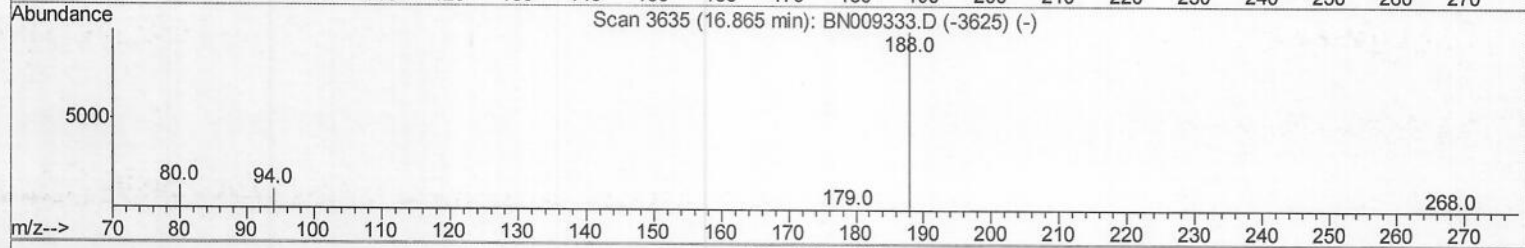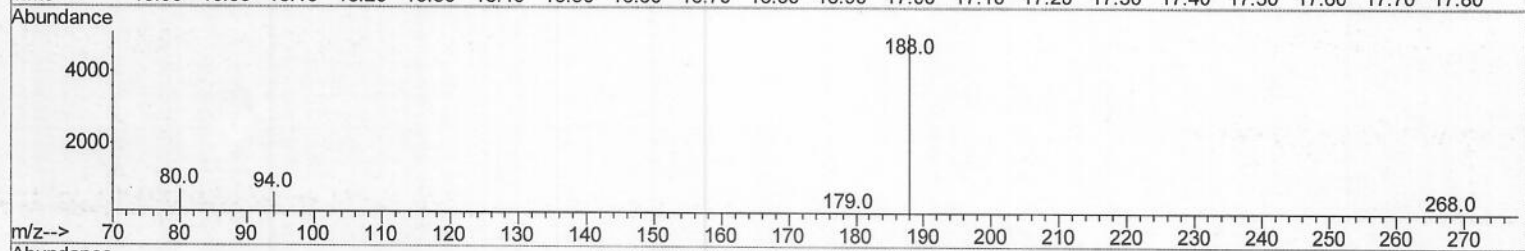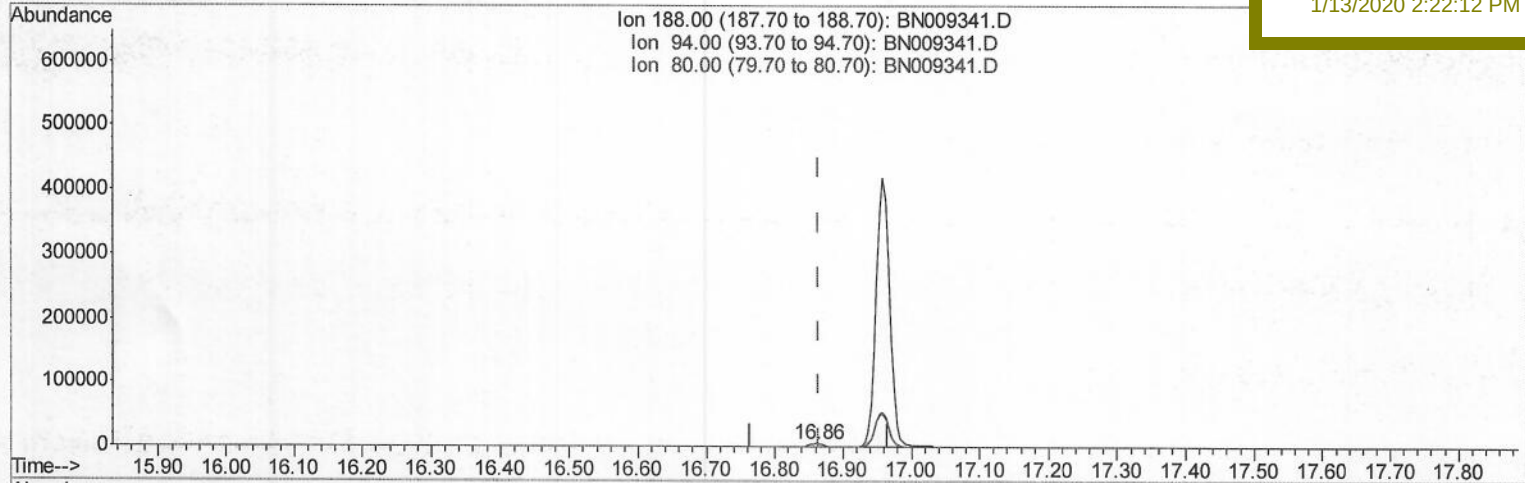

TIC: BN009341.D

(10) Phenanthrene-d10 (I)

16.861min (-0.004) 0.40ng/ul m JU 01/13/20

response 6698

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	11.44
80.00	13.40	13.29
0.00	0.00	0.00