


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011223\
Data File : BN023615.D
Acq On : 11 Jan 2023 17:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 12 00:22:07 2023

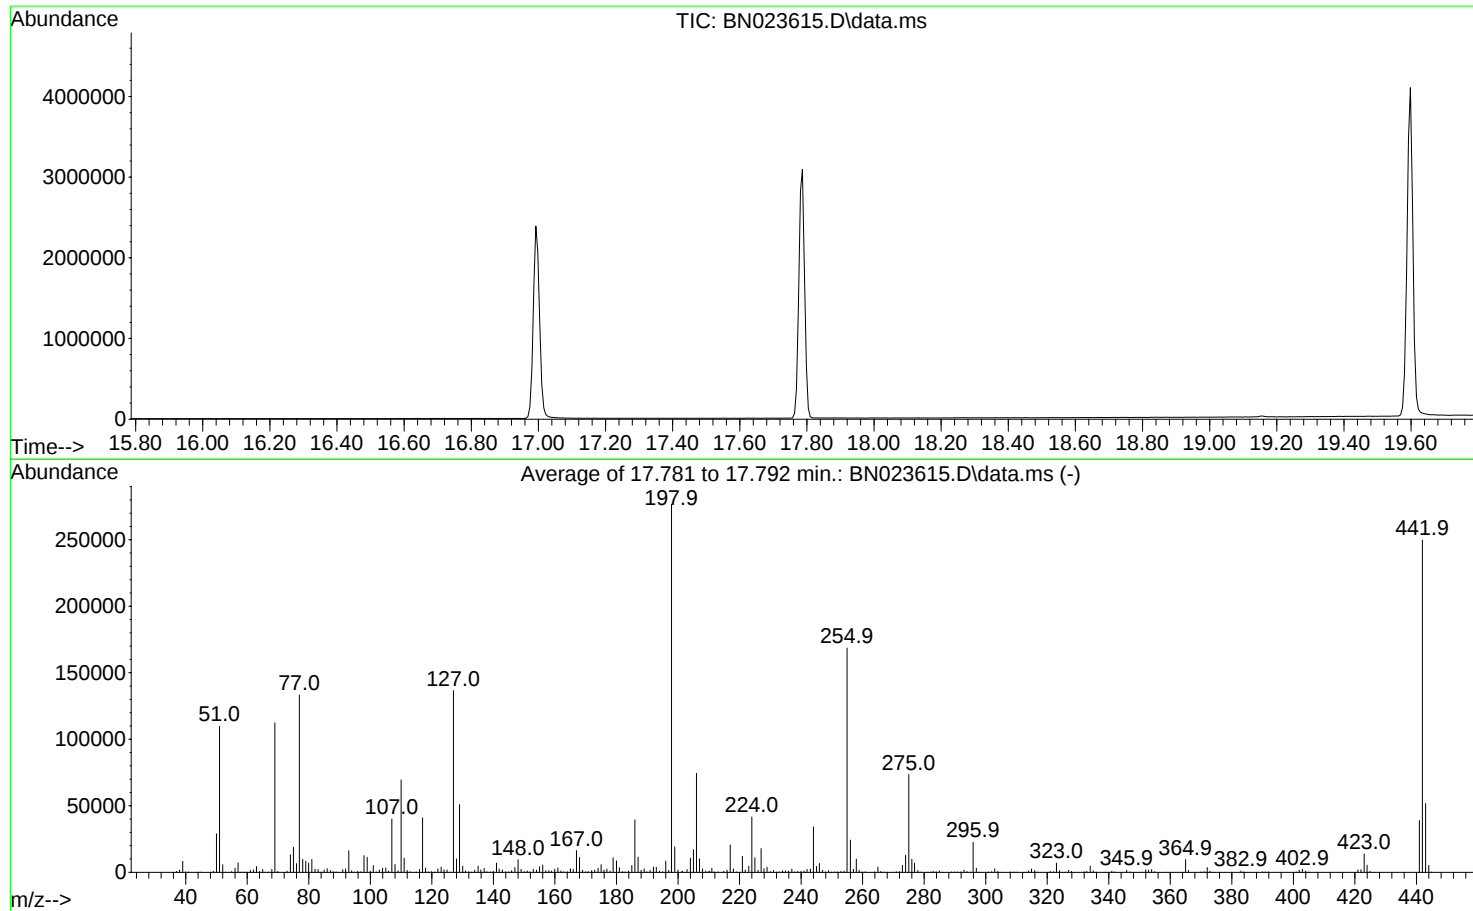




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	109752	PASS
68	69	0.00	2	2.0	2233	PASS
69	198	0.00	100	40.6	112272	PASS
70	69	0.00	2	0.6	670	PASS
127	198	10	80	49.4	136568	PASS
197	198	0.00	2	0.6	1535	PASS
198	198	100	100	100.0	276544	PASS
199	198	5	9	6.9	19045	PASS
275	198	10	60	26.5	73416	PASS
365	198	1	100	3.4	9522	PASS
441	198	0.01	100	14.1	38901	PASS
442	442	50	100	100.0	249771	PASS
443	442	15	24	20.7	51685	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011223\
 Data File : BN023615.D
 Acq On : 11 Jan 2023 17:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jan 12 04:02:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 12 04:02:28 2023
 Response via : Initial Calibration

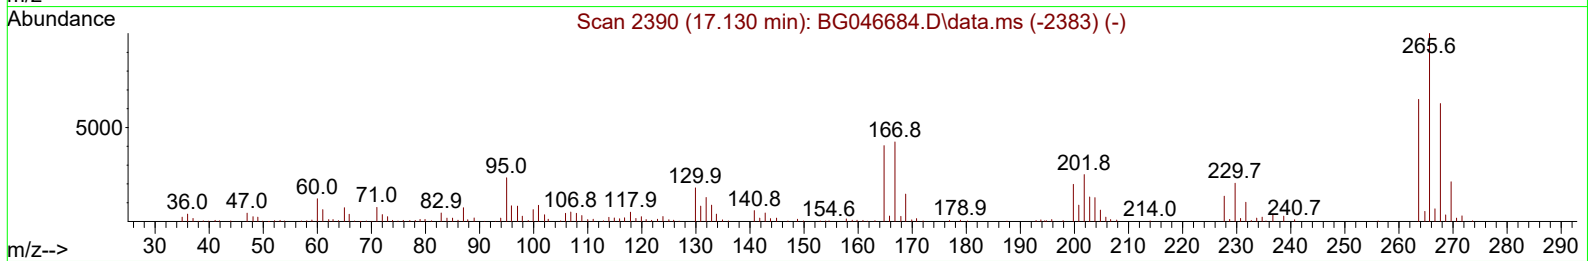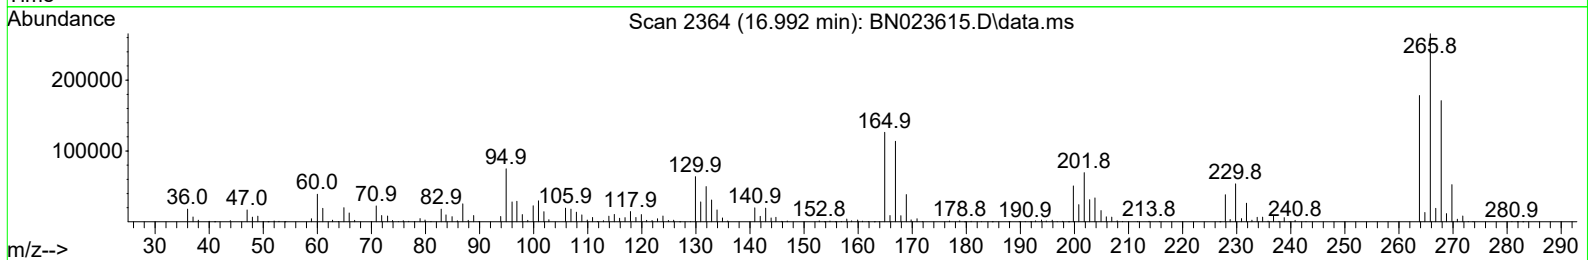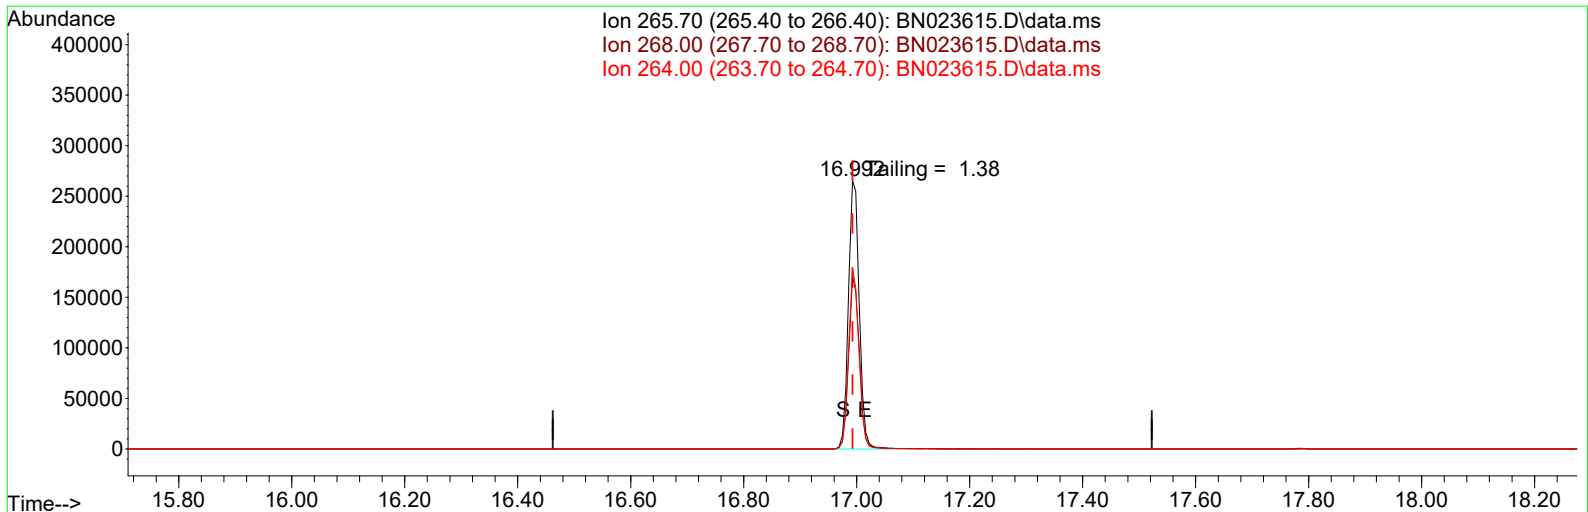

TIC: BN023615.D\data.ms

(70) Pentachlorophenol (C)

16.992min (0.000) 20863.53 ng




response 356444

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.49
264.00	61.60	67.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011223\
 Data File : BN023615.D
 Acq On : 11 Jan 2023 17:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jan 12 04:02:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 12 04:02:28 2023
 Response via : Initial Calibration

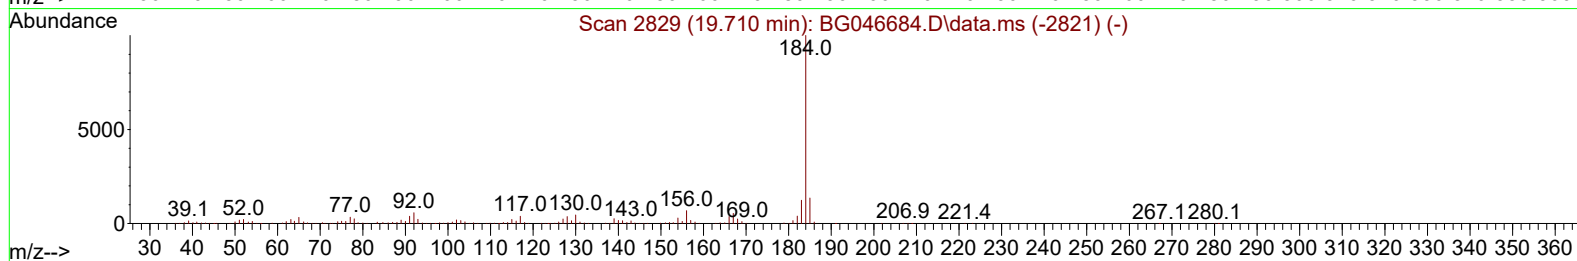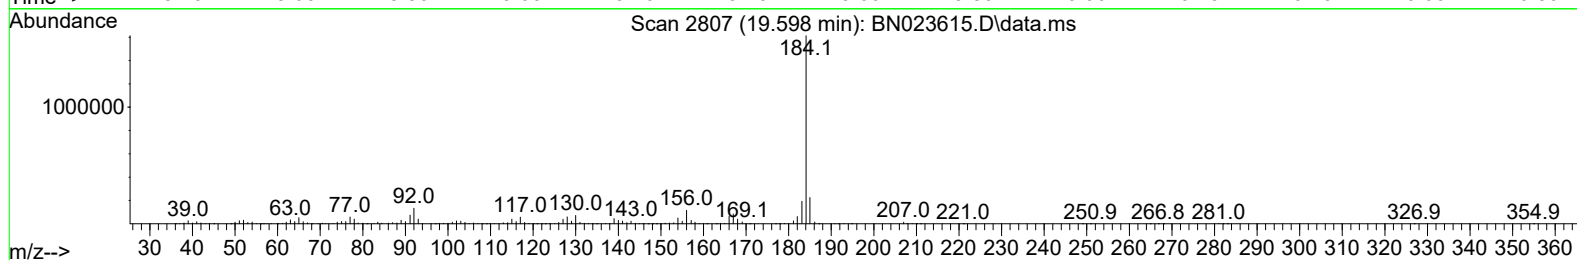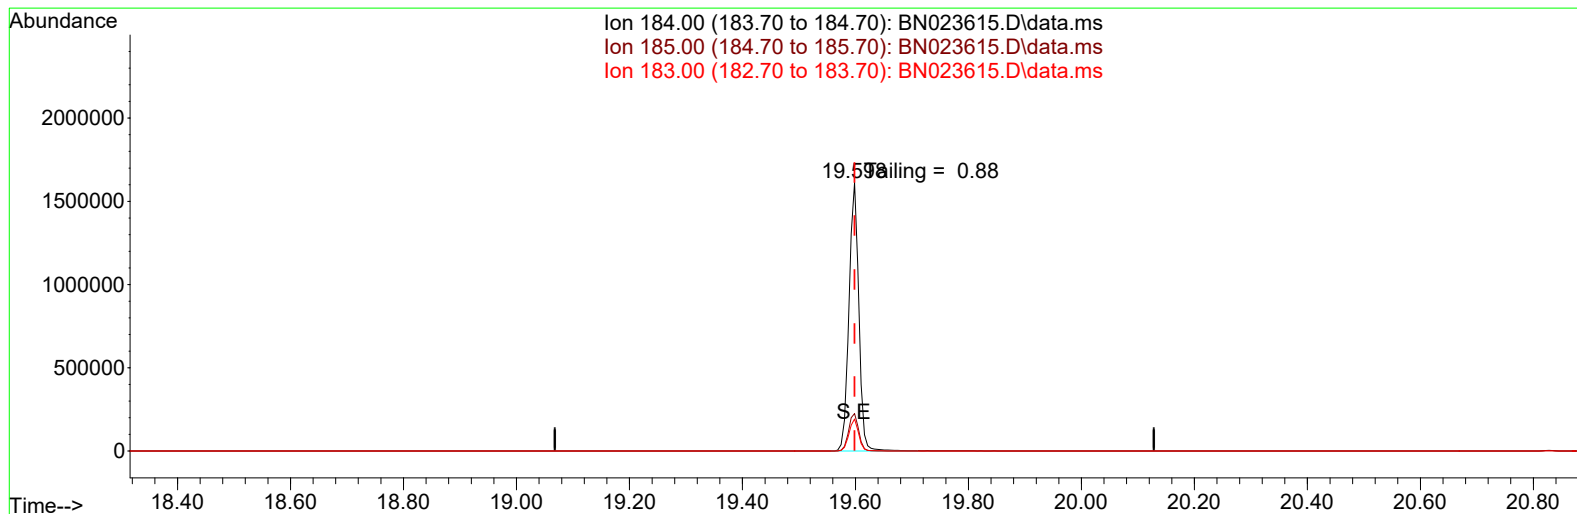

TIC: BN023615.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response 1953117

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/12/2023	BNA_N	<u>BN023615.D</u>
Compound Name	Response	Retention Time
DDT	949071	20.828
DDD	21721	20.386
DDE	950	19.881
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22671	971742	2.33

Instrument :
BNA_N
ClientSampleId :
DFTPP