


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN011320\
Data File : BN009360.D
Acq On : 13 Jan 2020 11:50
Operator : JU
Sample : PB125891BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 13 12:33:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 13 12:29:58 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK91

Manual Integrations
APPROVED

mohammad
1/14/2020 12:23:04 PM

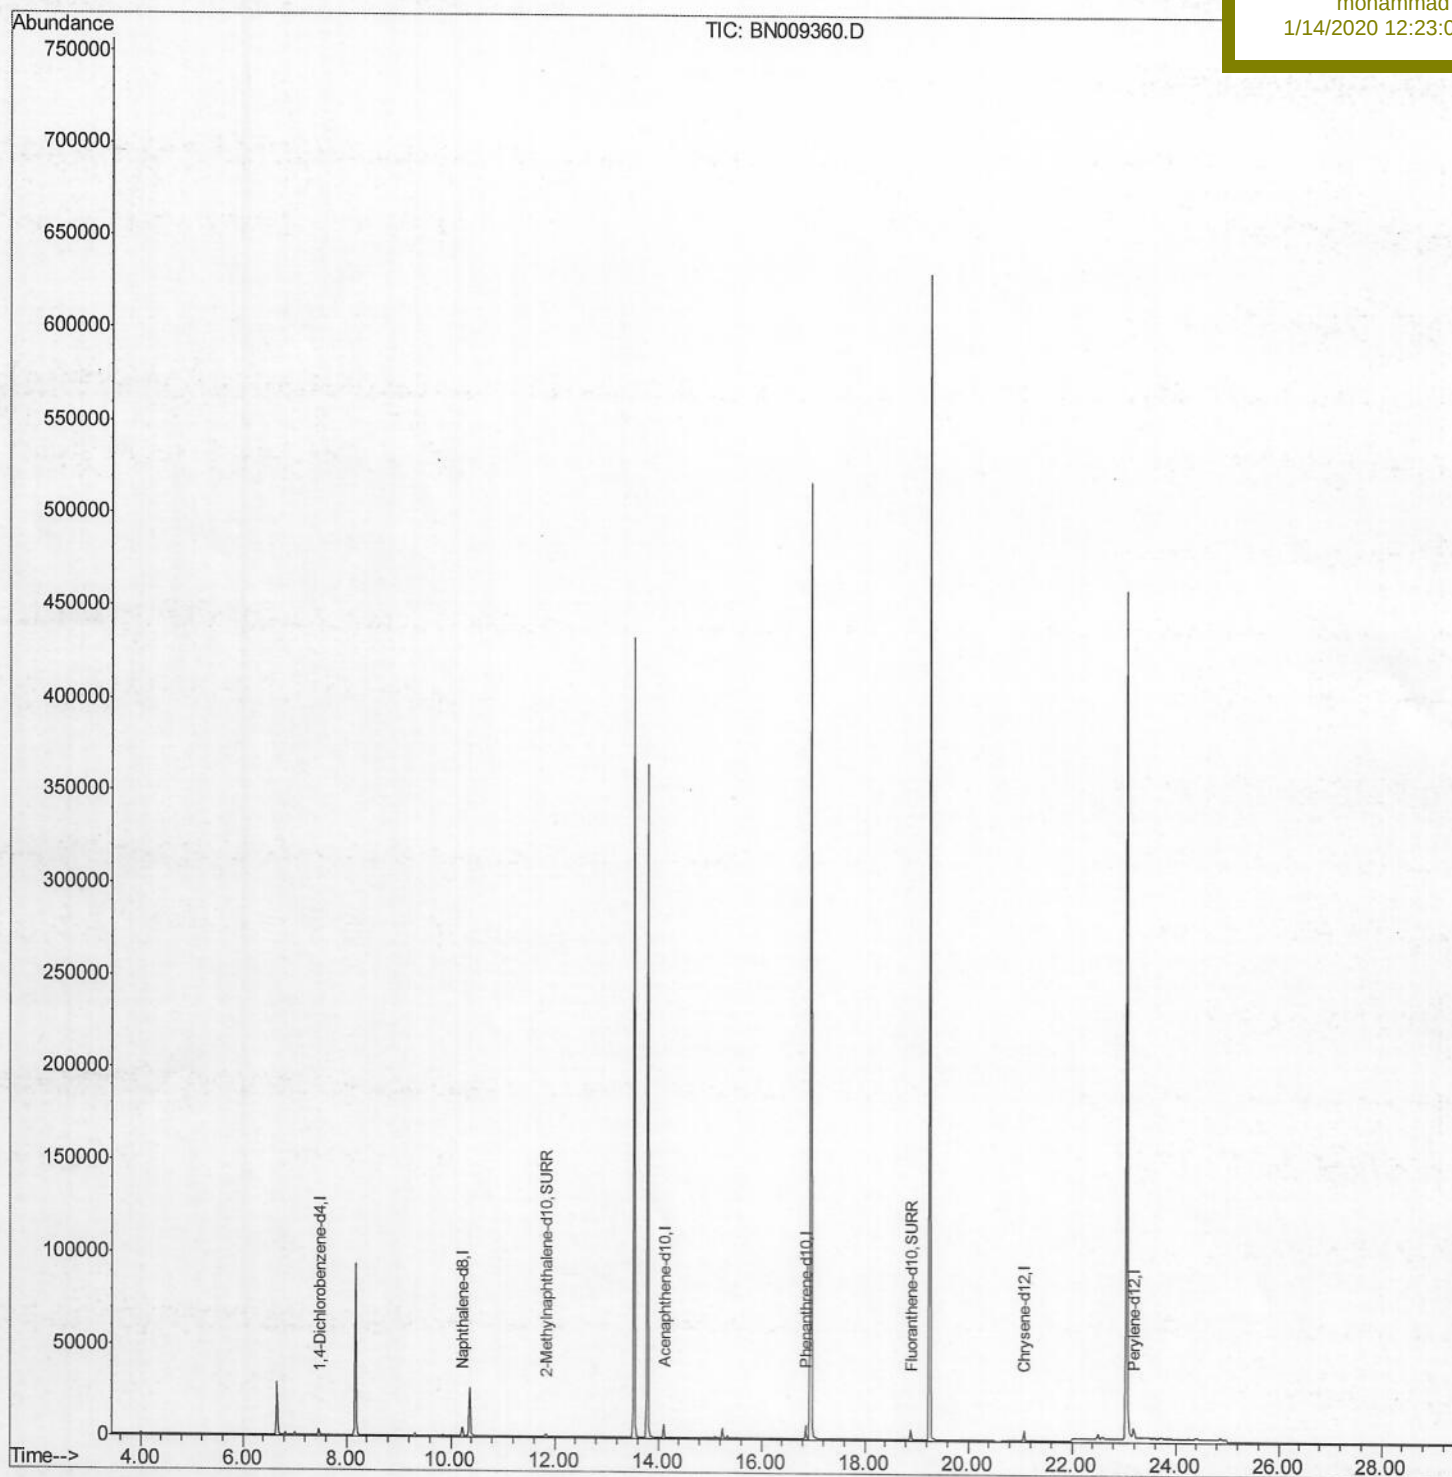

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN011320\

Data File : BN009360.D

Acq On : 13 Jan 2020 11:50

Operator : JU

Sample : PB125891BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 13 12:32:45 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jan 13 12:29:58 2020

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




SBLK91

Manual Integrations

APPROVED

mohammad

1/14/2020 12:23:04 PM

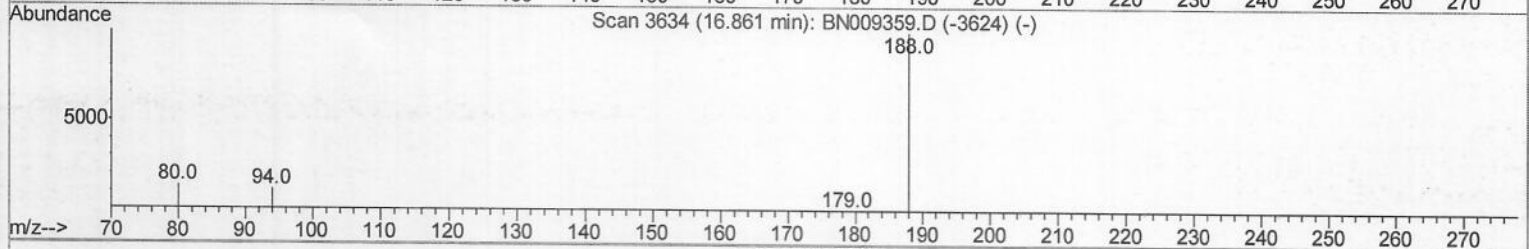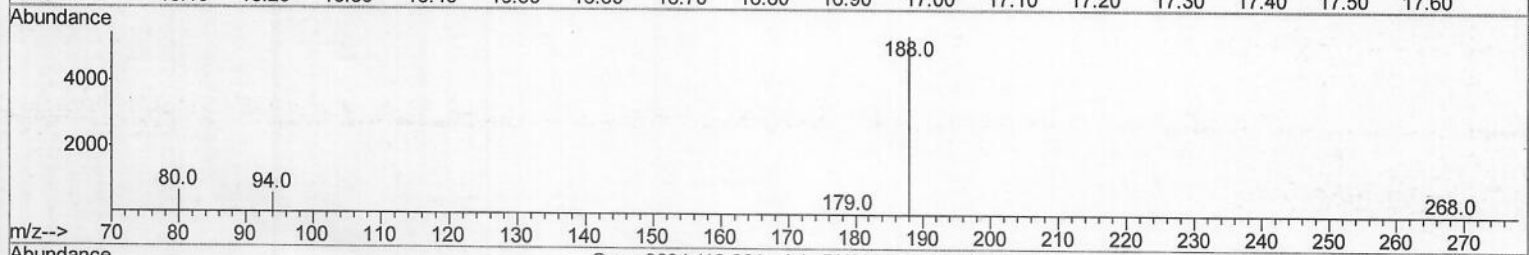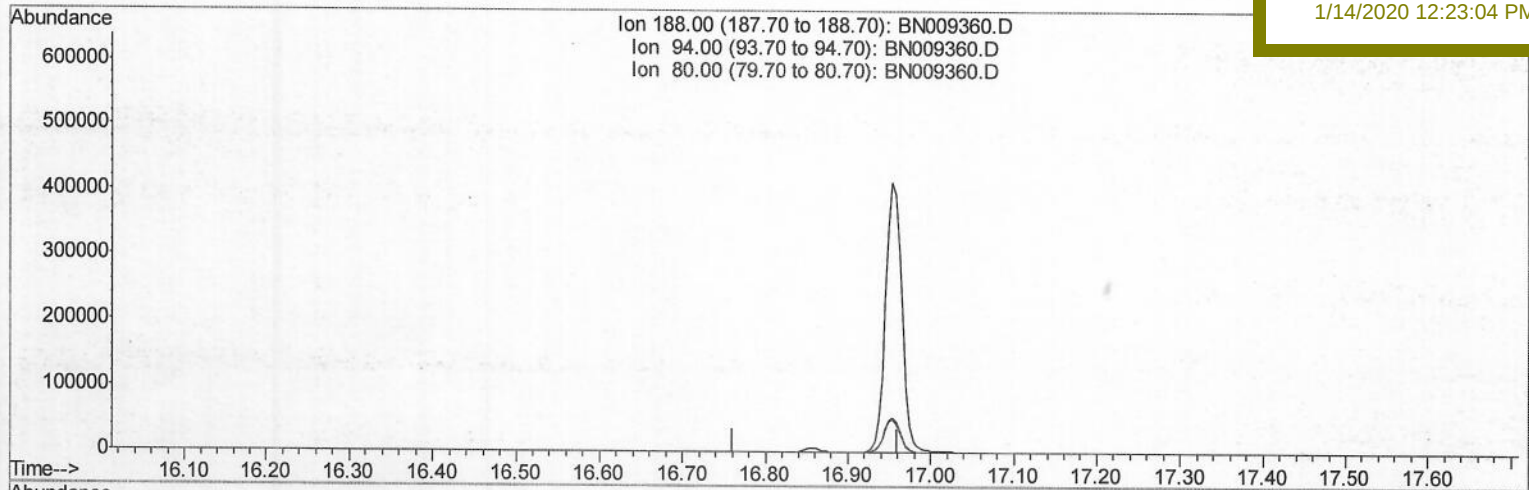

TIC: BN009360.D

(10) Phenanthrene-d10 (I)

16.861min (-16.861) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.70	0.00#
80.00	13.40	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN011320\

Data File : BN009360.D

Acq On : 13 Jan 2020 11:50

Operator : JU

Sample : PB125891BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 13 12:32:45 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jan 13 12:29:58 2020

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




SBLK91

Manual Integrations

APPROVED

mohammad

1/14/2020 12:23:04 PM

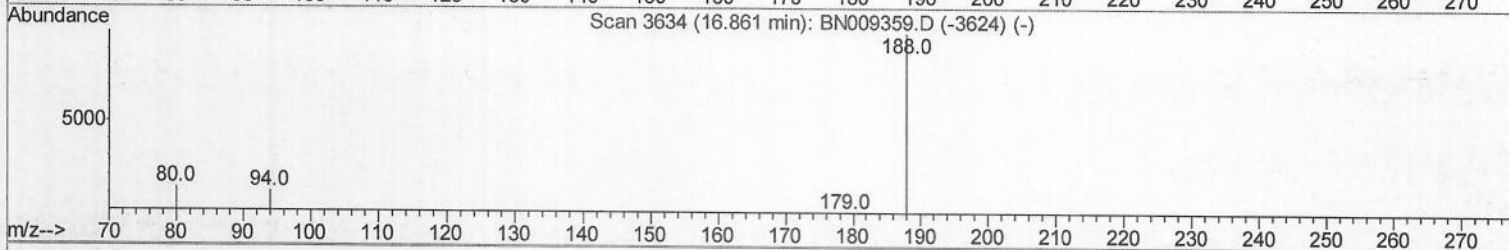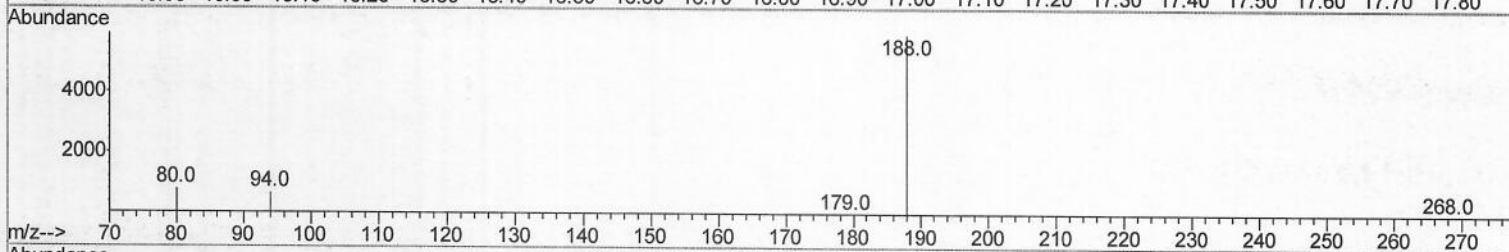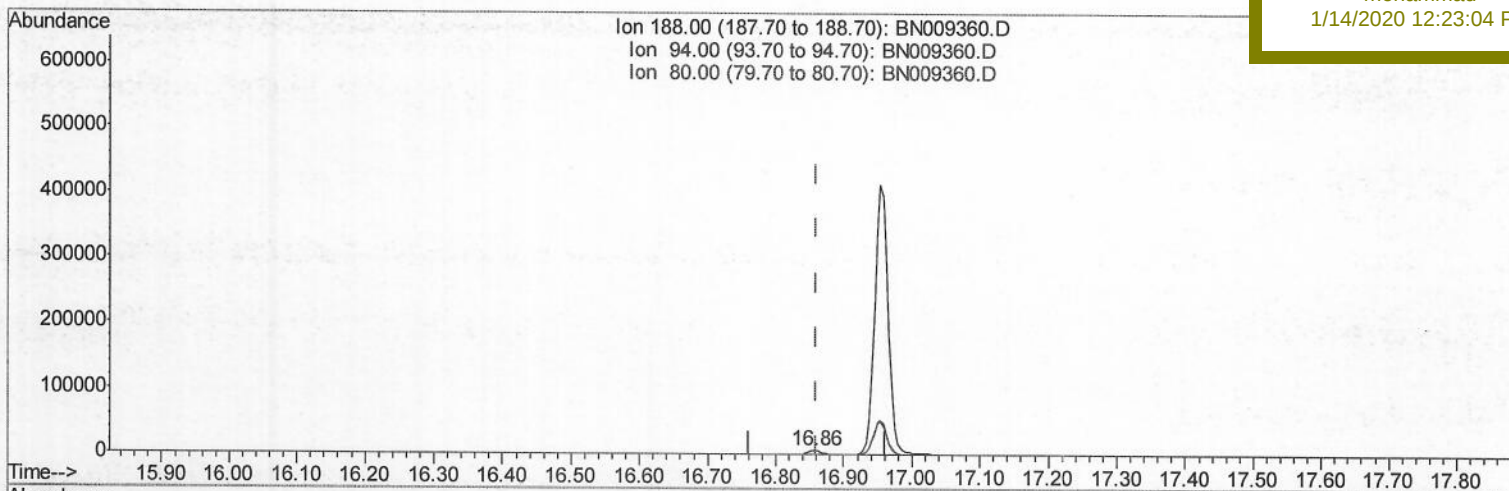

TIC: BN009360.D

(10) Phenanthrene-d10 (I)

16.857min (-0.004) 0.40ng/ul m

JU 01/14/20

response 8237

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	11.75
80.00	13.40	13.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN011320\
Data File : BN009360.D
Acq On : 13 Jan 2020 11:50
Operator : JU
Sample : PB125891BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jan 13 12:33:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN011020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 13 12:29:58 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK91

Manual Integrations
APPROVED

mohammad
1/14/2020 12:23:04 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	1771	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.22	136	6238	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.11	164	3766	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.86	188	8237m	0.40	ng/ul	0.00
16) Chrysene-d12	21.07	240	6179	0.40	ng/ul	0.00
20) Perylene-d12	23.19	264	7021	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.83	152	2664	0.26	ng/ul	0.00
14) Fluoranthene-d10	18.90	212	6581	0.26	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 01/14/20