
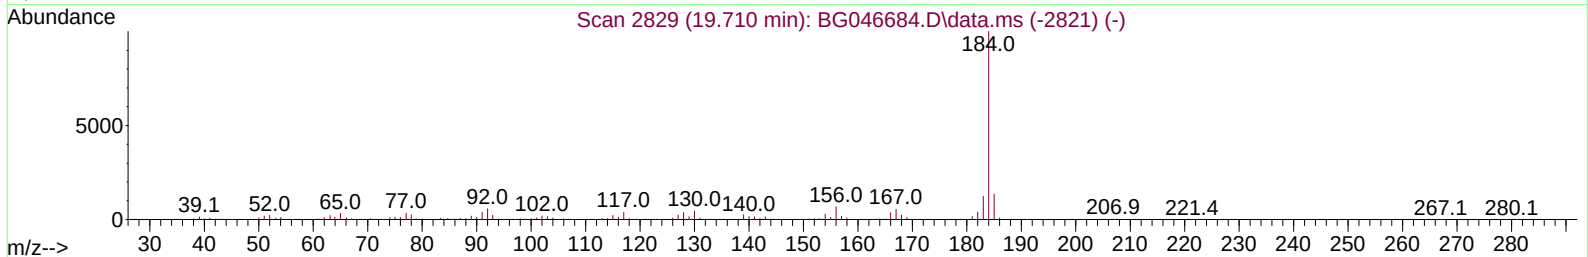
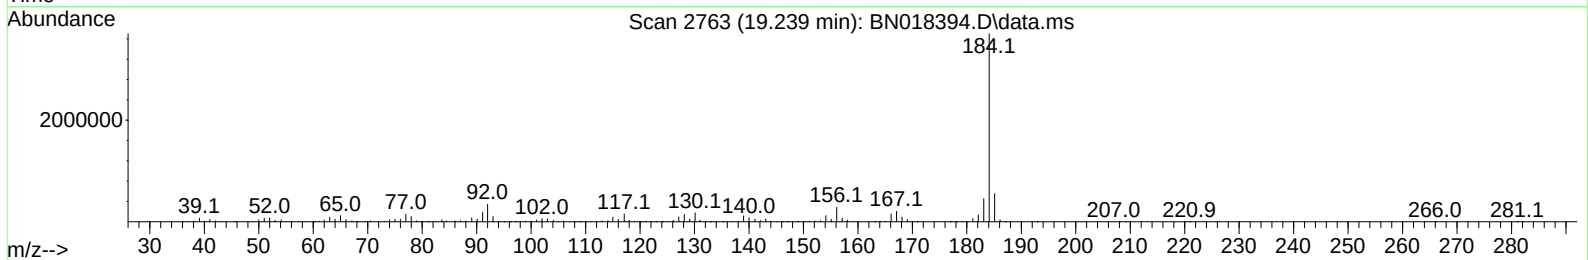


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011322\
 Data File : BN018394.D
 Acq On : 13 Jan 2022 11:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 20:43:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 10 14:39:41 2022
 Response via : Initial Calibration

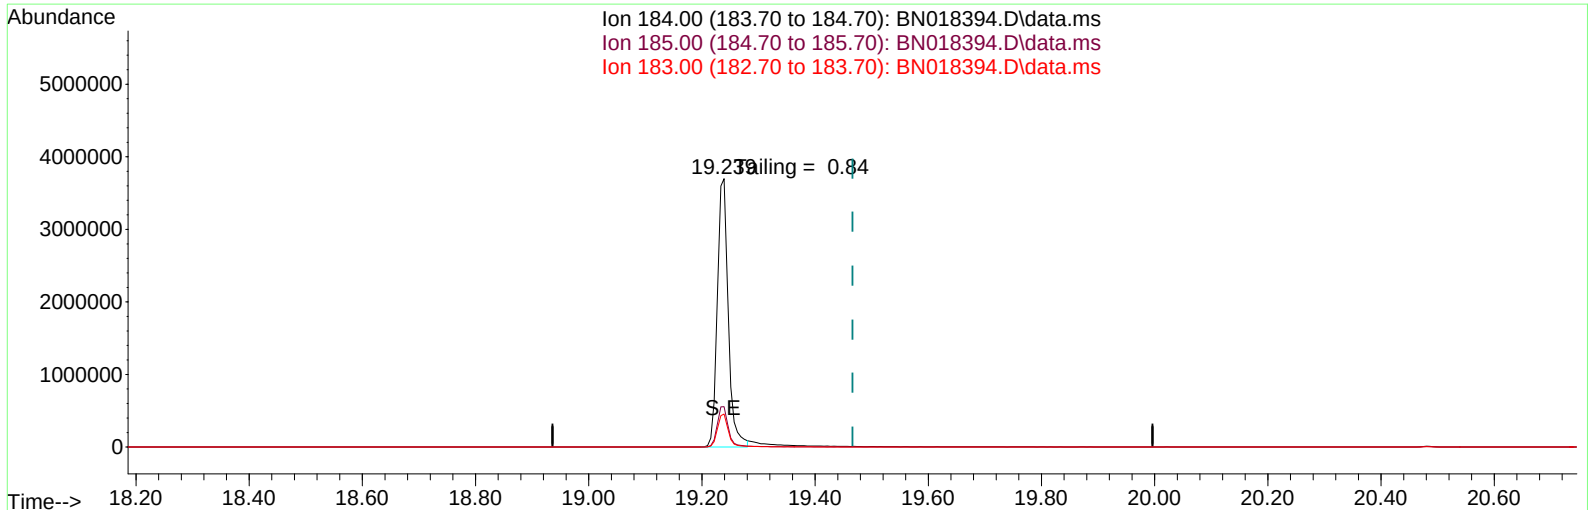

TIC: BN018394.D\data.ms

(77) Benzidine




19.239min (-0.227) 0.00 ng

response 5220217

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.02
183.00	13.20	12.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011322\
 Data File : BN018394.D
 Acq On : 13 Jan 2022 11:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 20:43:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 10 14:39:41 2022
 Response via : Initial Calibration

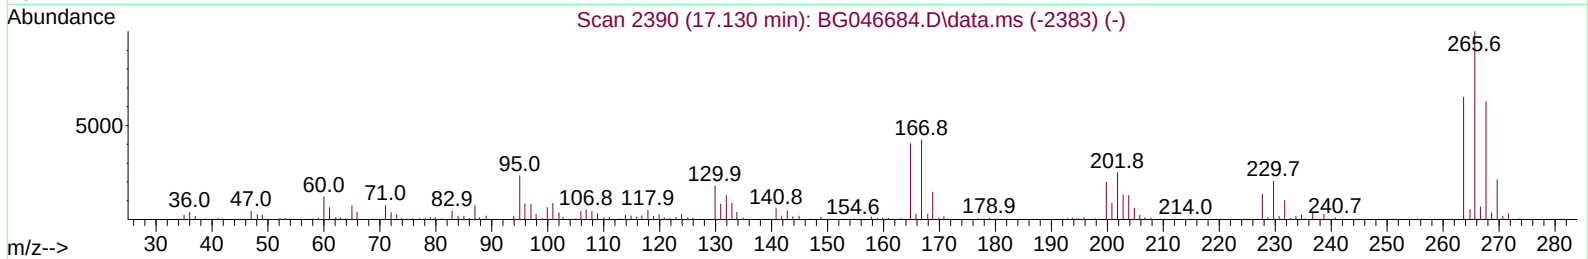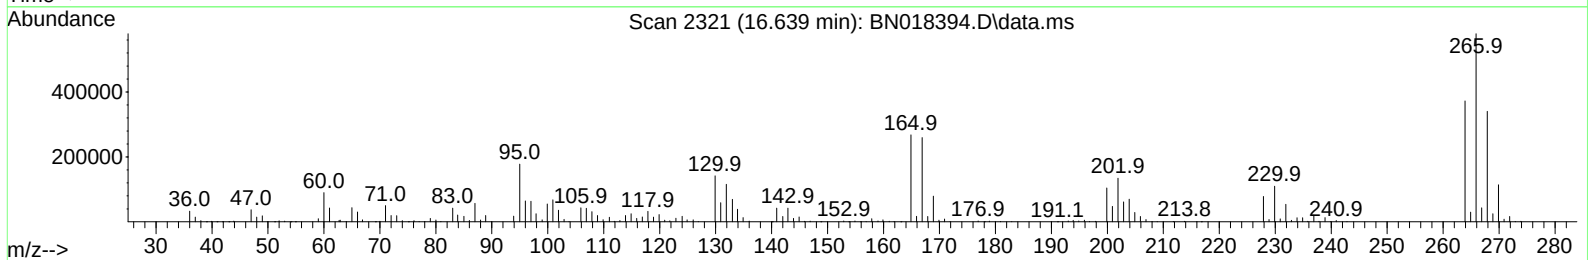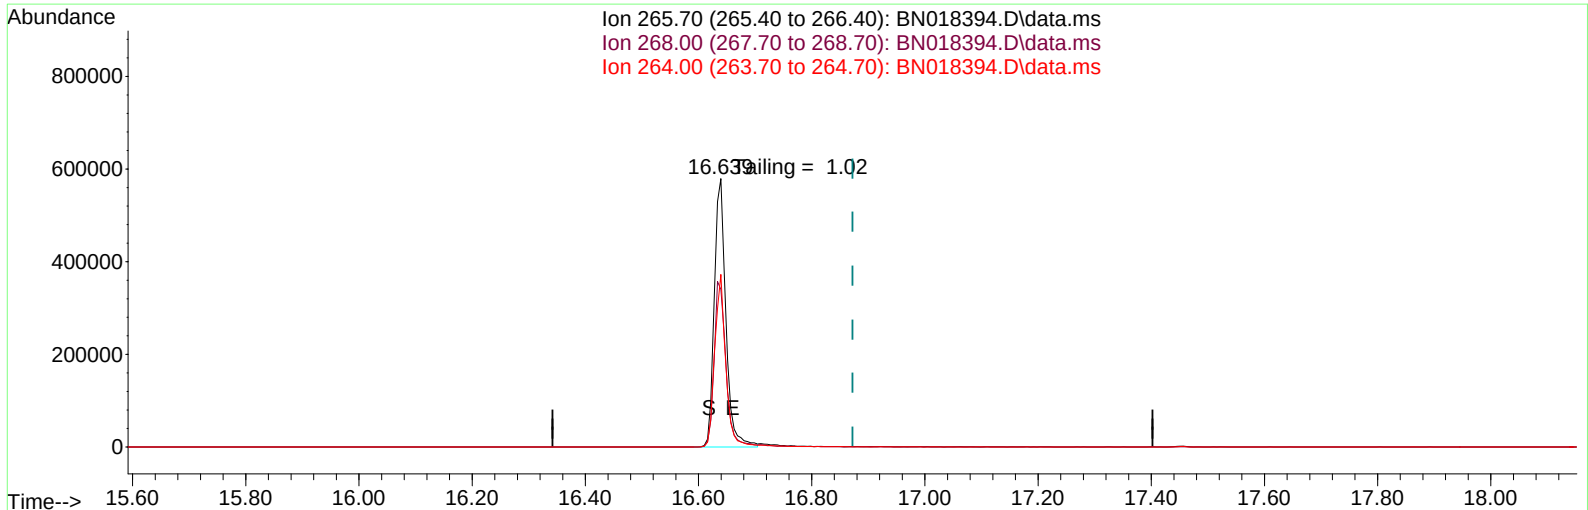

TIC: BN018394.D\data.ms

(70) Pentachlorophenol (C)

16.639min (-0.233) 19003.90 ng

response 843822

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.73
264.00	61.60	64.30
0.00	0.00	0.00