
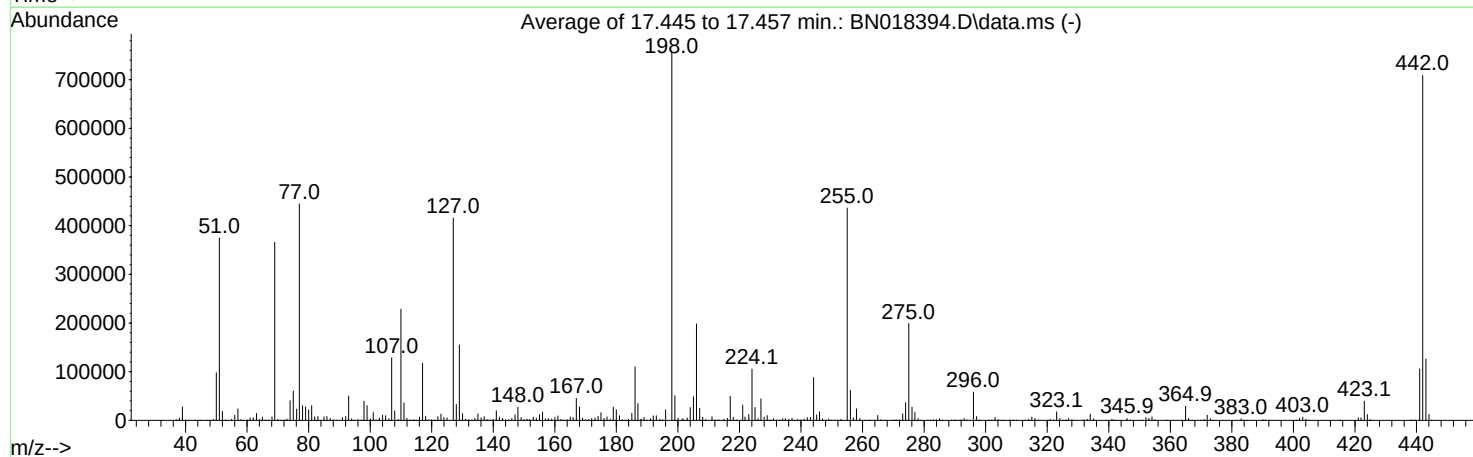


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011322\
 Data File : BN018394.D
 Acq On : 13 Jan 2022 11:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 14 12:12:13 2022

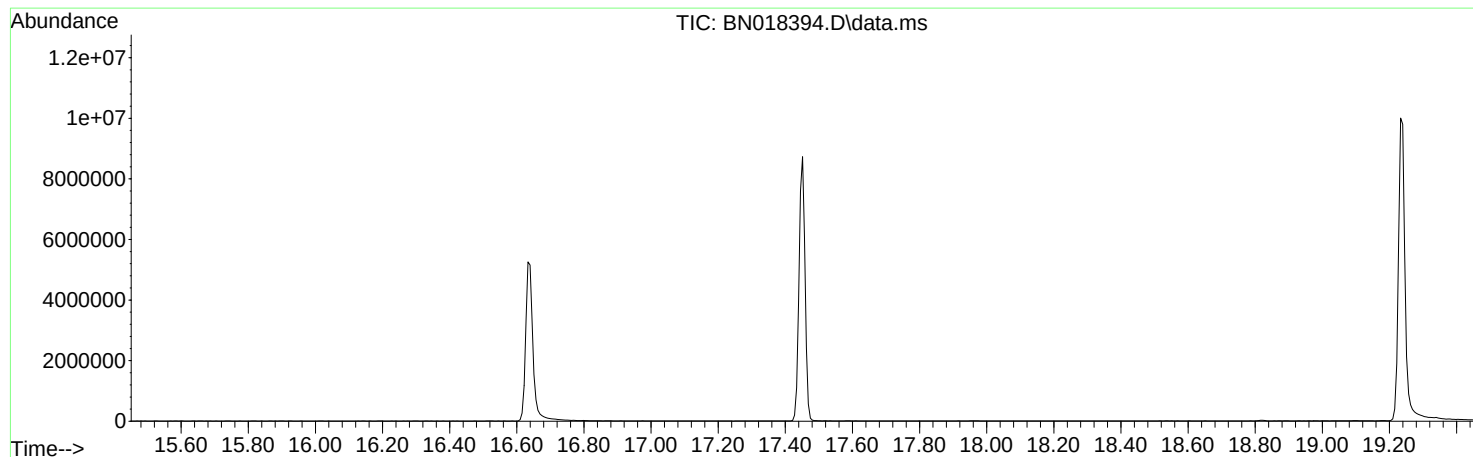




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.6	374763	PASS
68	69	0.00	2	2.0	7211	PASS
69	198	0.00	100	48.4	365781	PASS
70	69	0.00	2	0.5	1867	PASS
127	198	10	80	55.0	415616	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	755755	PASS
199	198	5	9	6.8	51037	PASS
275	198	10	60	26.4	199147	PASS
365	198	1	100	3.8	28872	PASS
441	198	0.01	100	14.0	105653	PASS
442	442	50	100	100.0	708779	PASS
443	442	15	24	17.8	126011	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011322\
Data File : BN018394.D
Acq On : 13 Jan 2022 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 13 20:43:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 10 14:39:41 2022
Response via : Initial Calibration

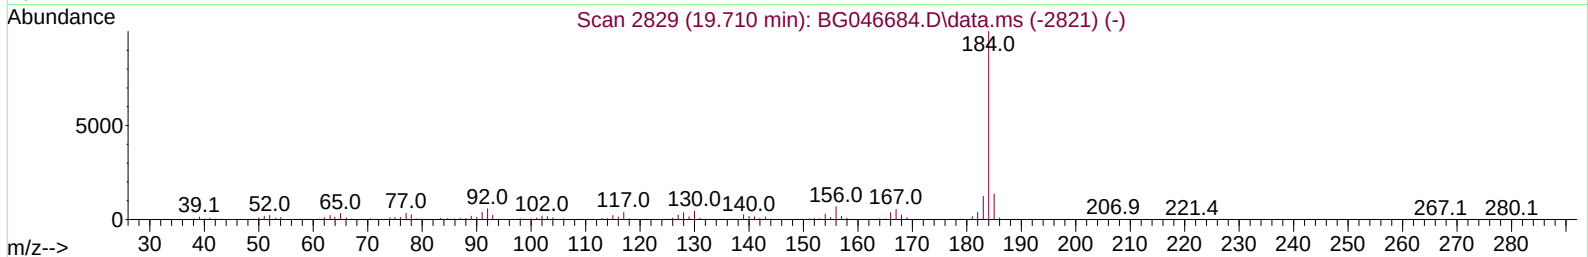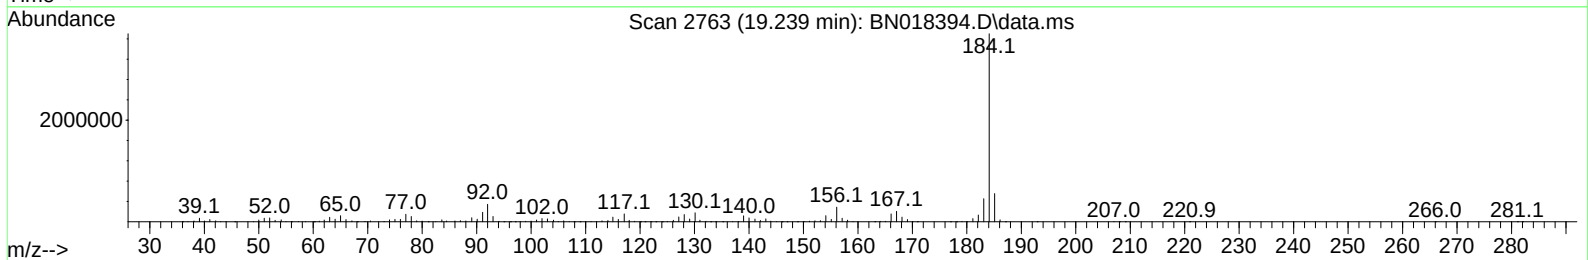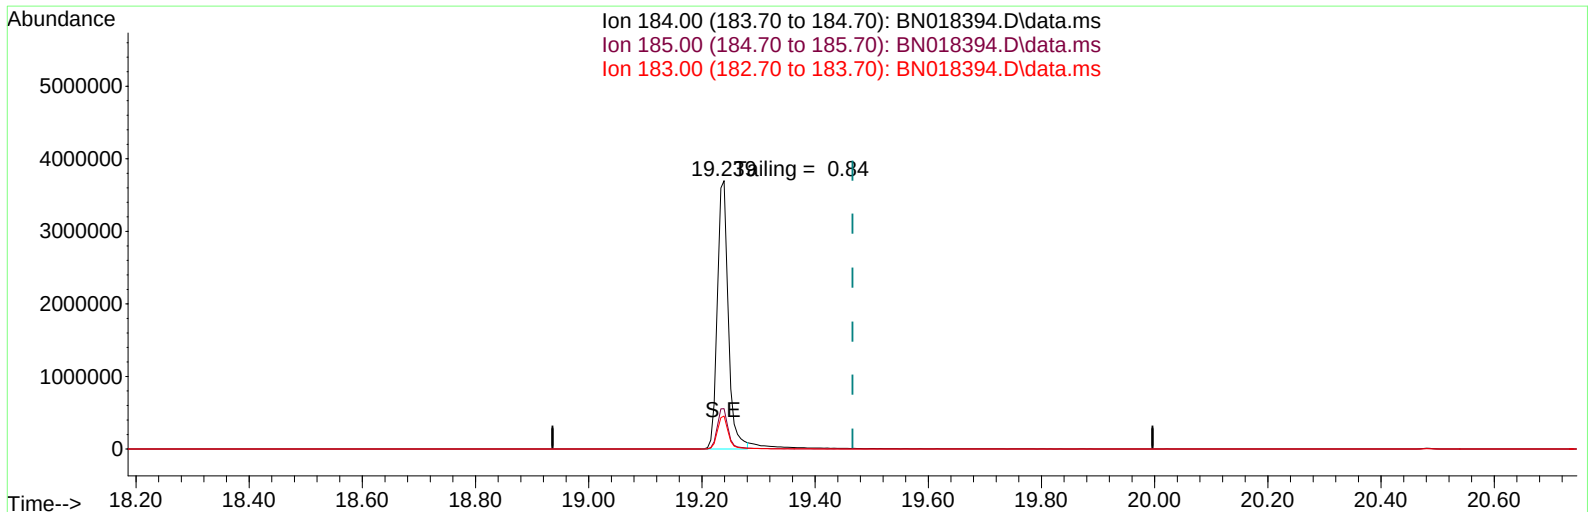

TIC: BN018394.D\data.ms

(77) Benzidine

19.239min (-0.227) 0.00 ng




response 5220217

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.02
183.00	13.20	12.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011322\
Data File : BN018394.D
Acq On : 13 Jan 2022 11:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 13 20:43:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 10 14:39:41 2022
Response via : Initial Calibration

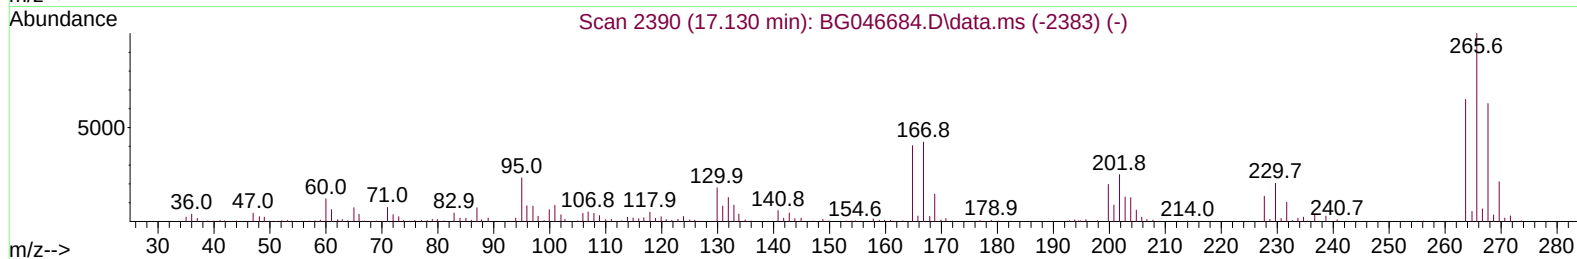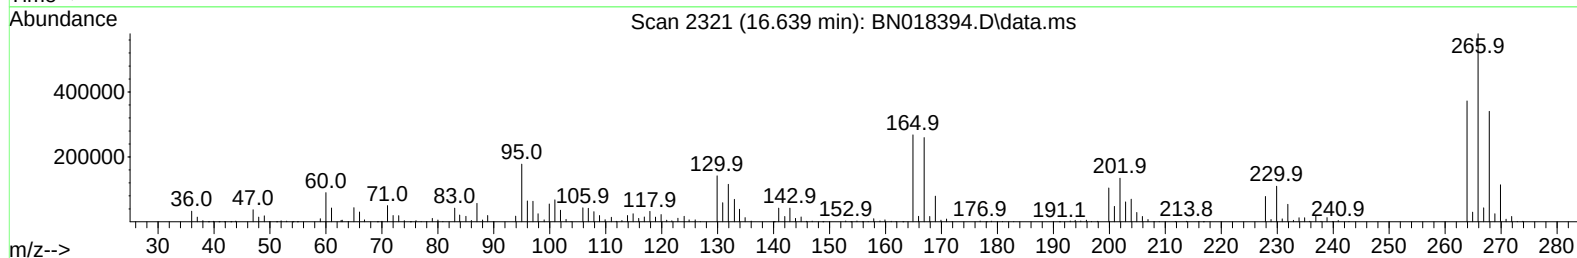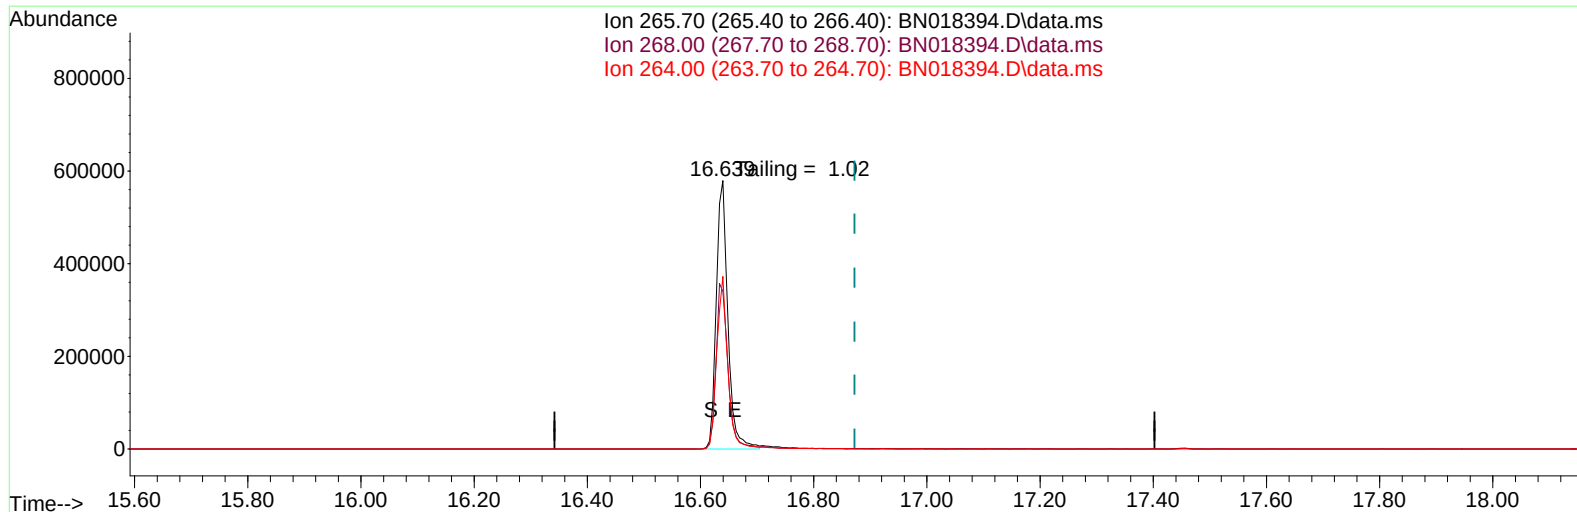

TIC: BN018394.D\data.ms

(70) Pentachlorophenol (C)

16.639min (-0.233) 19003.90 ng

response 843822

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.73
264.00	61.60	64.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/13/2022	BNA_N	<u>BN018394.D</u>
Compound Name	Response	Retention Time
DDT	2527838	20.48
DDD	21748	20.03
DDE	1304	19.53
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23052	2550890	0.90

Instrument :
BNA_N
ClientSampleId :
DFTPP