

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023749.D
 Acq On : 23 Jan 2023 12:55
 Operator : CG/JU
 Sample : 01146-12MEDL 50X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4418MEDL

Quant Time: Jan 23 23:59:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	193187	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	819181	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	453229	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	1104038	20.000	ng/ul	0.00
79) Chrysene-d12	21.475	240	1048218	20.000	ng/ul	-0.01
88) Perylene-d12	23.910	264	1078922	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	1042	0.232	ng/uL	0.00
4) Pyridine-d5	3.687	84	591	0.044	ng/ul	-0.01
7) Phenol-d5	7.052	99	7083	0.414	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	6278	0.598	ng/ul	0.00
11) 2-Chlorophenol-d4	7.417	132	5412	0.413	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	5110	0.374	ng/ul	0.00
21) Nitrobenzene-d5	9.058	128	2645	0.428	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	1979	0.303	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	3789	0.304	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	7011	0.357	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	19608	0.582	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	17767	0.476	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	223	0.032	ng/ul	0.01
60) Fluorene-d10	15.528	176	16924	0.587	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	338	0.051	ng/ul	0.00
73) Anthracene-d10	17.381	188	23980	0.485	ng/ul	0.00
81) Pyrene-d10	19.675	212	28825	0.481	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	23729	0.445	ng/ul	-0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.392	149	2038055	47.873	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023749.D
Acq On : 23 Jan 2023 12:55
Operator : CG/JU
Sample : 01146-12MEDL 50X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4418MEDL


Quant Time: Jan 23 23:59:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

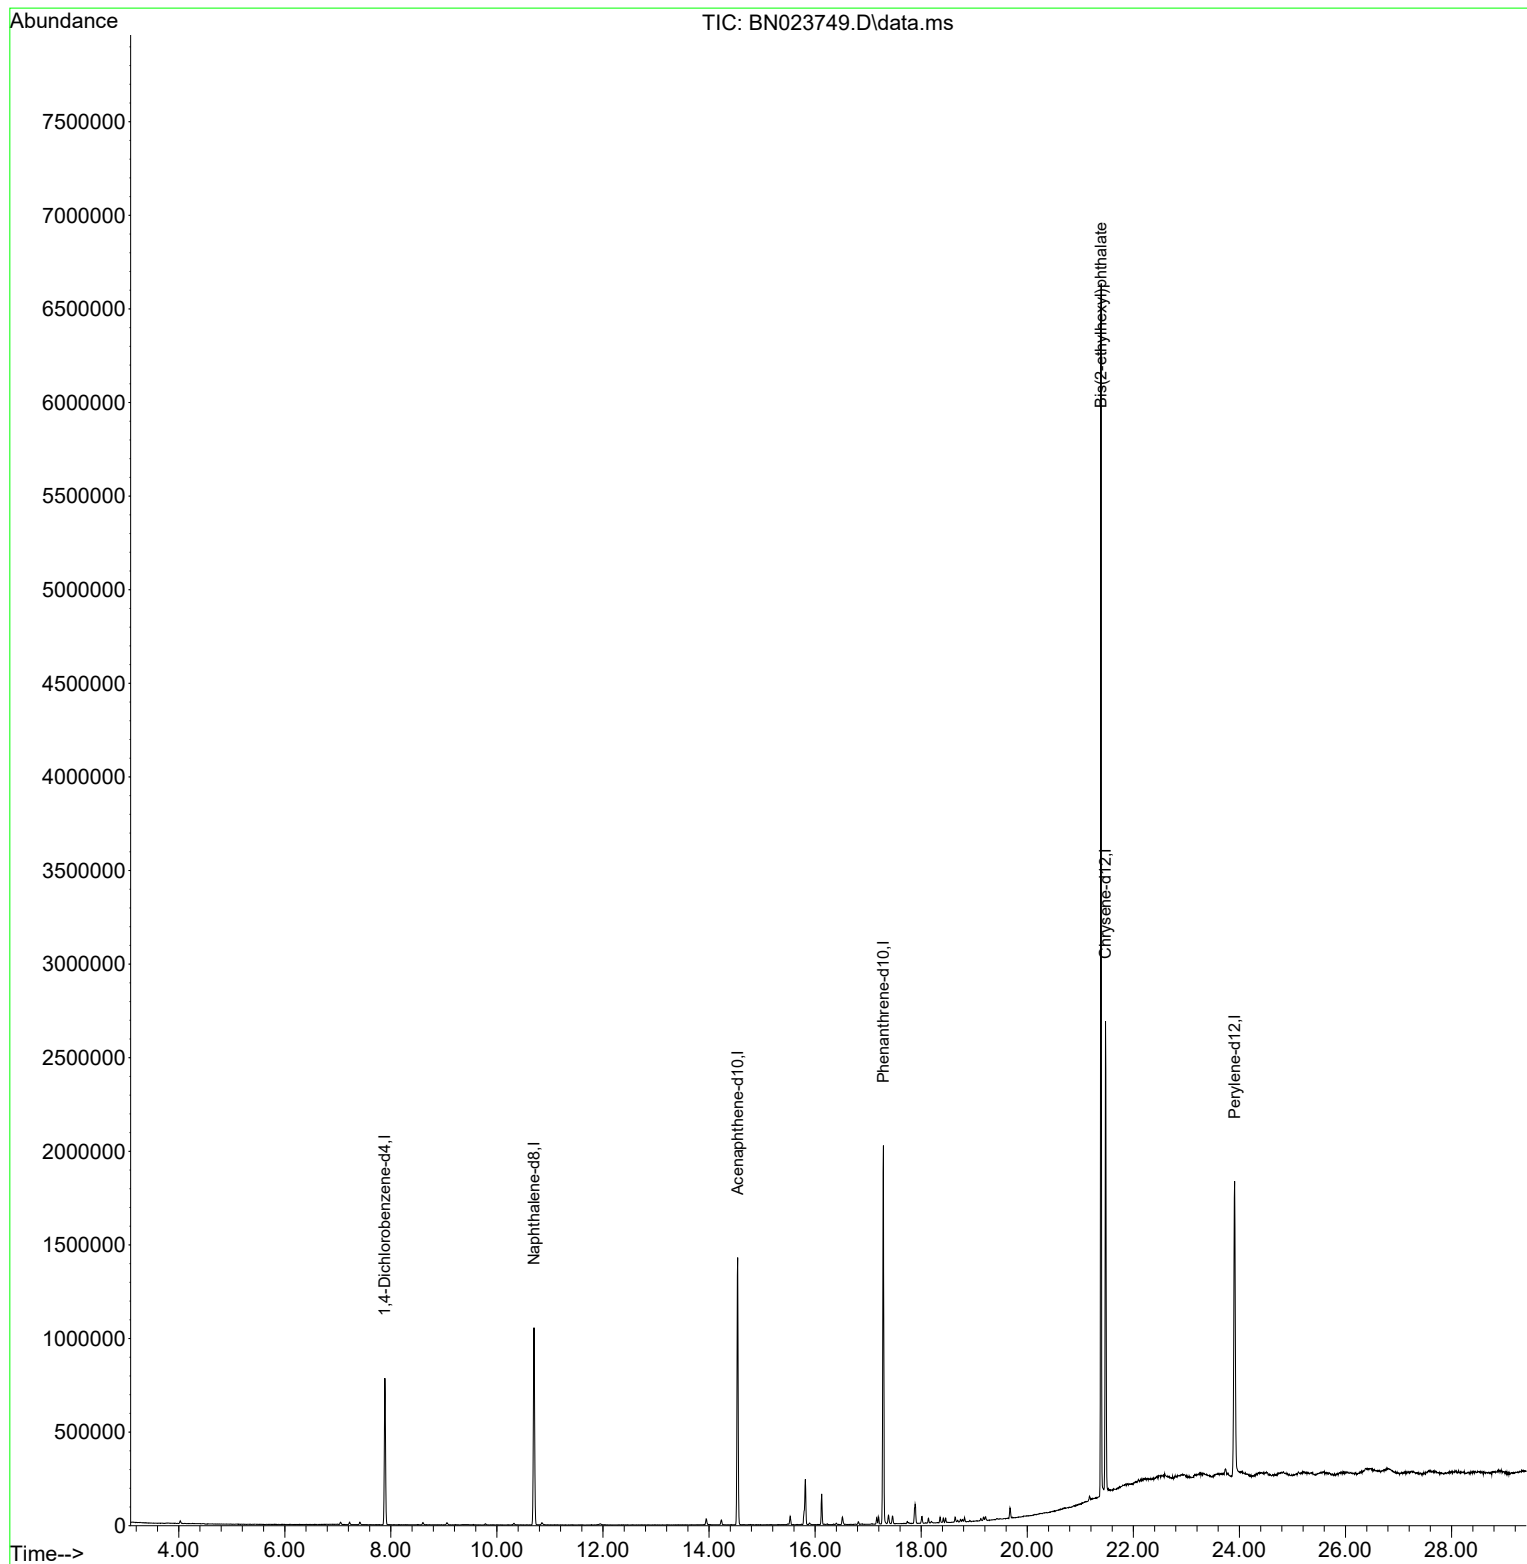

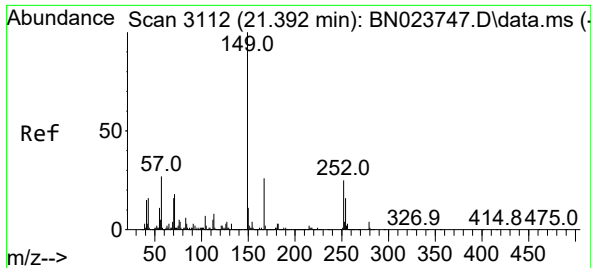

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 47.873 ng/ul
 RT: 21.392 min Scan# 3112
 Delta R.T. 0.000 min
 Lab File: BN023749.D
 Acq: 23 Jan 2023 12:55

Instrument :
 BNA_N
 ClientSampleId :
 A4418MEDL

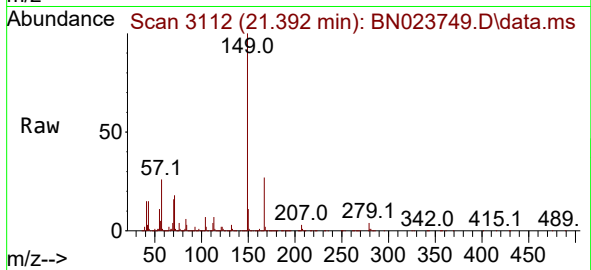

Tgt Ion:149 Resp: 2038055
 Ion Ratio Lower Upper
 149 100
 167 26.7 22.0 33.0
 279 4.3 3.4 5.2

