

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023751.D
 Acq On : 23 Jan 2023 14:09
 Operator : CG/JU
 Sample : 01146-16MEDL 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4470MEDL

Quant Time: Jan 24 00:00:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	179425	20.000	ng/ul	0.00
20) Naphthalene-d8	10.698	136	746807	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	440569	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	1042534	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	956304	20.000	ng/ul	0.00
88) Perylene-d12	23.910	264	1002127	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	2823	0.677	ng/uL	0.00
4) Pyridine-d5	3.716	84	19653	1.571	ng/ul	0.02
7) Phenol-d5	7.052	99	33947	2.135	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	25618	2.626	ng/ul	0.00
11) 2-Chlorophenol-d4	7.416	132	26562	2.181	ng/ul	0.00
15) 4-Methylphenol-d8	8.599	113	24473	1.928	ng/ul	-0.01
21) Nitrobenzene-d5	9.057	128	11674	2.073	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	9643	1.618	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	19333	1.700	ng/ul	0.00
31) 4-Chloroaniline-d4	10.845	131	36924	2.064	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	81077	2.474	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	73157	2.015	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	2455	0.368	ng/ul	0.00
60) Fluorene-d10	15.528	176	71002	2.535	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	1601	0.255	ng/ul	0.00
73) Anthracene-d10	17.380	188	108760	2.331	ng/ul	0.00
81) Pyrene-d10	19.680	212	139471	2.550	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	113461	2.289	ng/ul	-0.02


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.392	149	1187543	30.576 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023751.D
Acq On : 23 Jan 2023 14:09
Operator : CG/JU
Sample : 01146-16MEDL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4470MEDL


Quant Time: Jan 24 00:00:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

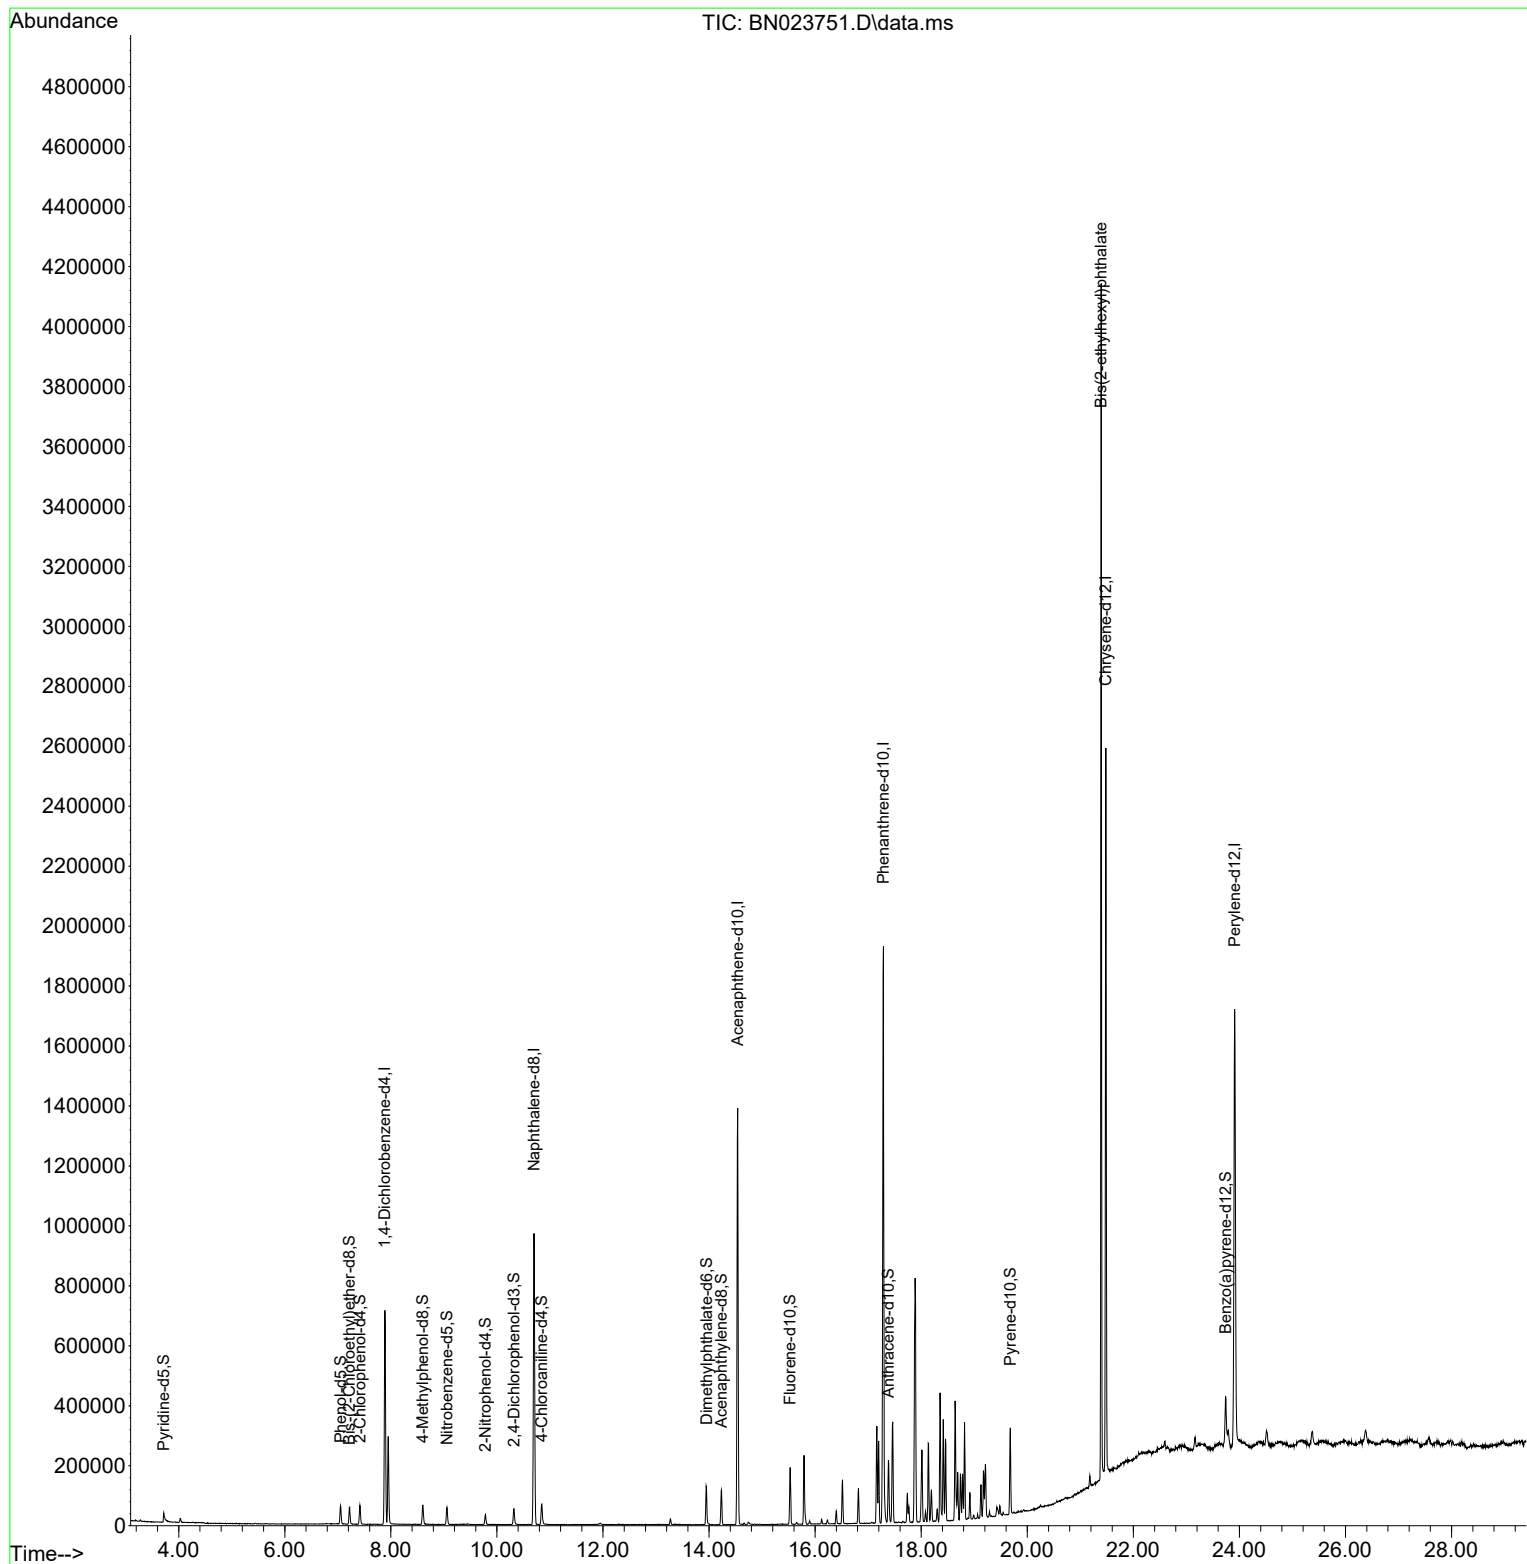

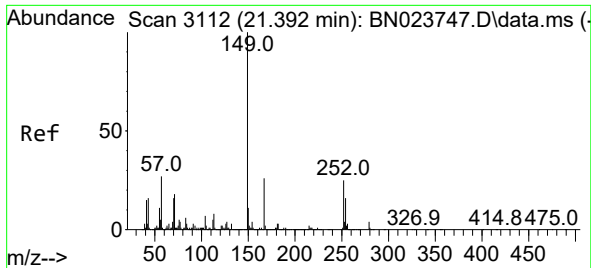

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 30.576 ng/ul
 RT: 21.392 min Scan# 3112
 Delta R.T. 0.000 min
 Lab File: BN023751.D
 Acq: 23 Jan 2023 14:09

Instrument :
 BNA_N
 ClientSampleId :
 A4470MEDL

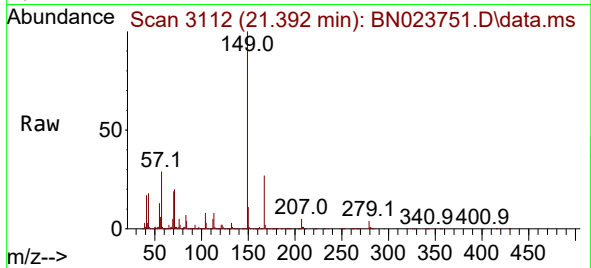

Tgt Ion:149 Resp: 1187543
 Ion Ratio Lower Upper
 149 100
 167 26.8 22.0 33.0
 279 3.8 3.4 5.2

