




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023750.D
Acq On : 23 Jan 2023 13:32
Operator : CG/JU
Sample : 01146-14MEDL 30X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4462MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 23 23:59:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/24/2023
Supervised By :mohammad ahmed 01/24/2023

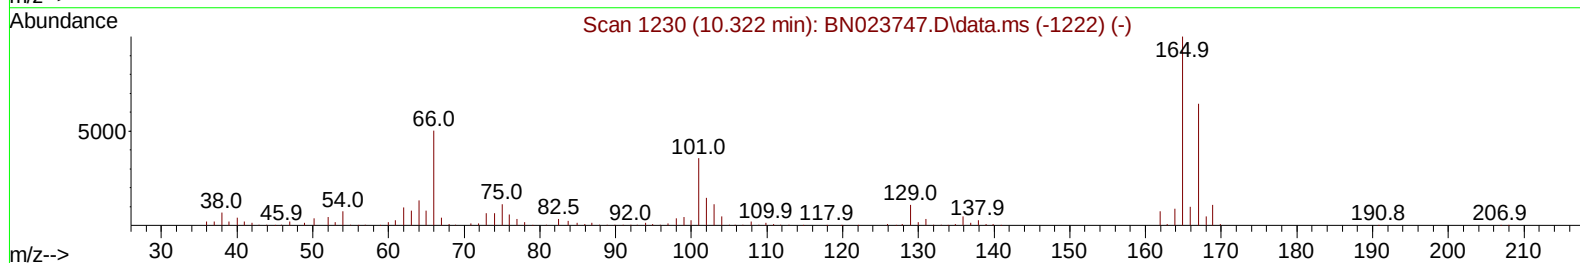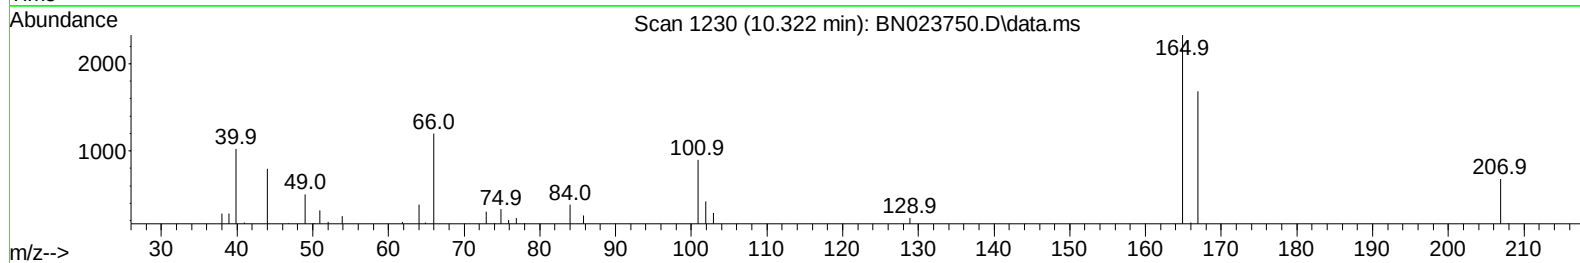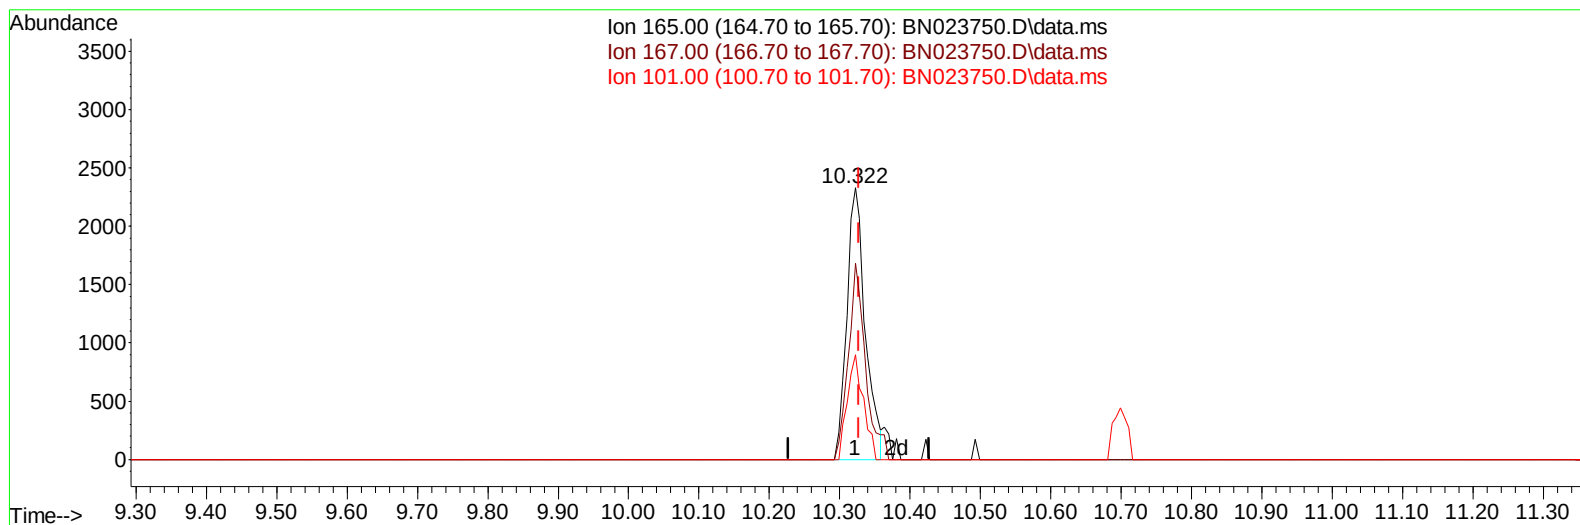

TIC: BN023750.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.322min (-0.006) 0.35 ng/ul

response 4207

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	63.60	72.31
101.00	34.00	38.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023750.D
Acq On : 23 Jan 2023 13:32
Operator : CG/JU
Sample : 01146-14MEDL 30X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4462MEDL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/24/2023
Supervised By :mohammad ahmed 01/24/2023

Quant Time: Jan 23 23:59:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

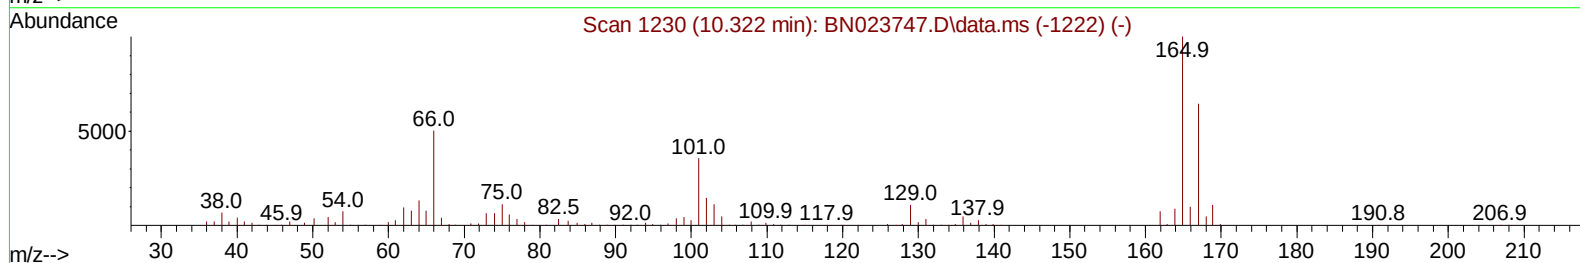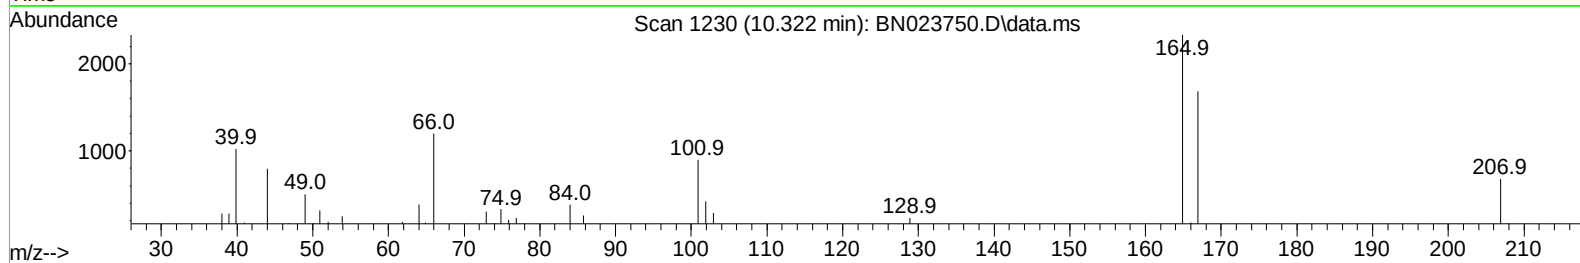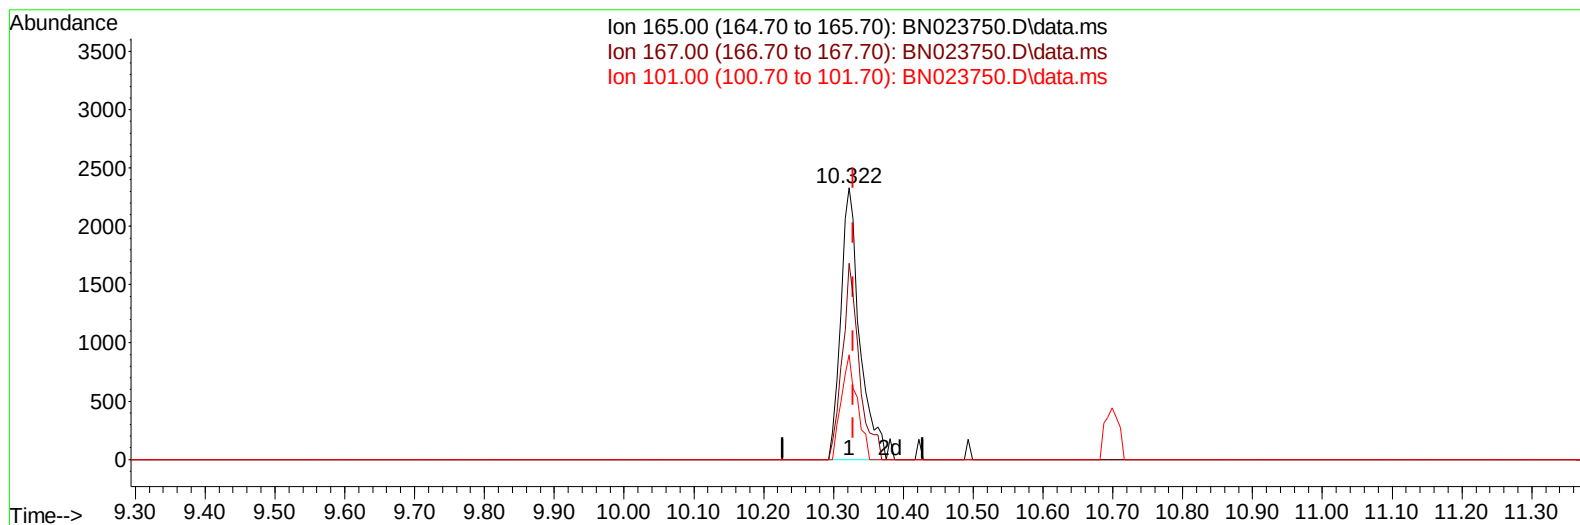

TIC: BN023750.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.322min (-0.006) 0.36 ng/ul m

response 4382

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	63.60	72.31
101.00	34.00	38.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023750.D
 Acq On : 23 Jan 2023 13:32
 Operator : CG/JU
 Sample : 01146-14MEDL 30X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4462MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 23 23:59:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/24/2023
 Supervised By :mohammad ahmed 01/24/2023

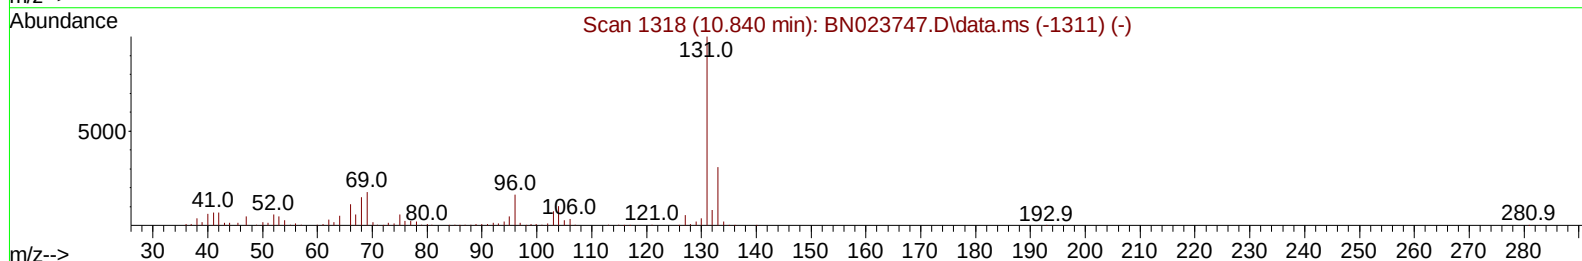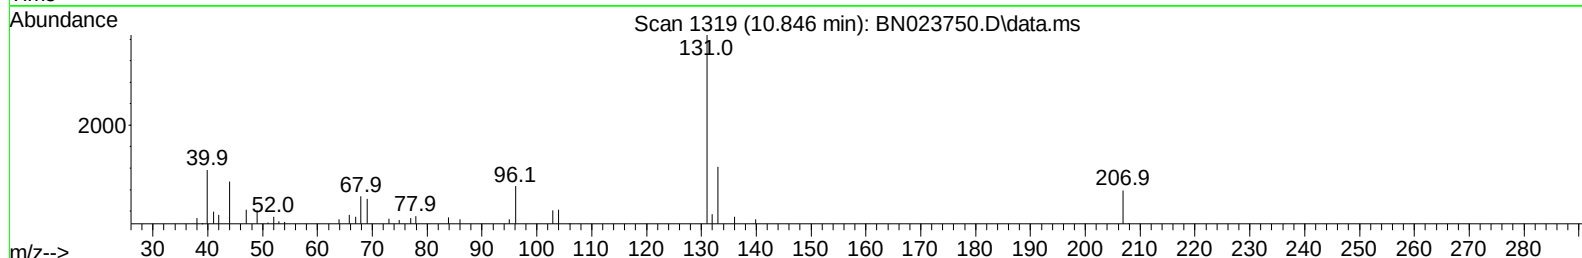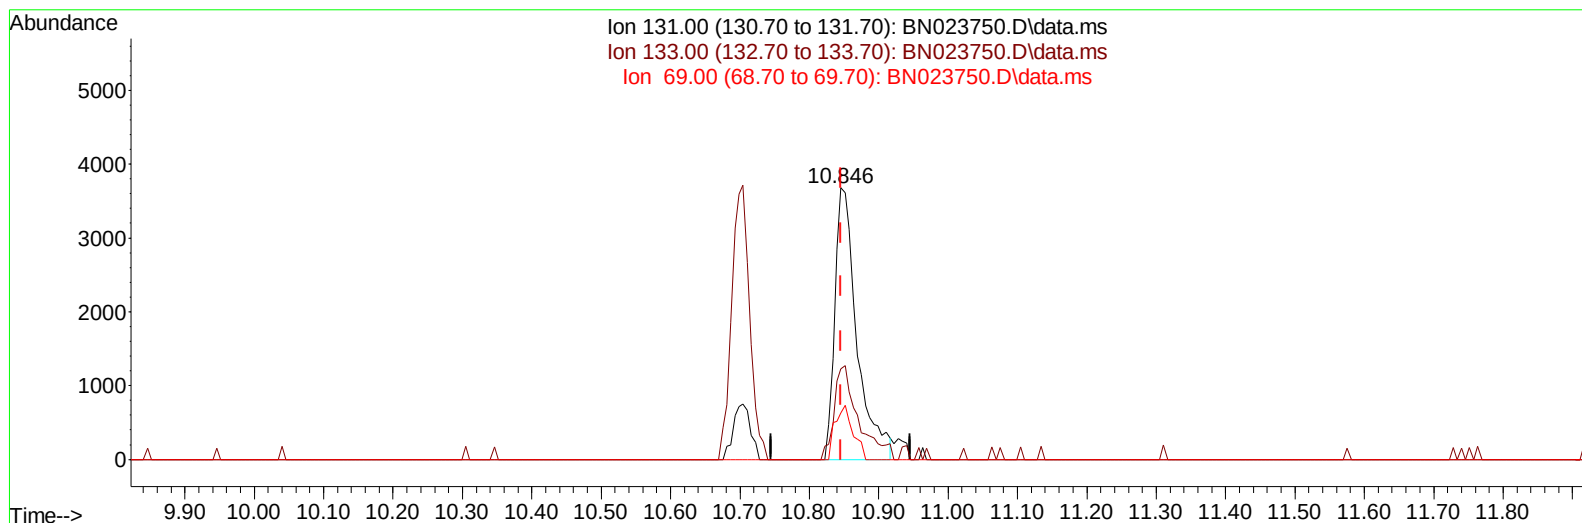

TIC: BN023750.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.846min (+ 0.000) 0.42 ng/ul

response 8104

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.40	33.28
69.00	17.20	17.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023750.D
 Acq On : 23 Jan 2023 13:32
 Operator : CG/JU
 Sample : 01146-14MEDL 30X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4462MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 23 23:59:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/24/2023
 Supervised By :mohammad ahmed 01/24/2023

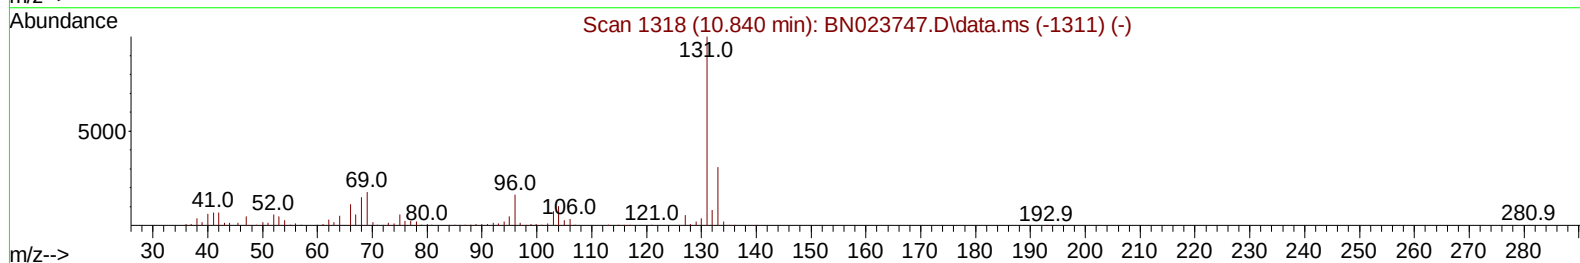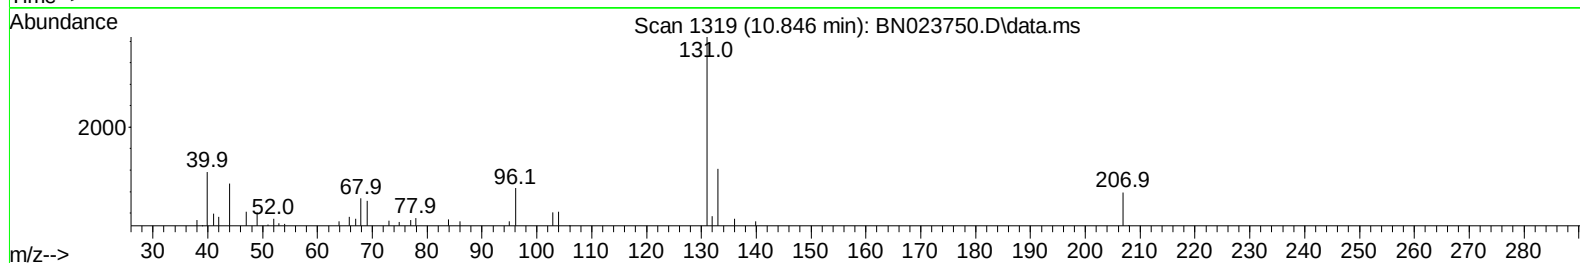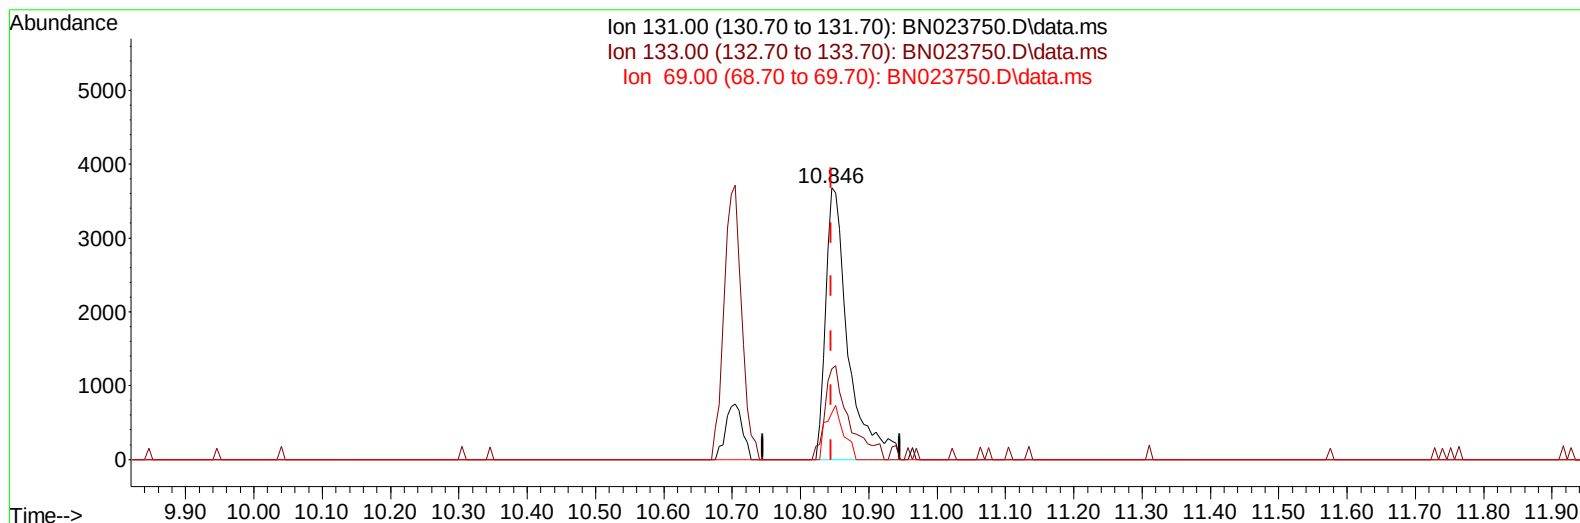

TIC: BN023750.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.846min (+ 0.000) 0.44 ng/ul m

response 8444

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.40	33.28
69.00	17.20	17.21
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023750.D
 Acq On : 23 Jan 2023 13:32
 Operator : CG/JU
 Sample : 01146-14MEDL 30X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4462MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 23 23:59:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/24/2023
 Supervised By :mohammad ahmed 01/24/2023

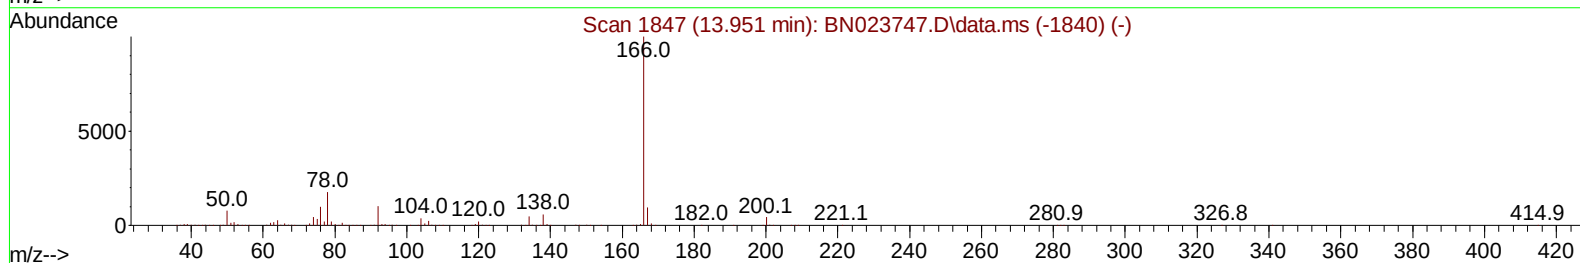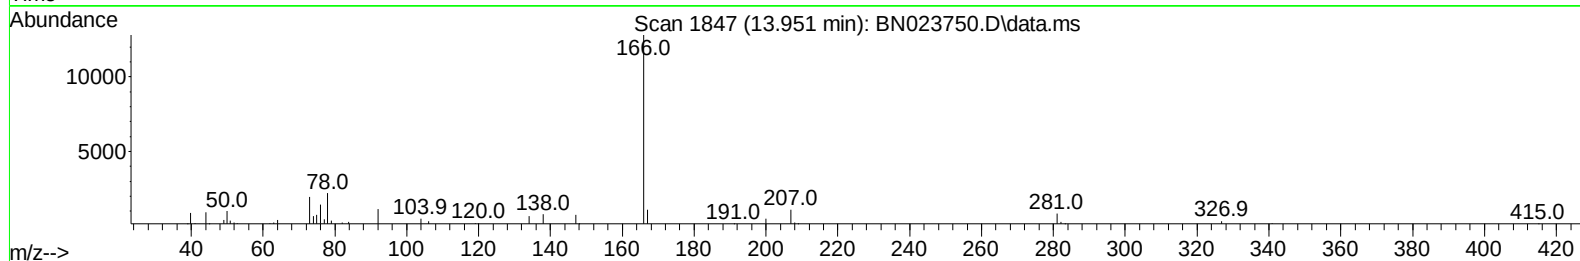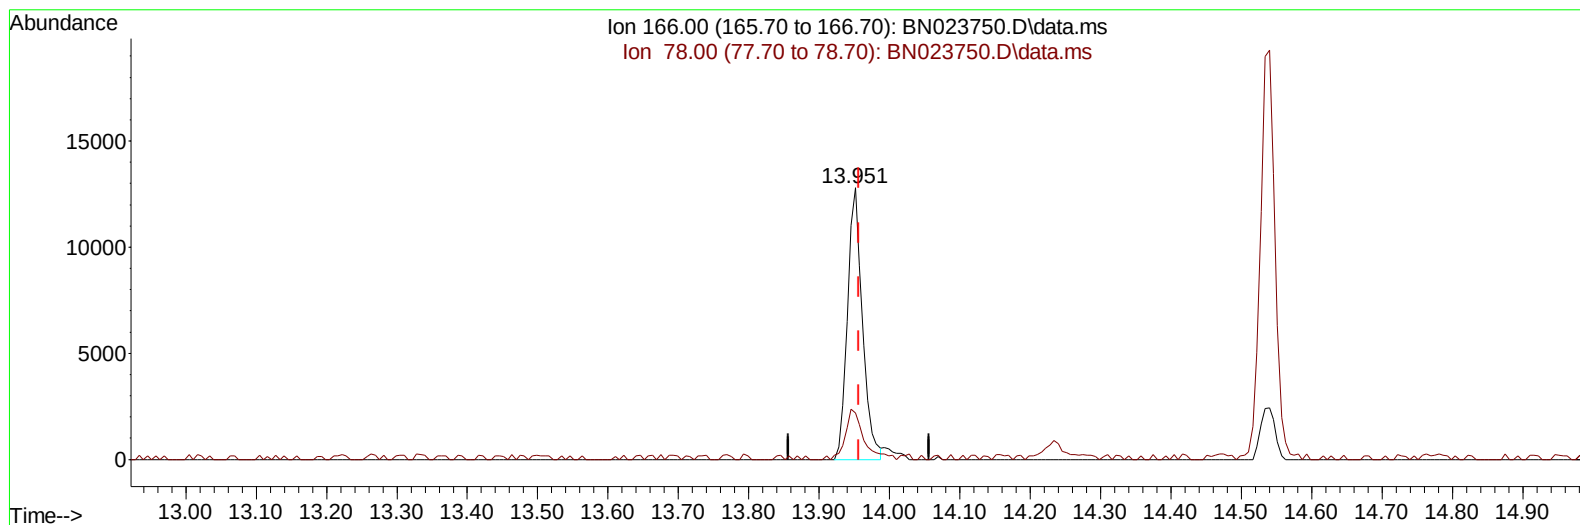

TIC: BN023750.D\data.ms

(46) Dimethylphthalate-d6 (S)

13.951min (-0.006) 0.55 ng/u1

response 18786

Ion	Exp%	Act%
166.00	100.00	100.00
78.00	16.80	17.20
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023750.D
 Acq On : 23 Jan 2023 13:32
 Operator : CG/JU
 Sample : 01146-14MEDL 30X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4462MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 23 23:59:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/24/2023
 Supervised By :mohammad ahmed 01/24/2023

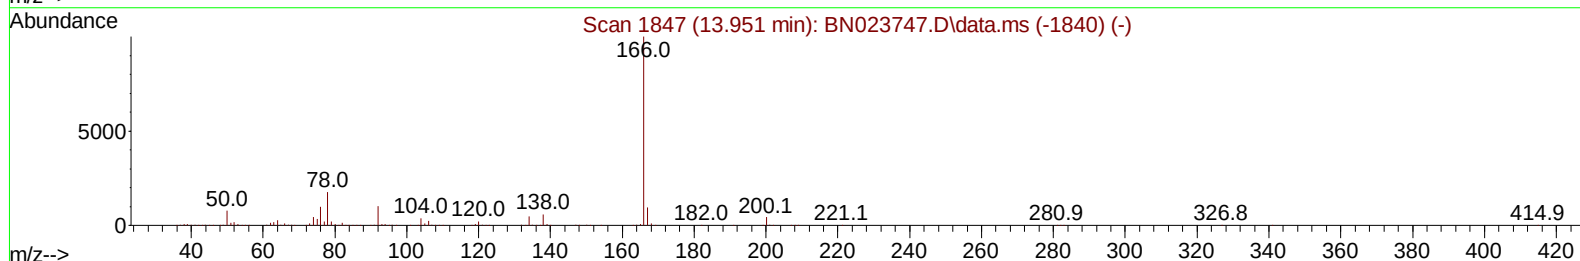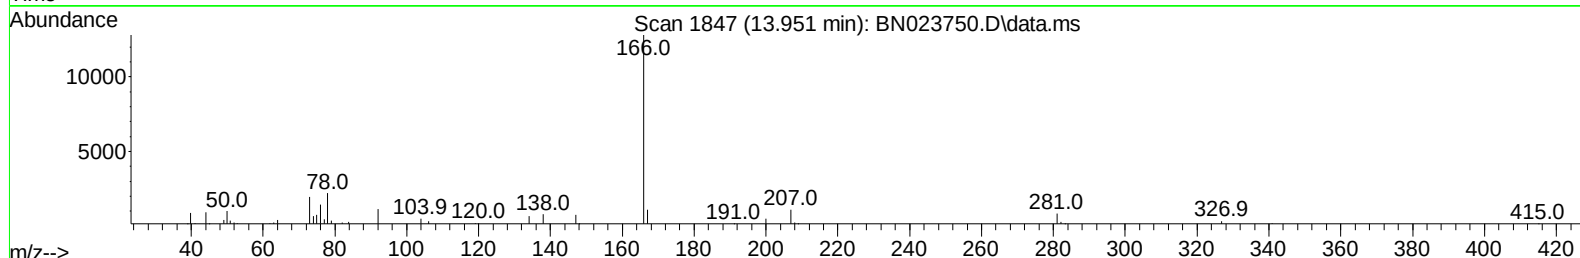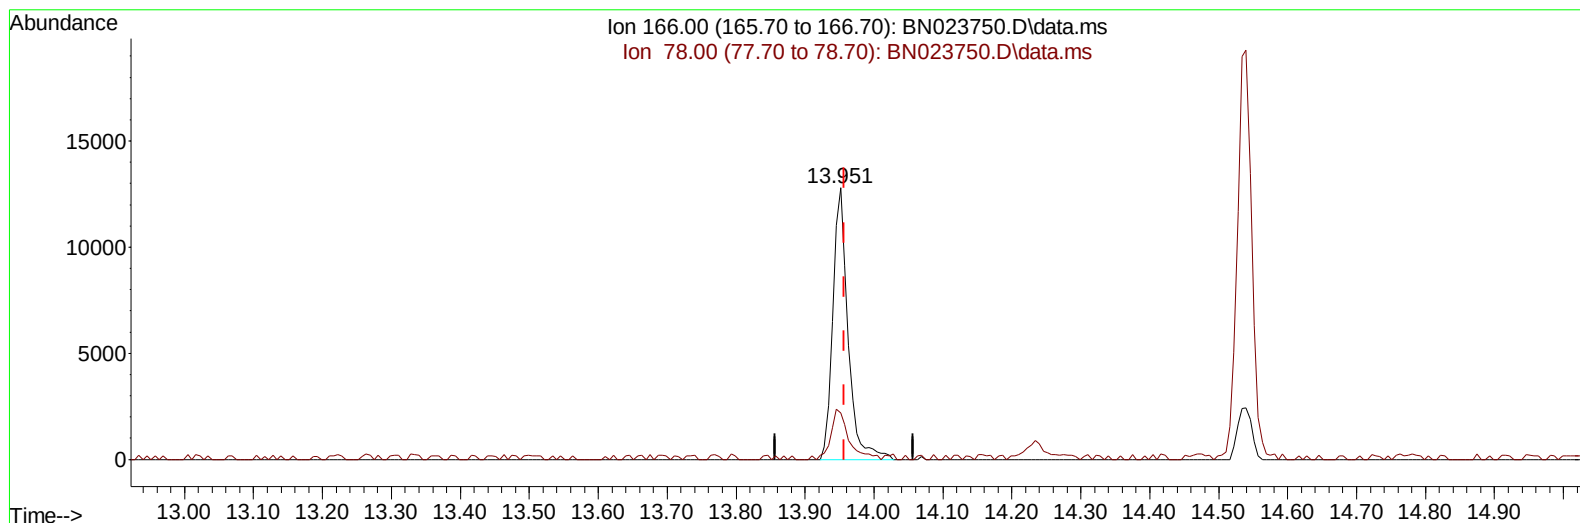

TIC: BN023750.D\data.ms

(46) Dimethylphthalate-d6 (S)

13.951min (-0.006) 0.57 ng/ul m

response 19554

Ion	Exp%	Act%
166.00	100.00	100.00
78.00	16.80	17.20
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023750.D
 Acq On : 23 Jan 2023 13:32
 Operator : CG/JU
 Sample : 01146-14MEDL 30X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4462MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 23 23:59:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/24/2023
 Supervised By :mohammad ahmed 01/24/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.887	152		200839	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136		798514	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164		457592	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188		931778	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240		843794	20.000	ng/ul	0.00
88) Perylene-d12	23.892	264		817913	20.000	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	0.000	96		0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	7.052	99		8023	0.451	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67		7383	0.676	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132		6848	0.502	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113		5285	0.372	ng/ul	0.00
21) Nitrobenzene-d5	9.058	128		2972	0.494	ng/ul	0.00
24) 2-Nitrophenol-d4	0.000	143		0d	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	10.322	165		4382m	0.360	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131		8444m	0.442	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166		19554m	0.574	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160		19078	0.506	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143		0d	0.000	ng/ul	
60) Fluorene-d10	15.528	176		17489	0.601	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200		0d	0.000	ng/ul	
73) Anthracene-d10	17.381	188		23313	0.559	ng/ul	0.00
81) Pyrene-d10	19.675	212		26579	0.551	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264		20160	0.498	ng/ul	-0.03
Target Compounds							
						Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.386	149		935975	27.312	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023750.D
Acq On : 23 Jan 2023 13:32
Operator : CG/JU
Sample : 01146-14MEDL 30X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4462MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 23 23:59:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/24/2023
Supervised By :mohammad ahmed 01/24/2023

