




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023769.D
 Acq On : 24 Jan 2023 10:10
 Operator : CG/JU
 Sample : 01216-01DL3 100X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH206DL3

Manual IntegrationsAPPROVED

Quant Time: Jan 24 23:55:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 24 23:52:16 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/25/2023
 Supervised By :Yogesh Patel 01/25/2023

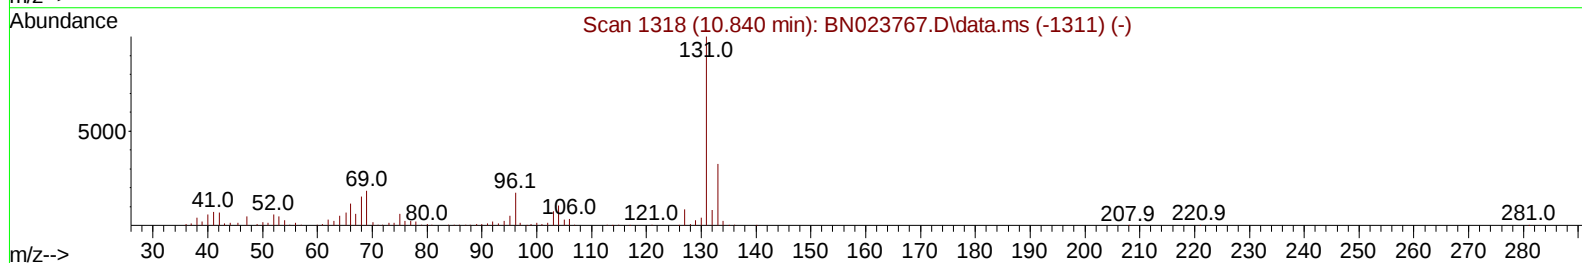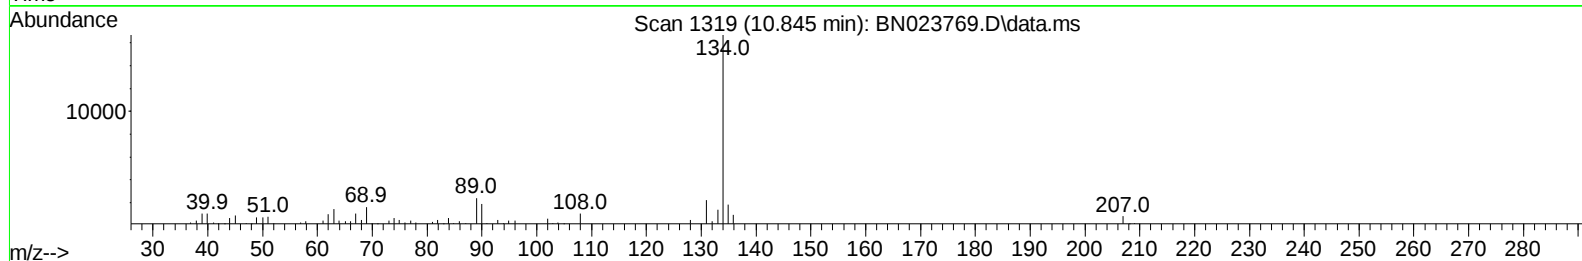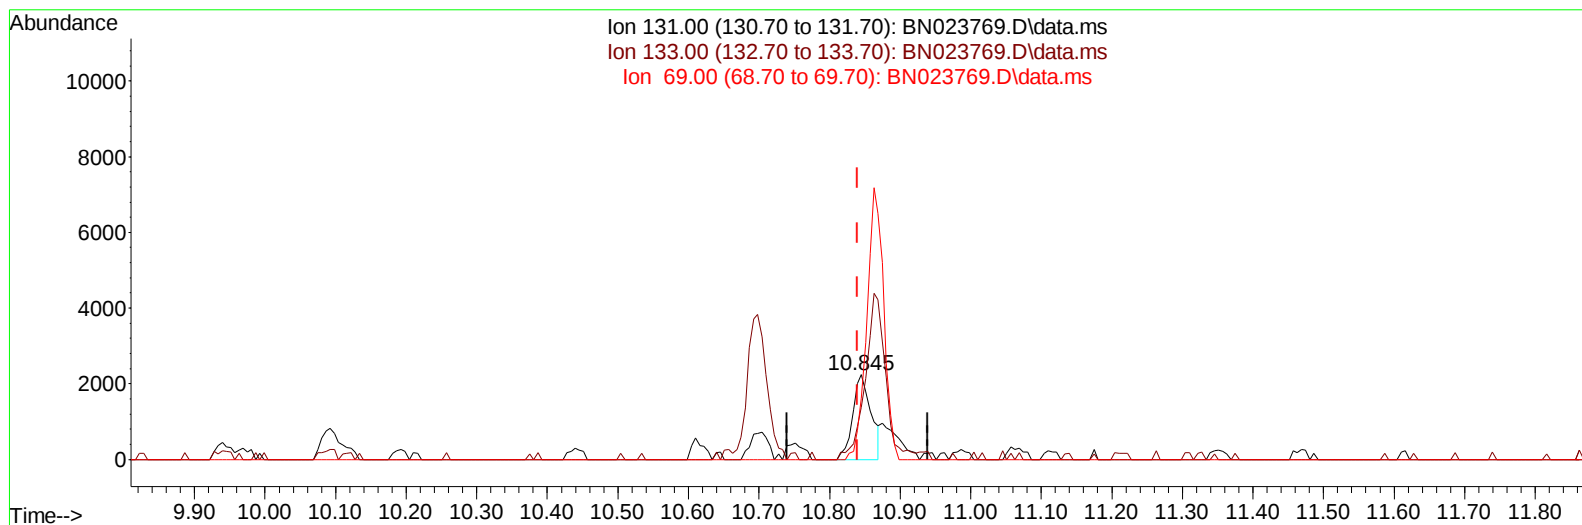

TIC: BN023769.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.845min (+ 0.005) 0.20 ng/ul

response 4072

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.40	61.40#
69.00	17.20	71.89#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023769.D
Acq On : 24 Jan 2023 10:10
Operator : CG/JU
Sample : 01216-01DL3 100X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH206DL3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/25/2023
Supervised By :Yogesh Patel 01/25/2023

Quant Time: Jan 24 23:55:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 24 23:52:16 2023
Response via : Initial Calibration

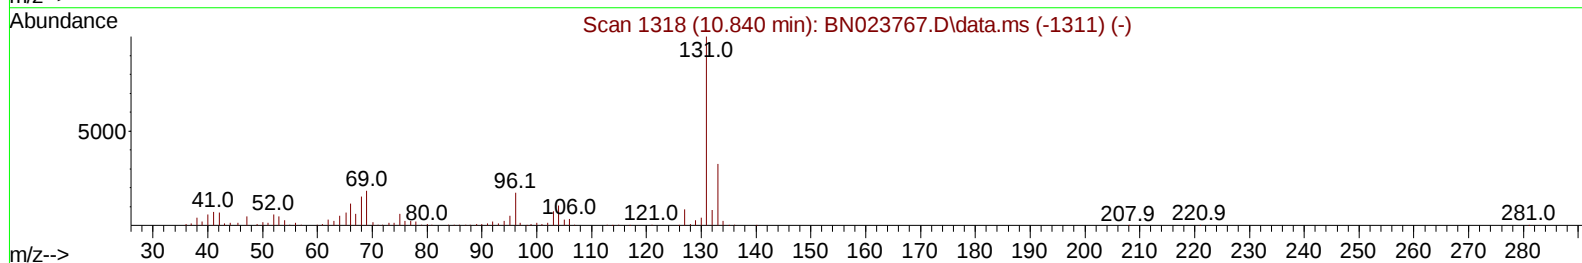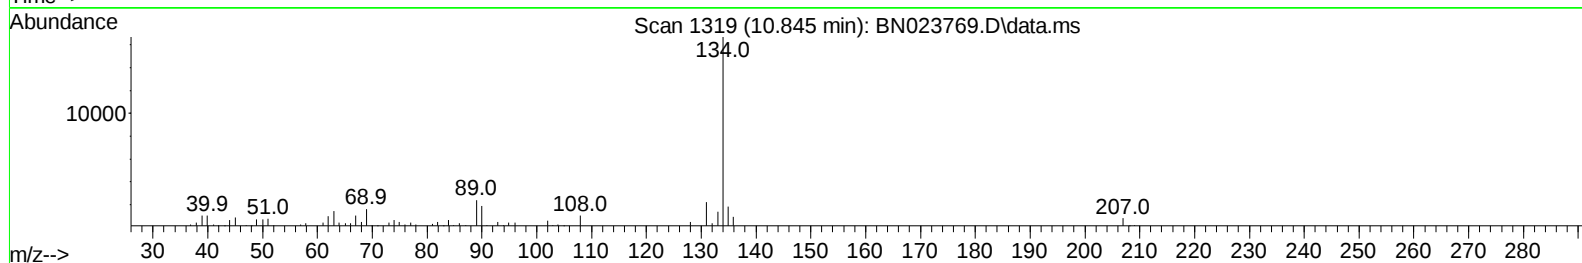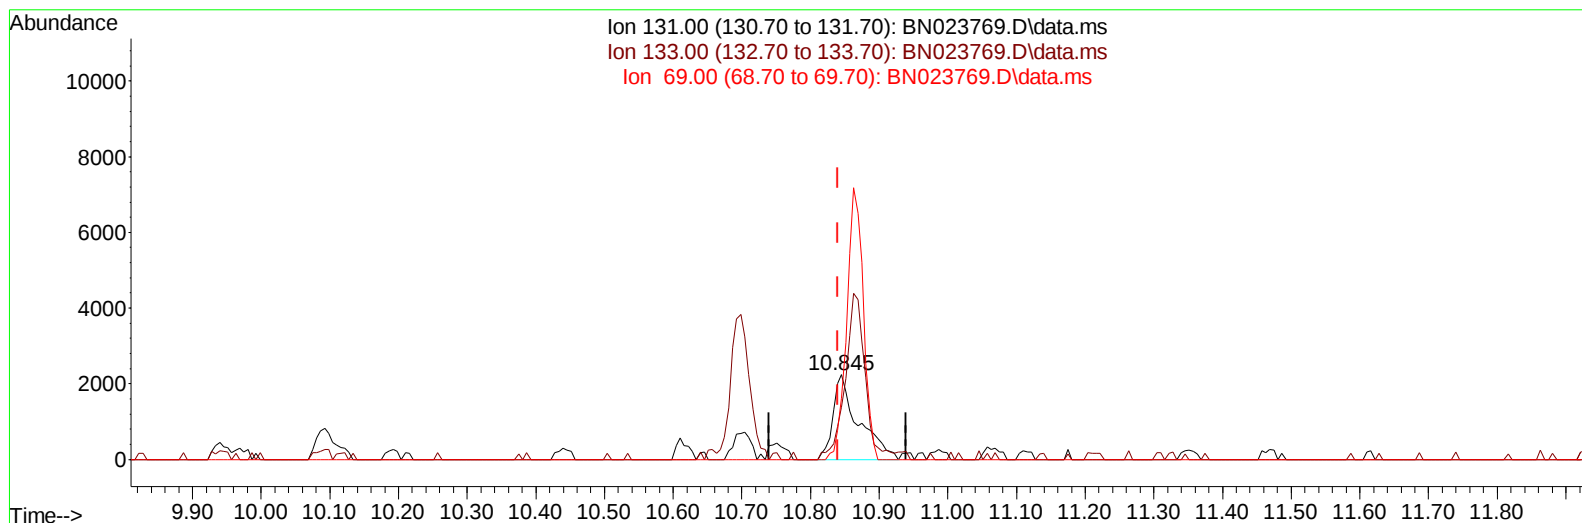

TIC: BN023769.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.845min (+ 0.005) 0.28 ng/ul m

response 5793

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.40	61.40#
69.00	17.20	71.89#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
 Data File : BN023769.D
 Acq On : 24 Jan 2023 10:10
 Operator : CG/JU
 Sample : 01216-01DL3 100X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH206DL3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/25/2023
 Supervised By :Yogesh Patel 01/25/2023

Quant Time: Jan 24 23:55:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 24 23:52:16 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.887	152		210879	20.000	ng/ul	0.00
20) Naphthalene-d8	10.698	136		863974	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.533	164		506570	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.280	188		1109773	20.000	ng/ul	0.00
79) Chrysene-d12	21.474	240		1077736	20.000	ng/ul	0.00
88) Perylene-d12	23.898	264		1026106	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	0.000	96		0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	7.051	99		884	0.047	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67		3943	0.344	ng/ul	0.00
11) 2-Chlorophenol-d4	7.416	132		2842	0.199	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113		1553	0.104	ng/ul	0.00
21) Nitrobenzene-d5	9.051	128		2138	0.328	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143		1590	0.231	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.316	165		2642	0.201	ng/ul	0.00
31) 4-Chloroaniline-d4	10.845	131		5793m	0.280	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166		11781	0.313	ng/ul	0.00
49) Acenaphthylene-d8	14.227	160		12260	0.294	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143		0	0.000	ng/ul	
60) Fluorene-d10	15.527	176		11929	0.370	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200		0d	0.000	ng/ul	
73) Anthracene-d10	17.380	188		16849	0.339	ng/ul	0.00
81) Pyrene-d10	19.674	212		20446	0.332	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264		15446	0.304	ng/ul	-0.01
Target Compounds							
						Qvalue	
30) Naphthalene	10.745	128		2476823	53.328	ng/ul	98
36) 2-Methylnaphthalene	12.357	142		71546	2.311	ng/ul	96
37) 1-Methylnaphthalene	12.575	142		44392	1.403	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012323\
Data File : BN023769.D
Acq On : 24 Jan 2023 10:10
Operator : CG/JU
Sample : 01216-01DL3 100X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH206DL3

Manual IntegrationsAPPROVED

Quant Time: Jan 24 23:55:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 24 23:52:16 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/25/2023
Supervised By :Yogesh Patel 01/25/2023

